

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110822\
 Data File : PD072849.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Nov 2022 13:19
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA2074

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 15:41:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110822CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 08 15:38:33 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.700	3.461	23519672	464.0E6	9.917	10.455
27)	SA Decachlor...	7.829	8.912	45863631	218.4E6	19.731	20.075
Target Compounds							
2)	A alpha-BHC	3.204	3.926	33578097	598.1E6	9.270	10.365
3)	MA gamma-BHC...	3.534	4.259	31269176	478.2E6	9.385	10.507
4)	MA Heptachlor	3.866	4.825	31653056	331.6E6	9.355	10.564
9)	A Endosulfan I	5.018	5.980	27388312	204.3E6	9.688	10.279
13)	MA Dieldrin	5.284	6.257	57452927	412.1E6	18.446	20.328
14)	MA Endrin	5.561	6.489	51620373	343.6E6	18.569	20.252
16)	A 4,4'-DDD	5.708	6.623	45388105	304.7E6	18.401	20.218
17)	MA 4,4'-DDT	5.957	6.930	42679988	289.3E6	17.642	19.770
20)	A Methoxychlor	6.540	7.410	126.3E6	652.2E6	93.481	99.351

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110822\
Data File : PD072849.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Nov 2022 13:19
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 15:41:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110822CLP.M
Quant Title : GC Extractables
QLast Update : Tue Nov 08 15:38:33 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

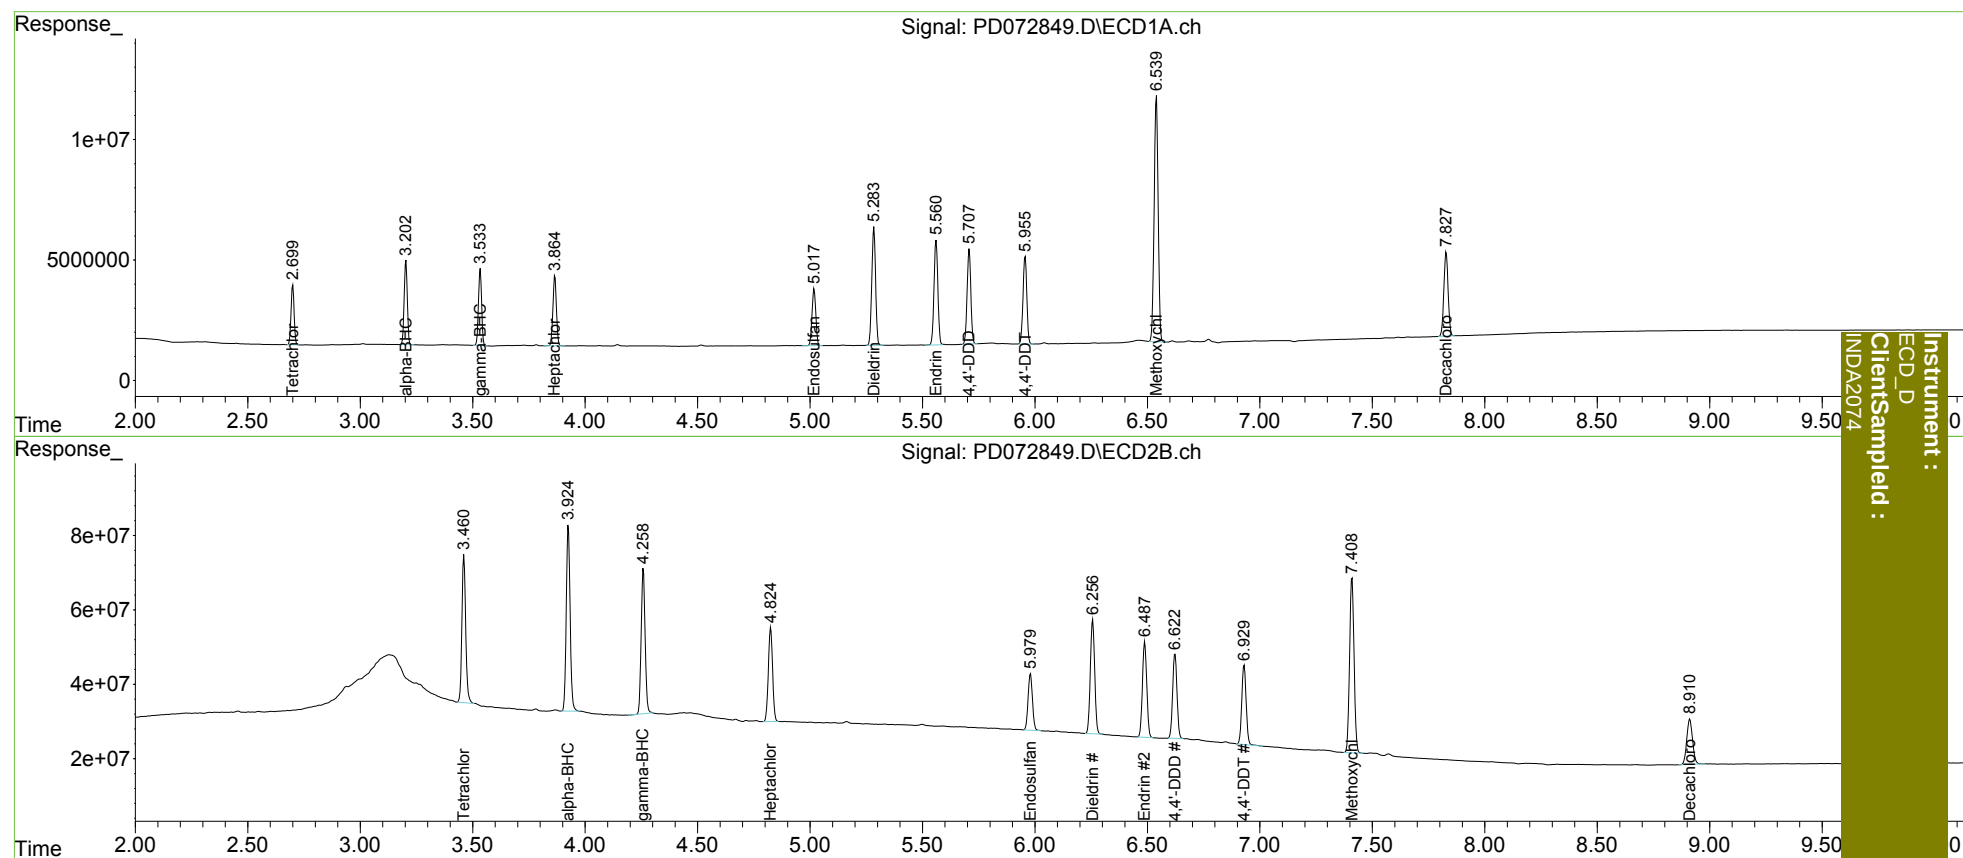

Instrument :
ECD_D
ClientSampled :
INDA2074