

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110822\
 Data File : PD072855.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Nov 2022 14:39
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA5080

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 15:42:38 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110822CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 08 15:38:33 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.700	3.462	178.6E6	2961.0E6	75.324	66.719
27)	SA Decachlor...	7.830	8.912	333.0E6	1498.6E6	143.244	137.747
Target Compounds							
2)	A alpha-BHC	3.204	3.926	300.6E6	3965.5E6	82.993	68.727
3)	MA gamma-BHC...	3.534	4.260	271.4E6	3061.4E6	81.452	67.269
4)	MA Heptachlor	3.867	4.825	269.1E6	2057.4E6	79.542	65.537
9)	A Endosulfan I	5.019	5.981	217.5E6	1332.8E6	76.930	67.044
13)	MA Dieldrin	5.285	6.257	496.0E6	2840.0E6	159.263	140.095
14)	MA Endrin	5.562	6.489	439.8E6	2377.9E6	158.192	140.158
16)	A 4,4'-DDD	5.709	6.623	389.7E6	2112.9E6	157.990	140.184
17)	MA 4,4'-DDT	5.957	6.931	399.5E6	2121.6E6	165.152	144.979
20)	A Methoxychlor	6.541	7.411	991.5E6	4538.4E6	733.970	691.395

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110822\
Data File : PD072855.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Nov 2022 14:39
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 15:42:38 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110822CLP.M
Quant Title : GC Extractables
QLast Update : Tue Nov 08 15:38:33 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

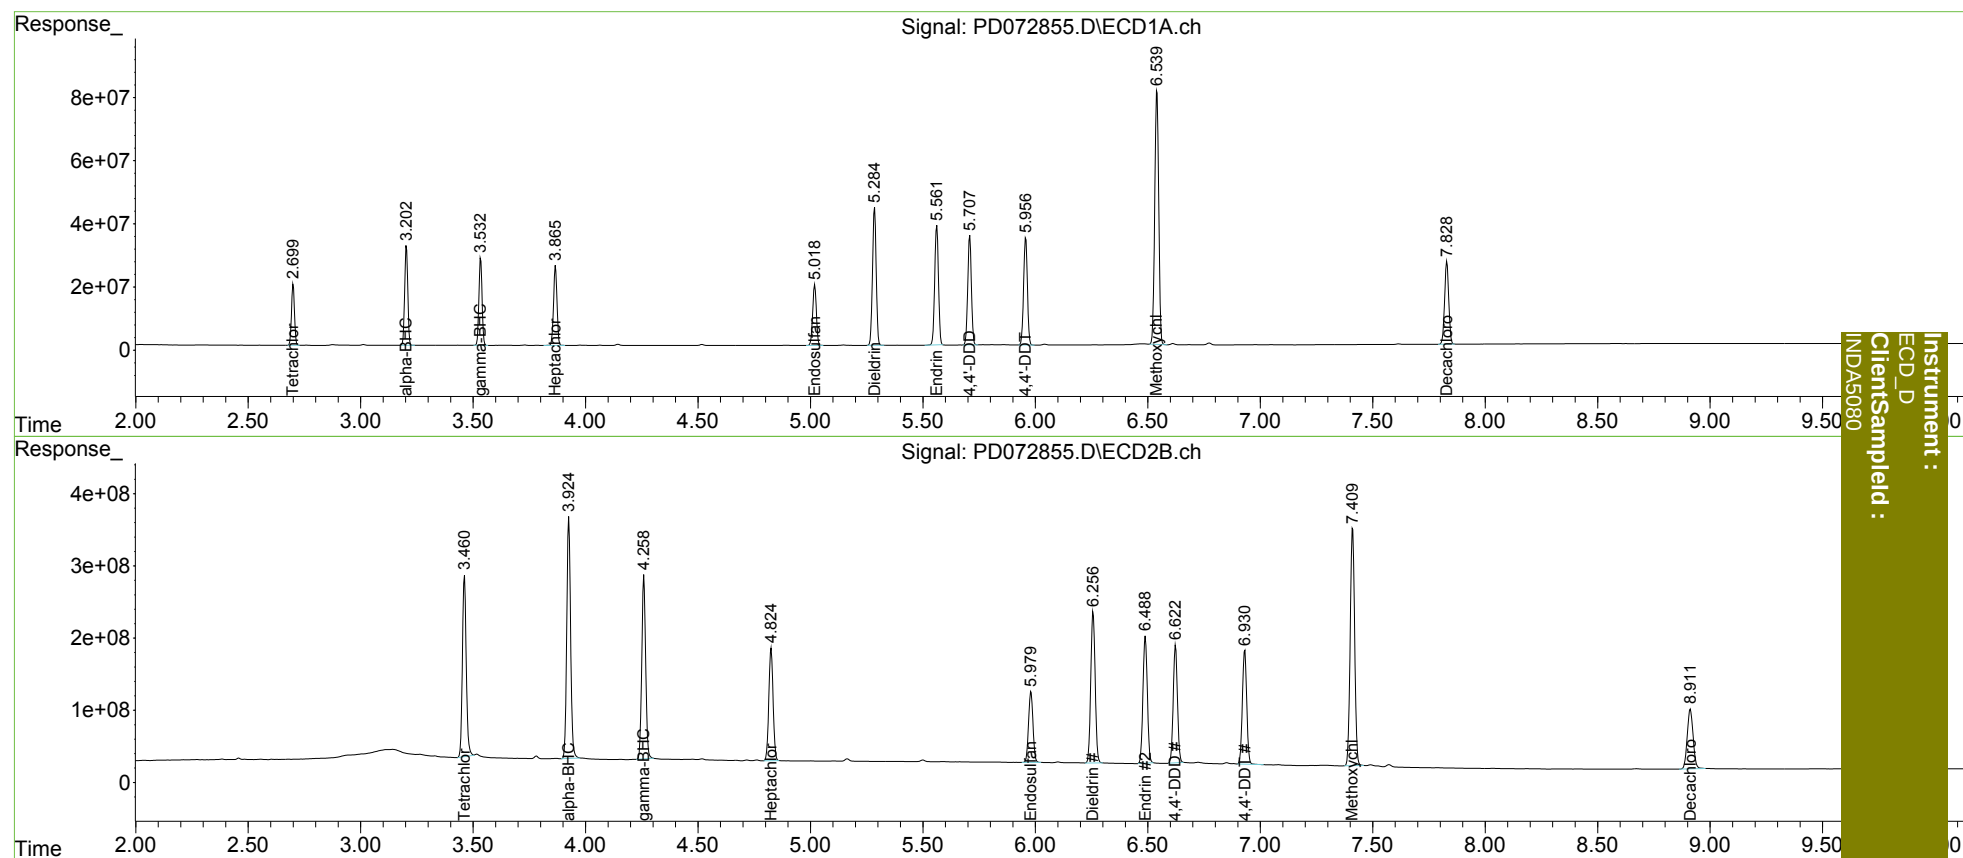

Instrument :
ECD_D
ClientSampled :
INDA5080