

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110822\
 Data File : PD072865.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Nov 2022 18:48
 Operator : AR\AJ
 Sample : N5407-14MS
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW4Z2MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 02:11:29 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110822CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 08 16:13:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.701	3.463	49491394	1130.7E6	21.206	25.938
2)	SA Decachlor...	7.830	8.913	85243262	410.9E6	37.528	39.039
Target Compounds							
2)	A alpha-BHC	3.204	3.926	170.7E6	2319.6E6	48.373	40.992
3)	MA gamma-BHC...	3.535	4.260	167.4E6	1940.6E6	51.494	43.352
4)	MA Heptachlor	3.867	4.826	180.2E6	1395.0E6	54.840	45.310
5)	MB Aldrin	4.146	5.164	179.8E6	1221.5E6	55.558	46.564
6)	B beta-BHC	3.836	4.474	75415659	797.9E6	49.449	45.117
7)	B delta-BHC	4.065	4.718	16357563	197.5E6	4.703	5.509
8)	B Heptachlo...	4.650	5.597	164.6E6	1081.9E6	54.946	48.879
9)	A Endosulfan I	5.019	5.981	151.2E6	960.6E6	54.624	49.786
10)	B trans-Chl...	4.899	5.850	167.9E6	1020.5E6	56.775	49.444
11)	B cis-Chlor...	4.962	5.925	161.4E6	1001.1E6	53.426	48.020
12)	B 4,4'-DDE	5.150	6.099	335.2E6	1966.2E6	116.176	102.757
13)	MA Dieldrin	5.285	6.258	350.8E6	2056.0E6	117.007	103.657
14)	MA Endrin	5.562	6.489	301.7E6	1670.8E6	112.868	101.172
15)	B Endosulfa...	5.860	6.719	286.4E6	1633.9E6	110.303	102.597
16)	A 4,4'-DDD	5.709	6.623	261.8E6	1483.9E6	110.694	101.166
17)	MA 4,4'-DDT	5.957	6.931	267.0E6	1523.4E6	115.532	107.053
18)	B Endrin al...	6.042	6.850	203.5E6	1151.3E6	97.513	92.290
19)	B Endosulfa...	6.265	7.083	180.0E6	990.8E6	73.945	72.199
20)	A Methoxychlor	6.541	7.411	716.4E6	3432.1E6	557.793	541.750
21)	B Endrin ke...	6.776	7.572	321.1E6	1608.3E6	113.600	107.034

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110822\
Data File : PD072865.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Nov 2022 18:48
Operator : AR\AJ
Sample : N5407-14MS
Misc :
ALS Vial : 26 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 02:11:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110822CLP.M
Quant Title : GC Extractables
QLast Update : Tue Nov 08 16:13:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

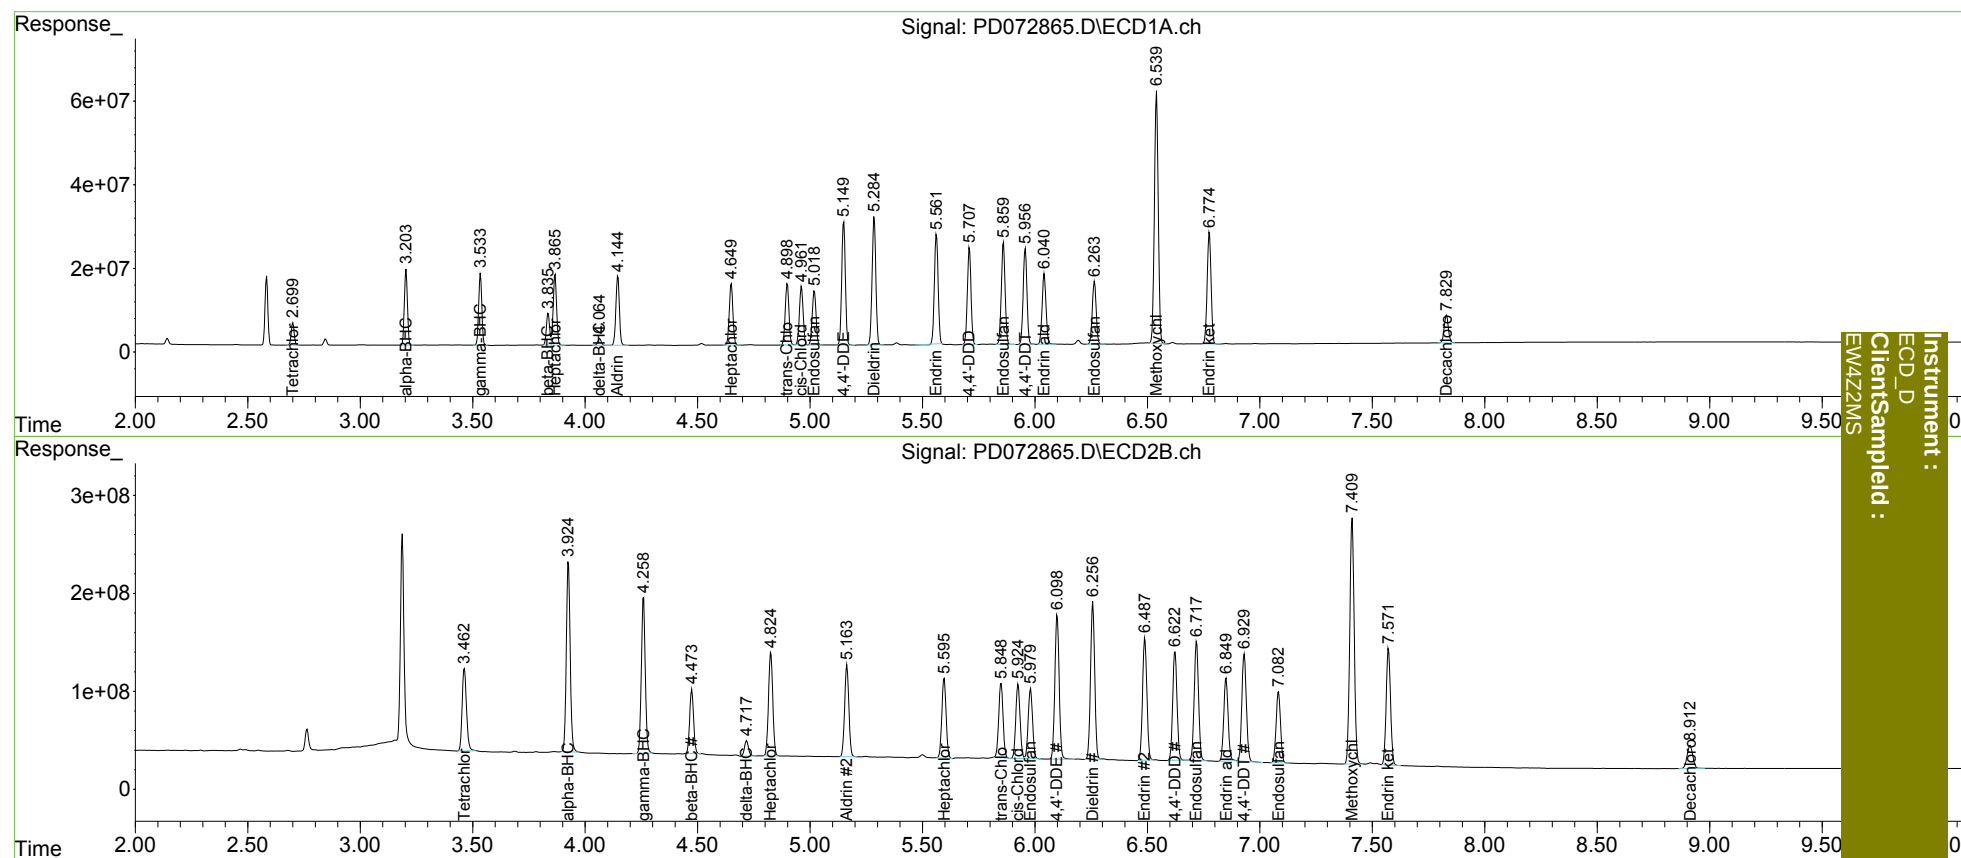

Instrument :
ECD_D
ClientSampled :
EW4ZMS