

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110822\
 Data File : PD072866.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Nov 2022 19:02
 Operator : AR\AJ
 Sample : N5407-15MSD
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW4Z2MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 02:11:49 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110822CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 08 16:13:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.701	3.464	44788750	1040.7E6	19.191	23.875
2)	SA Decachlor...	7.830	8.912	81629598	391.5E6	35.937	37.195
Target Compounds							
2)	A alpha-BHC	3.204	3.926	164.7E6	2261.0E6	46.678	39.957
3)	MA gamma-BHC...	3.535	4.260	162.5E6	1897.4E6	49.974	42.387
4)	MA Heptachlor	3.867	4.826	175.3E6	1370.9E6	53.347	44.525
5)	MB Aldrin	4.146	5.164	176.1E6	1208.8E6	54.426	46.079
6)	B beta-BHC	3.836	4.475	73803171	790.3E6	48.392	44.688
7)	B delta-BHC	4.065	4.719	15296353	182.9E6	4.398	5.104
8)	B Heptachlo...	4.651	5.596	160.2E6	1053.7E6	53.474	47.601
9)	A Endosulfan I	5.019	5.981	147.8E6	941.4E6	53.421	48.787
10)	B trans-Chl...	4.899	5.850	164.1E6	998.8E6	55.492	48.394
11)	B cis-Chlor...	4.962	5.925	158.0E6	981.0E6	52.294	47.056
12)	B 4,4'-DDE	5.151	6.099	326.7E6	1921.4E6	113.239	100.419
13)	MA Dieldrin	5.285	6.257	340.6E6	2007.1E6	113.613	101.190
14)	MA Endrin	5.562	6.490	296.7E6	1641.7E6	110.978	99.410
15)	B Endosulfa...	5.860	6.719	279.4E6	1595.2E6	107.611	100.169
16)	A 4,4'-DDD	5.708	6.623	255.6E6	1449.9E6	108.068	98.846
17)	MA 4,4'-DDT	5.957	6.931	260.9E6	1499.9E6	112.867	105.401
18)	B Endrin al...	6.042	6.850	199.3E6	1139.4E6	95.512	91.339
19)	B Endosulfa...	6.265	7.083	175.6E6	973.2E6	72.162	70.921
20)	A Methoxychlor	6.540	7.410	701.9E6	3351.2E6	546.507	528.980
21)	B Endrin ke...	6.775	7.572	314.6E6	1583.6E6	111.300	105.392

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110822\
Data File : PD072866.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Nov 2022 19:02
Operator : AR\AJ
Sample : N5407-15MSD
Misc :
ALS Vial : 27 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 02:11:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110822CLP.M
Quant Title : GC Extractables
QLast Update : Tue Nov 08 16:13:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

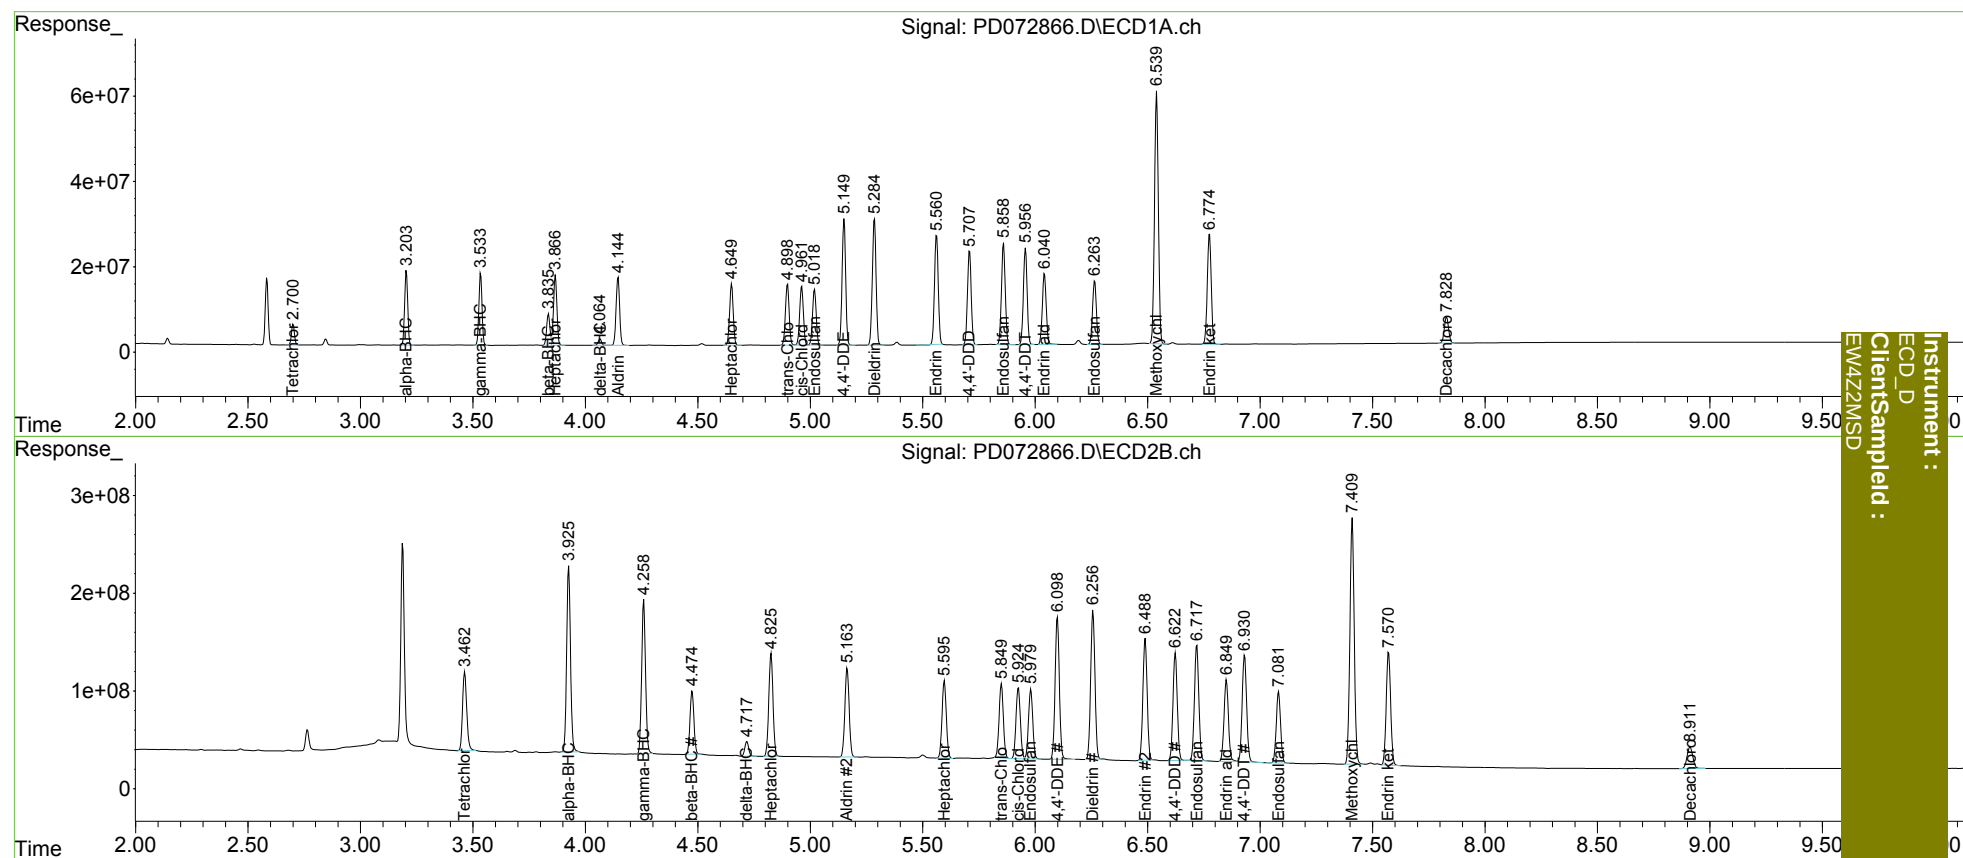

Instrument :
ECD_D
Client Sampled :
EW42MSD