

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110823\
 Data File : PD079494.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2023 15:51
 Operator : AR\AJ
 Sample : PIBLK070
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 20:36:14 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 04 07:14:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	2.803	34974326	56062449	23.949	24.510
27)	SA Decachlor...	9.118	7.949	72205923	107.7E6	40.690	45.123
Target Compounds							
2)	A alpha-BHC	0.000	3.294	0	133049	N.D.	<MDL
3)	MA gamma-BHC...	0.000	3.656	0	171342	N.D.	<MDL
4)	MA Heptachlor	0.000	3.942f	0	681377	N.D.	0.204
5)	MB Aldrin	0.000	4.266	0	944875	N.D.	0.290
6)	B beta-BHC	0.000	3.942	0	681377	N.D.	0.416
7)	B delta-BHC	4.794	4.186	4597983	648708	1.845	0.182 #
8)	B Heptachlo...	0.000	4.789	0	698724	N.D.	0.226
10)	B trans-Chl...	6.008	0.000	1309343	0	0.615	N.D. #
11)	B cis-Chlor...	6.008f	0.000	1309343	0	0.601	N.D. #
13)	MA Dieldrin	0.000	5.375	0	200677	N.D.	<MDL
14)	MA Endrin	0.000	5.688	0	54304	N.D.	<MDL
15)	B Endosulfa...	0.000	5.996	0	179437	N.D.	<MDL
18)	B Endrin al...	0.000	6.149	0	235247	N.D.	0.116
19)	B Endosulfa...	0.000	6.371	0	34561	N.D.	<MDL
23)	Toxaphene-2	0.000	5.375	0	200677	N.D.	11.942
25)	Toxaphene-4	0.000	6.795f	0	3608	N.D.	<MDL


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110823\
Data File : PD079494.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2023 15:51
Operator : AR\AJ
Sample : PIBLK070
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 20:36:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 07:14:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

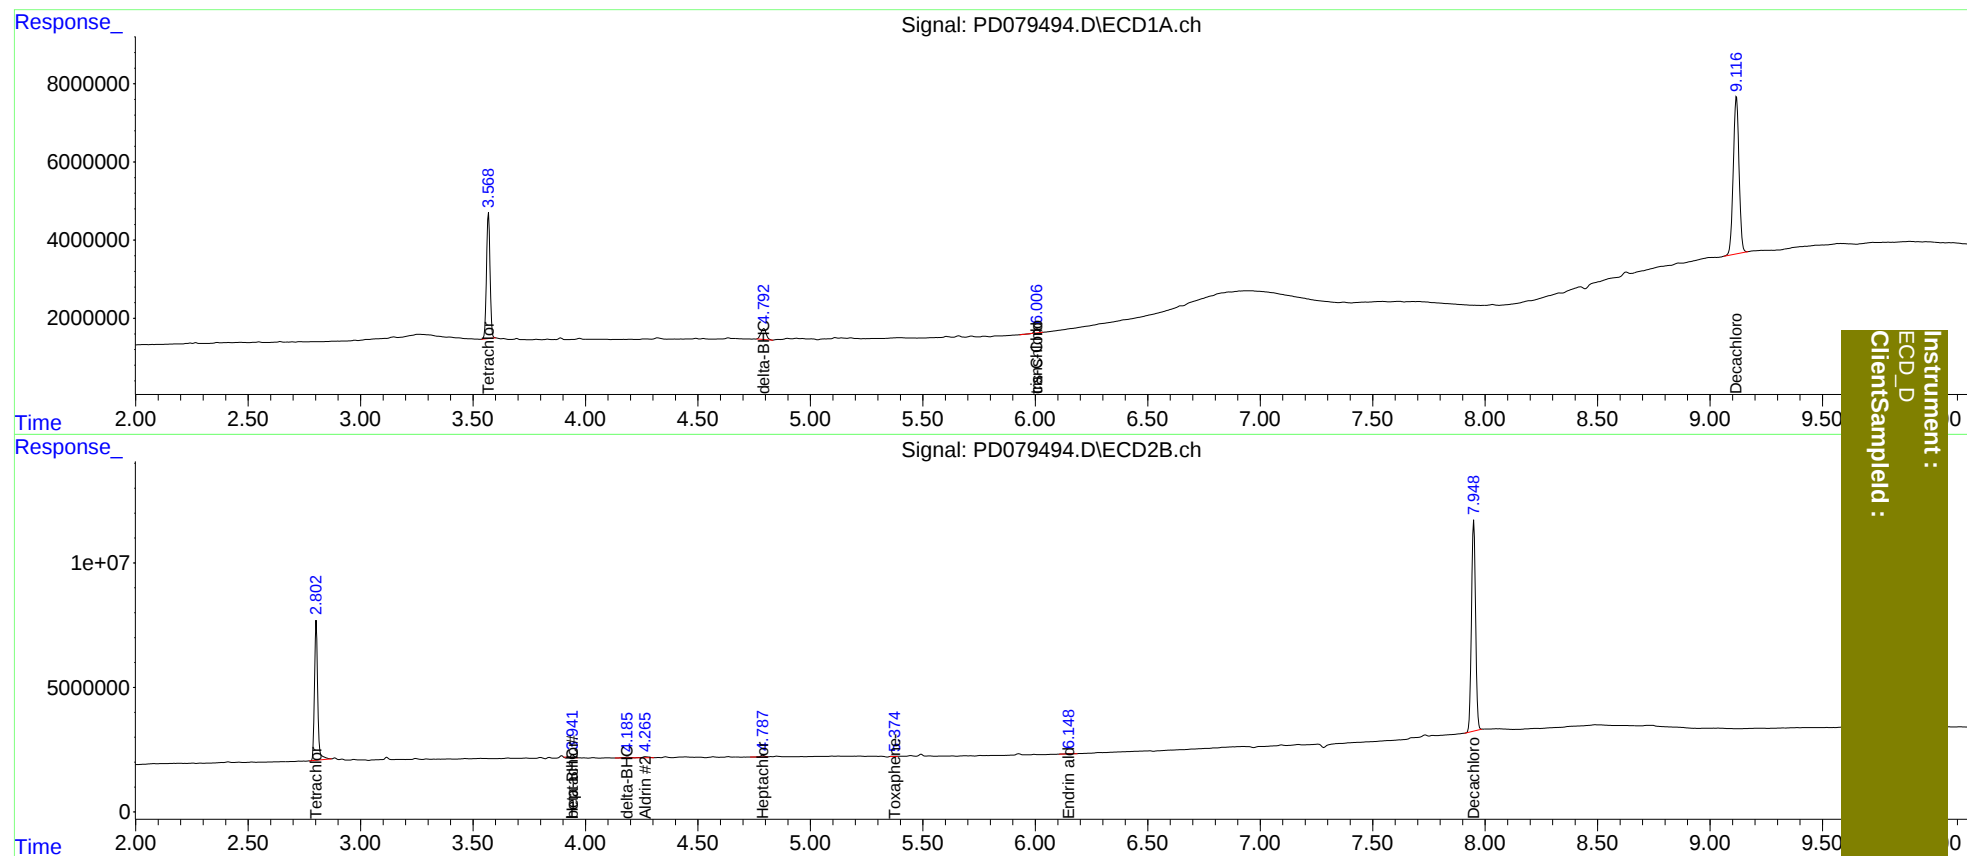


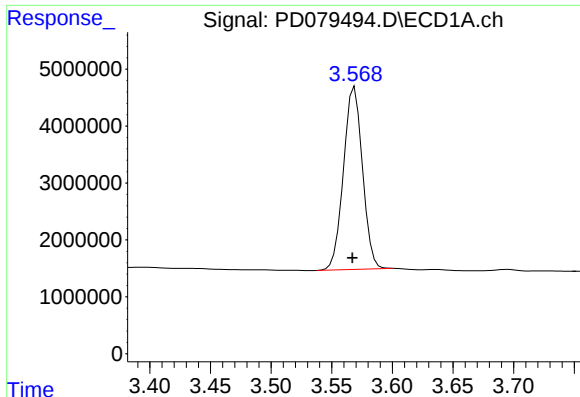

#1 Tetrachloro-m-xylene


R.T.: 3.569 min
Delta R.T.: 0.002 min
Response: 34974326
Conc: 23.95 ng/ml

Instrument :
ECD_D
ClientSampleId :

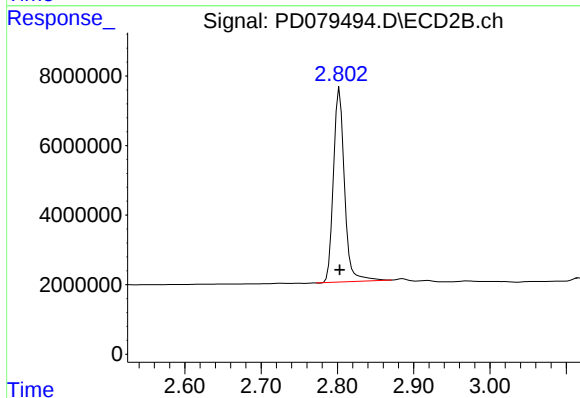


#1 Tetrachloro-m-xylene

R.T.: 2.803 min
Delta R.T.: 0.000 min
Response: 56062449
Conc: 24.51 ng/ml

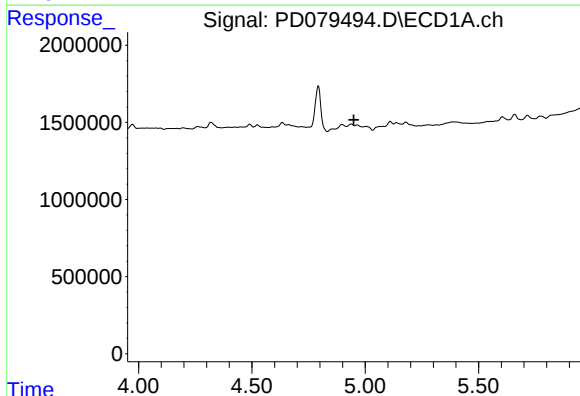


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.950 min
Response: 0
Conc: N.D.

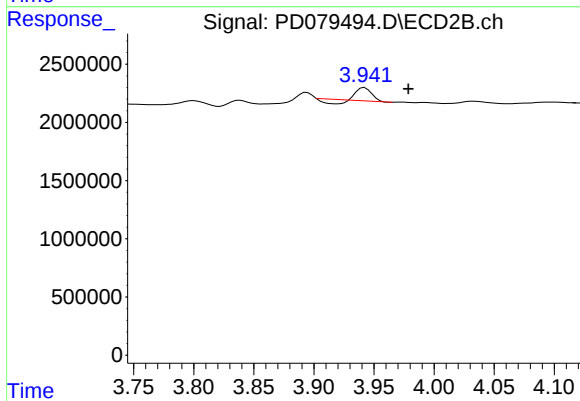

#4 Heptachlor


R.T.: 3.942 min
Delta R.T.: -0.036 min
Response: 681377
Conc: 0.20 ng/ml

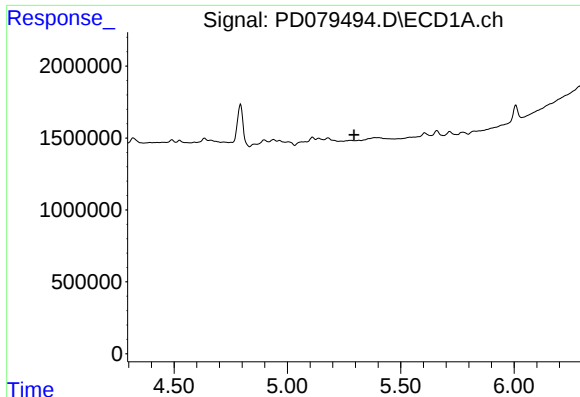

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.294 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

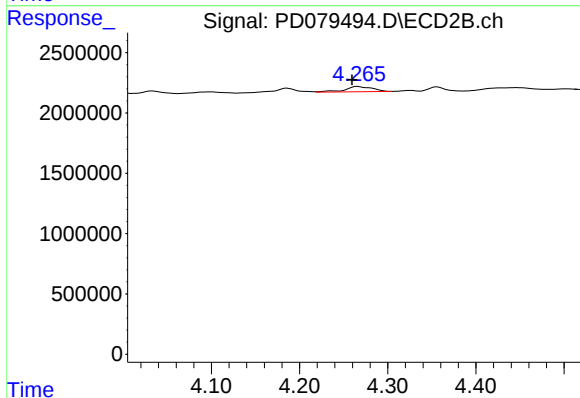


#5 Aldrin

R.T.: 4.266 min
Delta R.T.: 0.006 min
Response: 944875
Conc: 0.29 ng/ml

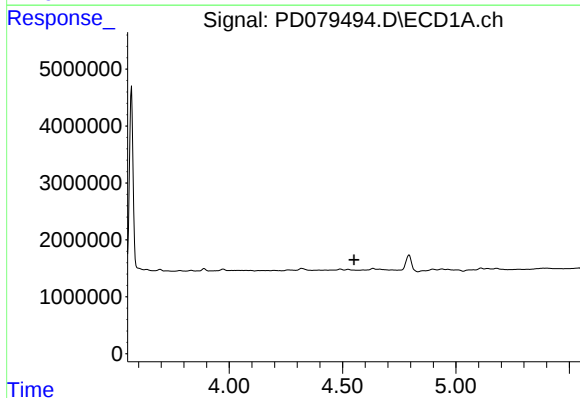


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.551 min
Response: 0
Conc: N.D.

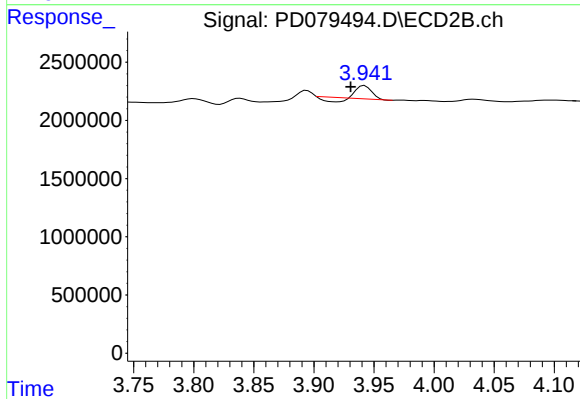

#6 beta-BHC


R.T.: 3.942 min
Delta R.T.: 0.012 min
Response: 681377
Conc: 0.42 ng/ml

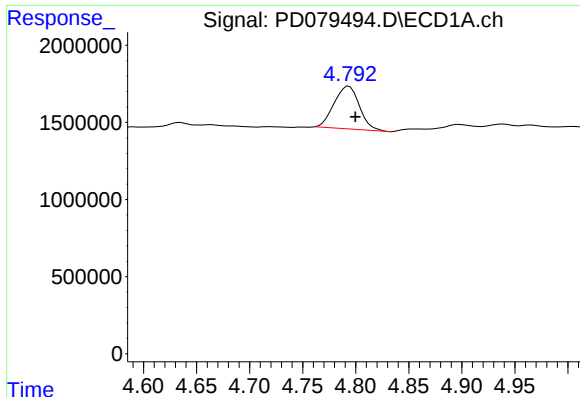

#7 delta-BHC


R.T.: 4.794 min
Delta R.T.: -0.006 min
Response: 4597983
Conc: 1.85 ng/ml

Instrument :
ECD_D
ClientSampleId :

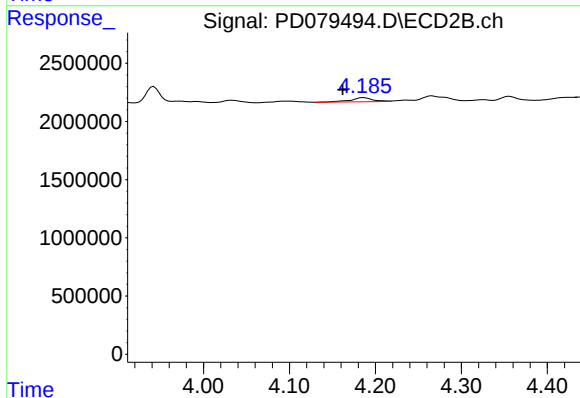


#7 delta-BHC

R.T.: 4.186 min
Delta R.T.: 0.024 min
Response: 648708
Conc: 0.18 ng/ml

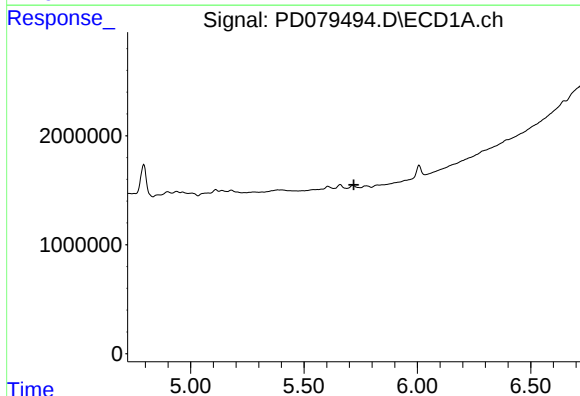


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.720 min
Response: 0
Conc: N.D.

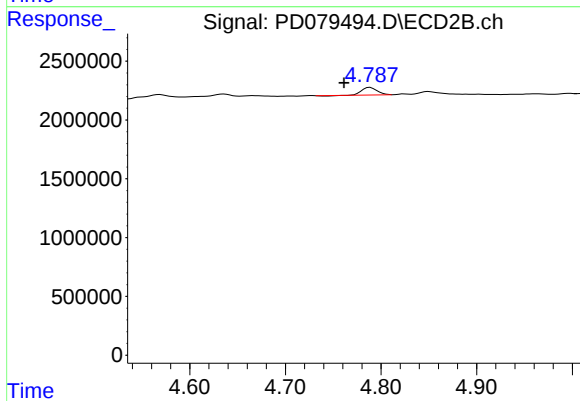

#8 Heptachlor epoxide


R.T.: 4.789 min
Delta R.T.: 0.027 min
Response: 698724
Conc: 0.23 ng/ml

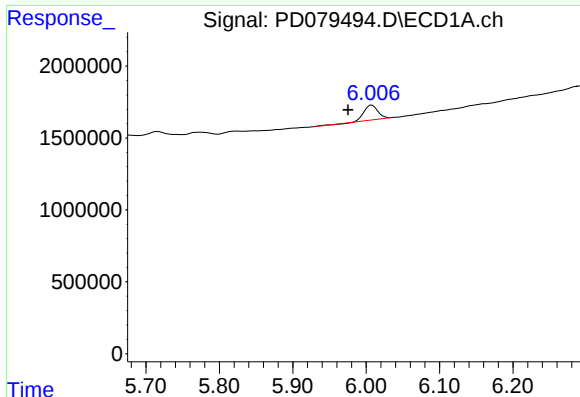

#10 trans-Chlordane


R.T.: 6.008 min
Delta R.T.: 0.032 min
Response: 1309343
Conc: 0.62 ng/ml

Instrument :
ECD_D
ClientSampleId :

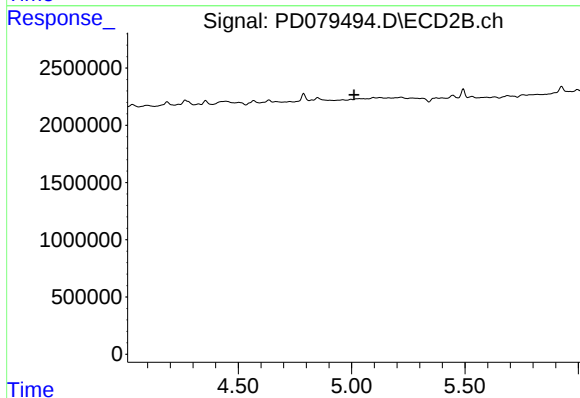


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.011 min
Response: 0
Conc: N.D.

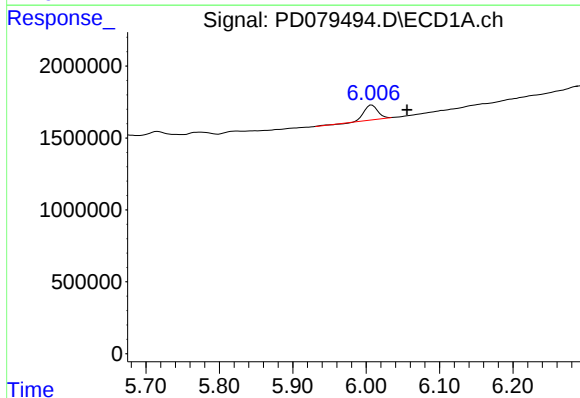


#11 cis-Chlordane

R.T.: 6.008 min
Delta R.T.: -0.048 min
Response: 1309343
Conc: 0.60 ng/ml

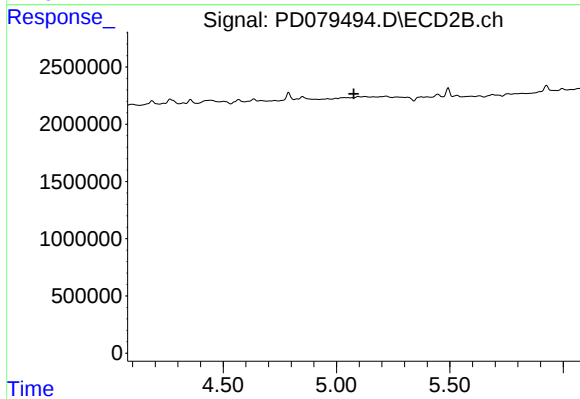

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.076 min
Response: 0
Conc: N.D.

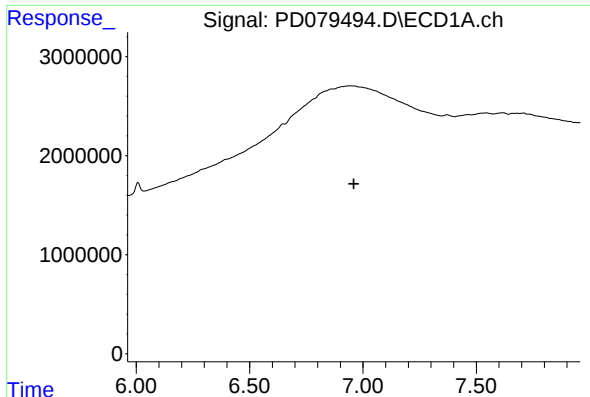

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.959 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

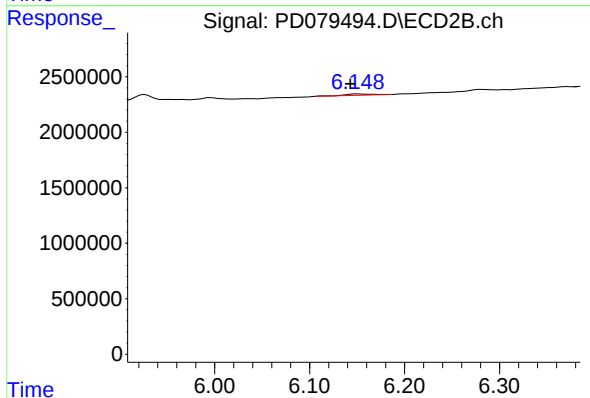


#18 Endrin aldehyde

R.T.: 6.149 min
Delta R.T.: 0.006 min
Response: 235247
Conc: 0.12 ng/ml

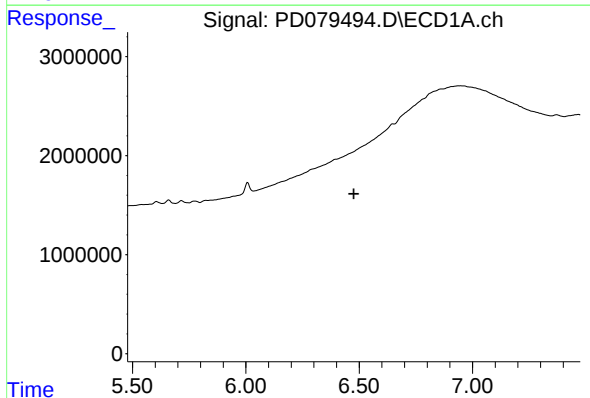


#23 Toxaphene-2

R.T.: 0.000 min
Exp R.T.: 6.477 min
Response: 0
Conc: N.D.

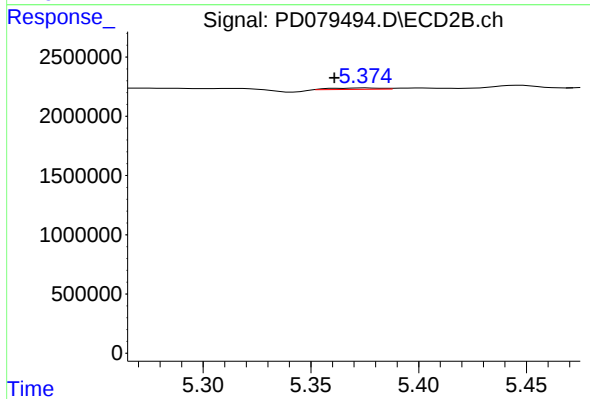

#23 Toxaphene-2


R.T.: 5.375 min
Delta R.T.: 0.014 min
Response: 200677
Conc: 11.94 ng/ml

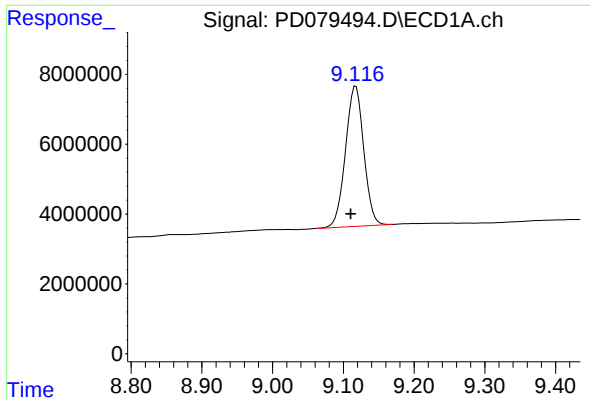

#27 Decachlorobiphenyl

R.T.: 9.118 min
Delta R.T.: 0.007 min
Response: 72205923
Conc: 40.69 ng/ml

Instrument :
ECD_D
ClientSampleId :

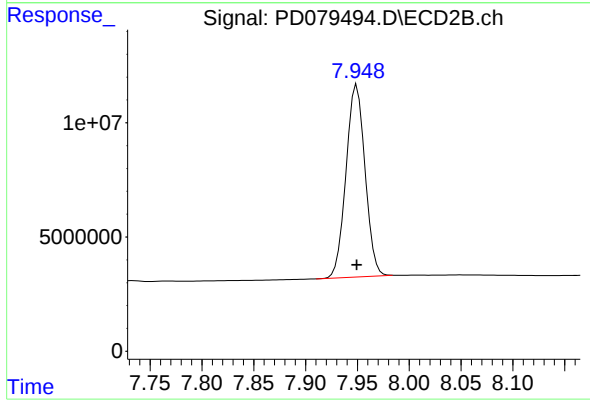

#27 Decachlorobiphenyl

R.T.: 7.949 min
Delta R.T.: 0.000 min
Response: 107730828
Conc: 45.12 ng/ml