

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110823\
 Data File : PD079497.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2023 17:30
 Operator : AR\AJ
 Sample : SFAMPESTSPIKE
 Misc : 50/100PPB
 ALS Vial : 100 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SFAMPESTSPIKE

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/07/2023
 Supervised By :Ankita Jodhani 11/07/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 17:46:15 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 04 07:14:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

11/07/2023
 Supervised By :Ankita
 Jodhani

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

11/07/2023

System Monitoring Compounds


Target Compounds						
2) A	alpha-BHC	4.031	3.305	125.4E6	184.7E6	50.622
3) MA	gamma-BHC...	4.365	3.634	112.5E6	165.0E6	47.620
4) MA	Heptachlor	4.958	3.977	120.1E6	164.1E6	47.956
5) MB	Aldrin	5.302	4.258	117.5E6	163.0E6	50.119
6) B	beta-BHC	4.558	3.930	47868352	69859784	44.086
7) B	delta-BHC	4.808	4.161	119.0E6	169.7E6	47.745
8) B	Heptachlo...	5.727	4.760	108.3E6	151.0E6	48.851
9) A	Endosulfan I	6.115	5.131	104.0E6	137.4E6	50.306
10) B	trans-Chl...	5.984	5.011	106.2E6	146.2E6	49.913
11) B	cis-Chlor...	6.064	5.075	107.4E6	144.1E6	49.310
12) B	4,4'-DDE	6.234	5.265	209.3E6	291.8E6	106.023
13) MA	Dieldrin	6.390	5.396	225.8E6	321.5E6	102.623
14) MA	Endrin	6.620	5.671	180.5E6	278.4E6	98.938
15) B	Endosulfa...	6.838	5.964	191.2E6	276.9E6	100.520
16) A	4,4'-DDD	6.751	5.818	173.1E6	255.1E6	106.848
17) MA	4,4'-DDT	7.066	6.070	168.6E6	242.1E6	98.960
18) B	Endrin al...	6.968	6.144	142.3E6	207.4E6	95.455
19) B	Endosulfa...	7.202	6.366	180.4E6	262.5E6	96.875
20) A	Methoxychlor	7.539	6.646	434.0E6	596.9E6	470.749
21) B	Endrin ke...	7.687	6.872	204.4E6	304.6E6	104.596m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110823\
Data File : PD079497.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2023 17:30
Operator : AR\AJ
Sample : SFAMPESTSPIKE
Misc : 50/100PPB
ALS Vial : 100 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 17:46:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 07:14:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

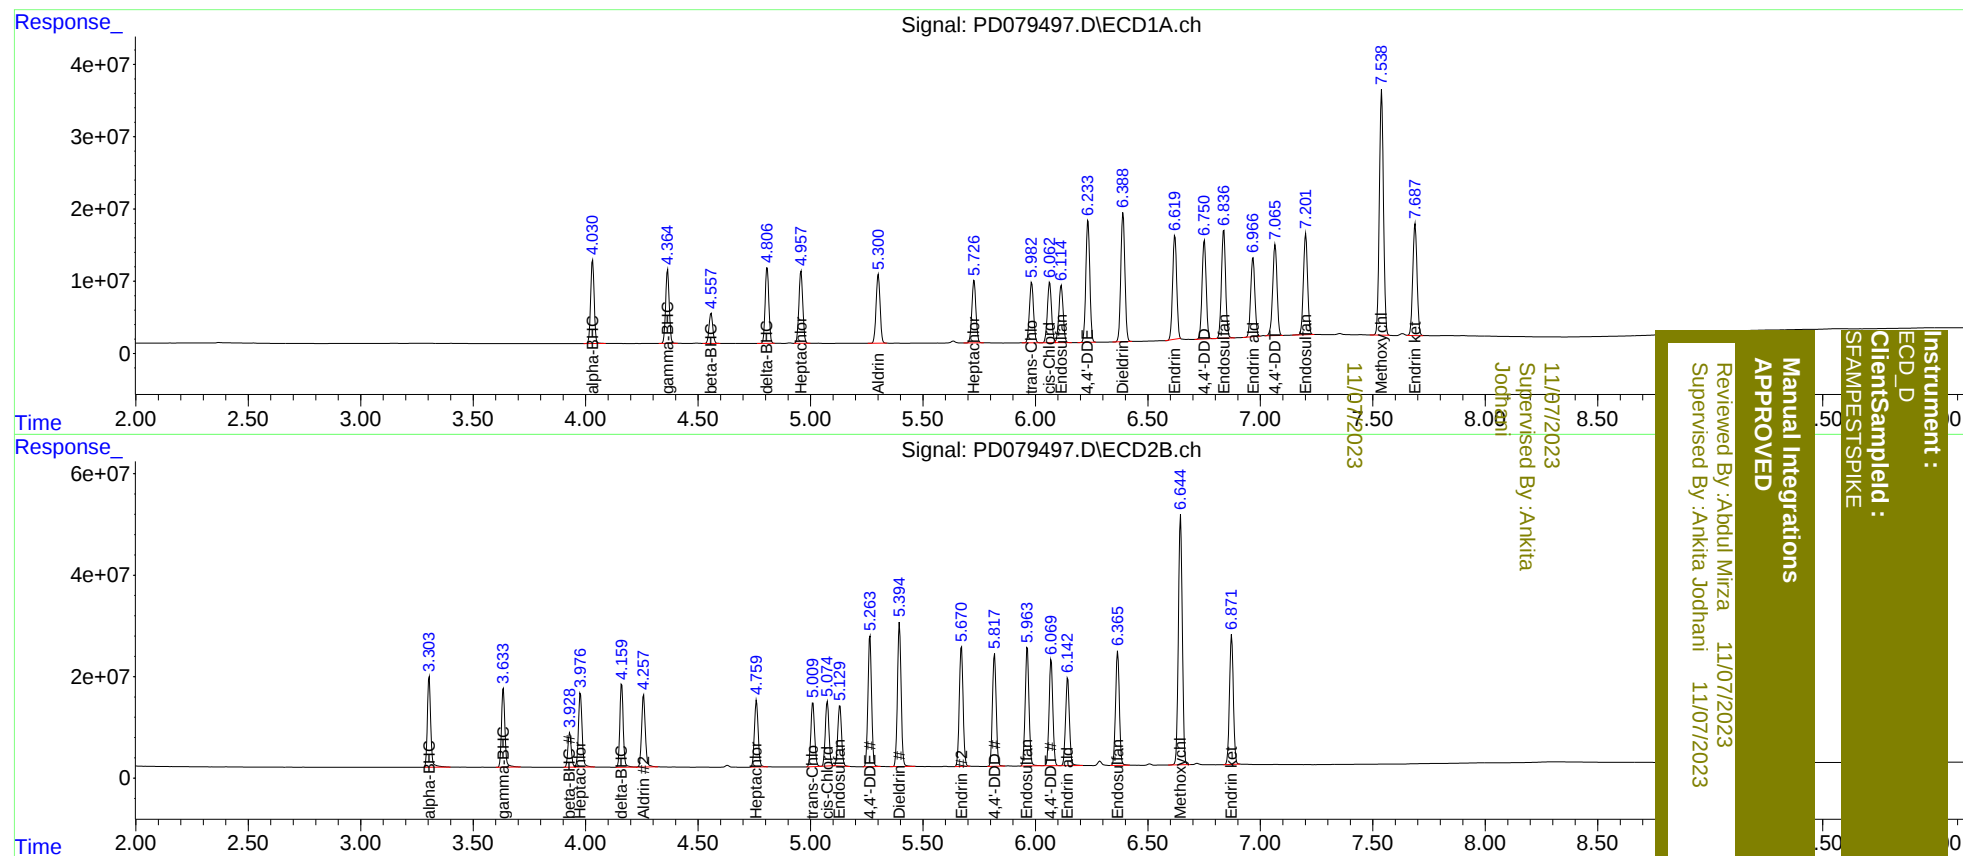

Instrument :
ECD_D
Client Sampled :
SFAMPESTSPIKE

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 11/07/2023
Supervised By: Ankita Jodhani 11/07/2023