

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110824\
 Data File : PD086480.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Nov 2024 21:15
 Operator : AR\AJ
 Sample : P4637-03MSD
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CC0R6MSD

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/11/2024
 Supervised By :mohammad ahmed 11/11/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 22:06:11 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102524CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 25 14:36:38 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.559	2.885	26401610	194.9E6	20.053	21.008m
27)	SA Decachlor...	9.096	8.094	31063382	177.4E6	17.327	18.763
Target Compounds							
2)	A alpha-BHC	4.009	3.401	154.8E6	821.3E6	62.185	57.163
3)	MA gamma-BHC...	4.341	3.738	152.6E6	754.0E6	61.349	55.903
4)	MA Heptachlor	4.942	4.092	149.3E6	755.9E6	60.389	55.331m
5)	MB Aldrin	5.284	4.381	139.6E6	729.7E6	57.586	53.787
6)	B beta-BHC	4.524	4.033	65792914	297.2E6	59.243	47.407
7)	B delta-BHC	4.773	4.271	154.7E6	758.7E6	59.744	54.072
8)	B Heptachlo...	5.704	4.886	124.8E6	636.3E6	54.617	50.745
9)	A Endosulfan I	6.089	5.261	115.4E6	597.7E6	56.956	52.062
10)	B trans-Chl...	5.959	5.140	122.8E6	676.2E6	55.636	51.407
11)	B cis-Chlor...	6.041	5.204	127.4E6	654.2E6	57.628	51.510
12)	B 4,4'-DDE	6.210	5.390	243.7E6	1250.0E6	114.112	101.943
13)	MA Dieldrin	6.362	5.526	268.0E6	1289.7E6	117.477	104.534m
14)	MA Endrin	6.589	5.804	221.6E6	1150.3E6	117.917	102.356
15)	B Endosulfa...	6.800	6.094	217.0E6	1093.9E6	108.222	99.151m
16)	A 4,4'-DDD	6.719	5.945	192.3E6	976.4E6	118.645	99.470
17)	MA 4,4'-DDT	7.035	6.200	195.3E6	1027.3E6	117.127m	100.108
18)	B Endrin al...	6.929	6.274	145.4E6	685.0E6	97.442	82.516
19)	B Endosulfa...	7.163	6.498	208.7E6	986.2E6	113.197	93.559
20)	A Methoxychlor	7.508	6.773	505.4E6	2209.9E6	537.051	464.916
21)	B Endrin ke...	7.645	7.007	224.7E6	1032.0E6	109.054	90.191

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110824\
Data File : PD086480.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Nov 2024 21:15
Operator : AR\AJ
Sample : P4637-03MSD
Misc :
ALS Vial : 27 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 22:06:11 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102524CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 25 14:36:38 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

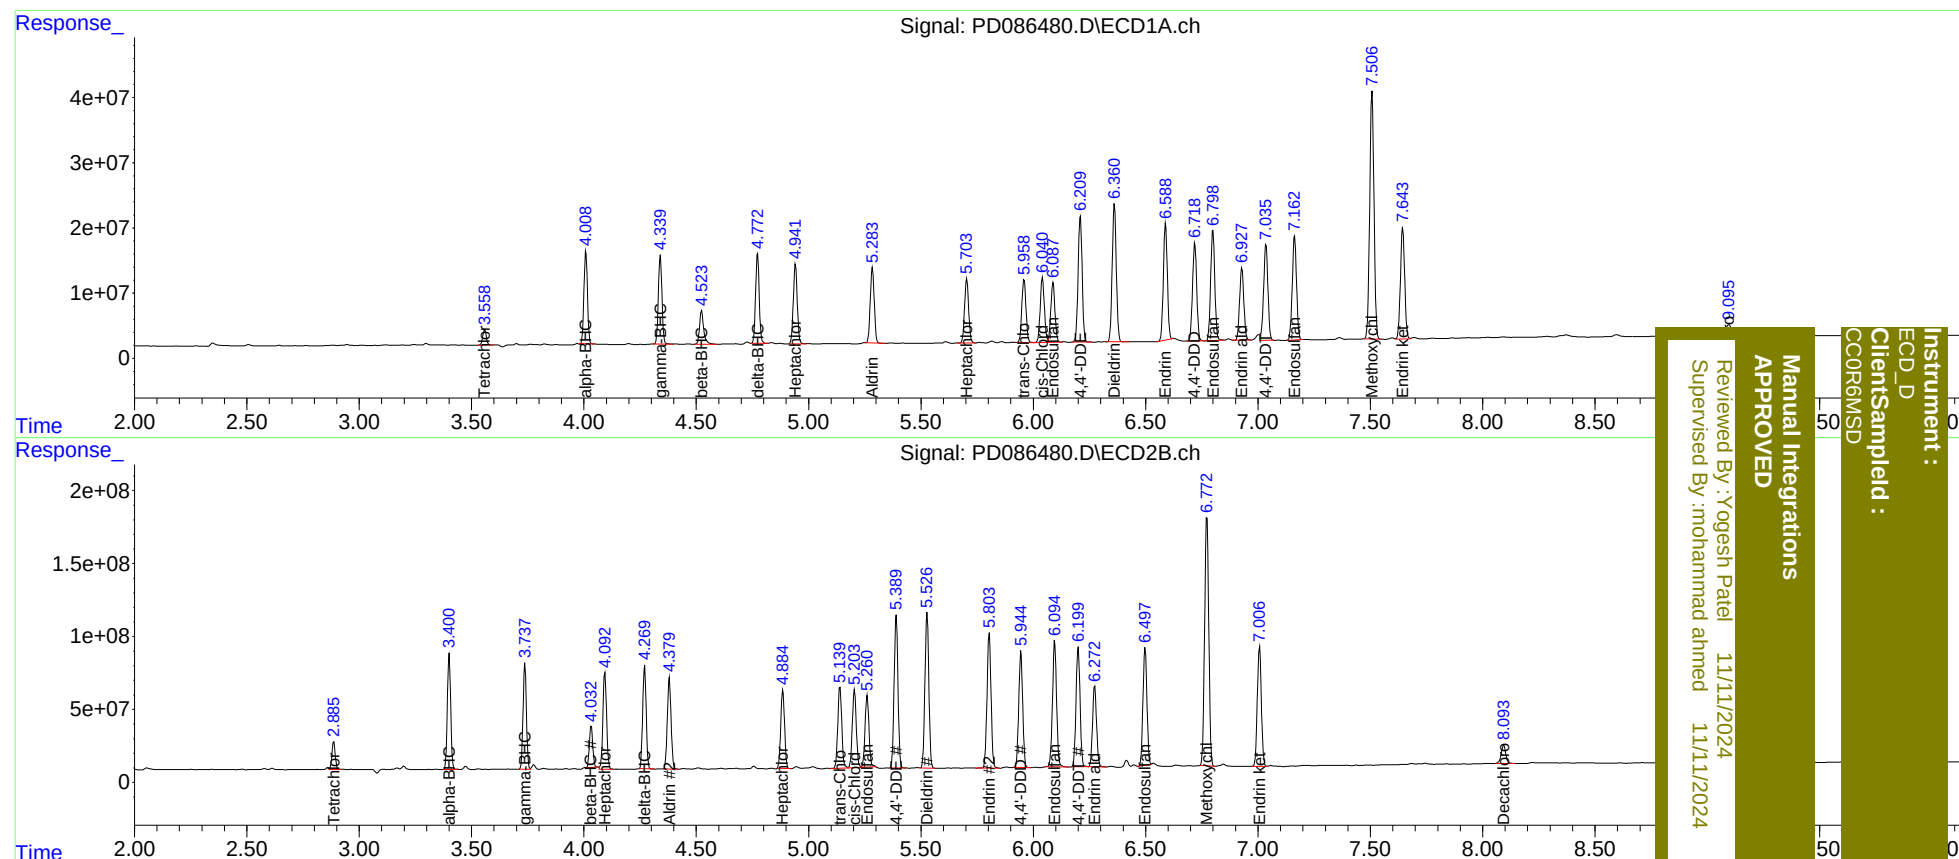

Manual Integrations
APPROVED
Reviewed By : Yogesh Patel 11/11/2024
Supervised By : mohammad ahmed 11/11/2024

Instrument :
ECD_D
Client Sampled :
CC0R6MSD