

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110824\
 Data File : PD086500.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Nov 2024 01:57
 Operator : AR\AJ
 Sample : P4687-18MS
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0CD4MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/12/2024
 Supervised By :Ankita Jodhani 11/12/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 04:05:59 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102524CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 25 14:36:38 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.558	2.886	23806583	186.0E6	18.082	20.047
27)	SA Decachlor...	9.094	8.093	39998449	230.2E6	22.311	24.346
Target Compounds							
2)	A alpha-BHC	4.008	3.401	165.7E6	868.3E6	66.569	60.436
3)	MA gamma-BHC...	4.340	3.738	164.2E6	813.5E6	66.006	60.311
4)	MA Heptachlor	4.941	4.093	142.2E6	735.4E6	57.533	53.826m
5)	MB Aldrin	5.284	4.380	133.6E6	699.8E6	55.108	51.585m
6)	B beta-BHC	4.524	4.032	62675077	350.3E6	56.435	55.869m
7)	B delta-BHC	4.773	4.269	129.3E6	660.8E6	49.947	47.095m
8)	B Heptachlo...	5.703	4.885	139.9E6	722.0E6	61.237	57.577m
9)	A Endosulfan I	6.087	5.261	130.1E6	674.8E6	64.211	58.776
10)	B trans-Chl...	5.958	5.140	133.9E6	742.0E6	60.704	56.408
11)	B cis-Chlor...	6.040	5.205	138.2E6	731.9E6	62.496	57.623
12)	B 4,4'-DDE	6.209	5.391	268.1E6	1381.3E6	125.517	112.652
13)	MA Dieldrin	6.360	5.526	300.1E6	1434.7E6	131.561	116.285m
14)	MA Endrin	6.587	5.804	235.2E6	1245.2E6	125.145	110.800
15)	B Endosulfa...	6.799	6.093	246.0E6	1236.5E6	122.694	112.072m
16)	A 4,4'-DDD	6.718	5.945	217.0E6	1181.7E6	133.945	120.380
17)	MA 4,4'-DDT	7.033	6.198	204.6E6	1158.8E6	122.739m	112.924m
18)	B Endrin al...	6.927	6.273	173.0E6	882.3E6	115.979	106.292
19)	B Endosulfa...	7.161	6.497	220.6E6	1156.2E6	119.690	109.681
20)	A Methoxychlor	7.507	6.772	531.5E6	2394.9E6	564.754	503.846
21)	B Endrin ke...	7.643	7.006	257.6E6	1313.9E6	125.005	114.826

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110824\
Data File : PD086500.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Nov 2024 01:57
Operator : AR\AJ
Sample : P4687-18MS
Misc :
ALS Vial : 52 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 04:05:59 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102524CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 25 14:36:38 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

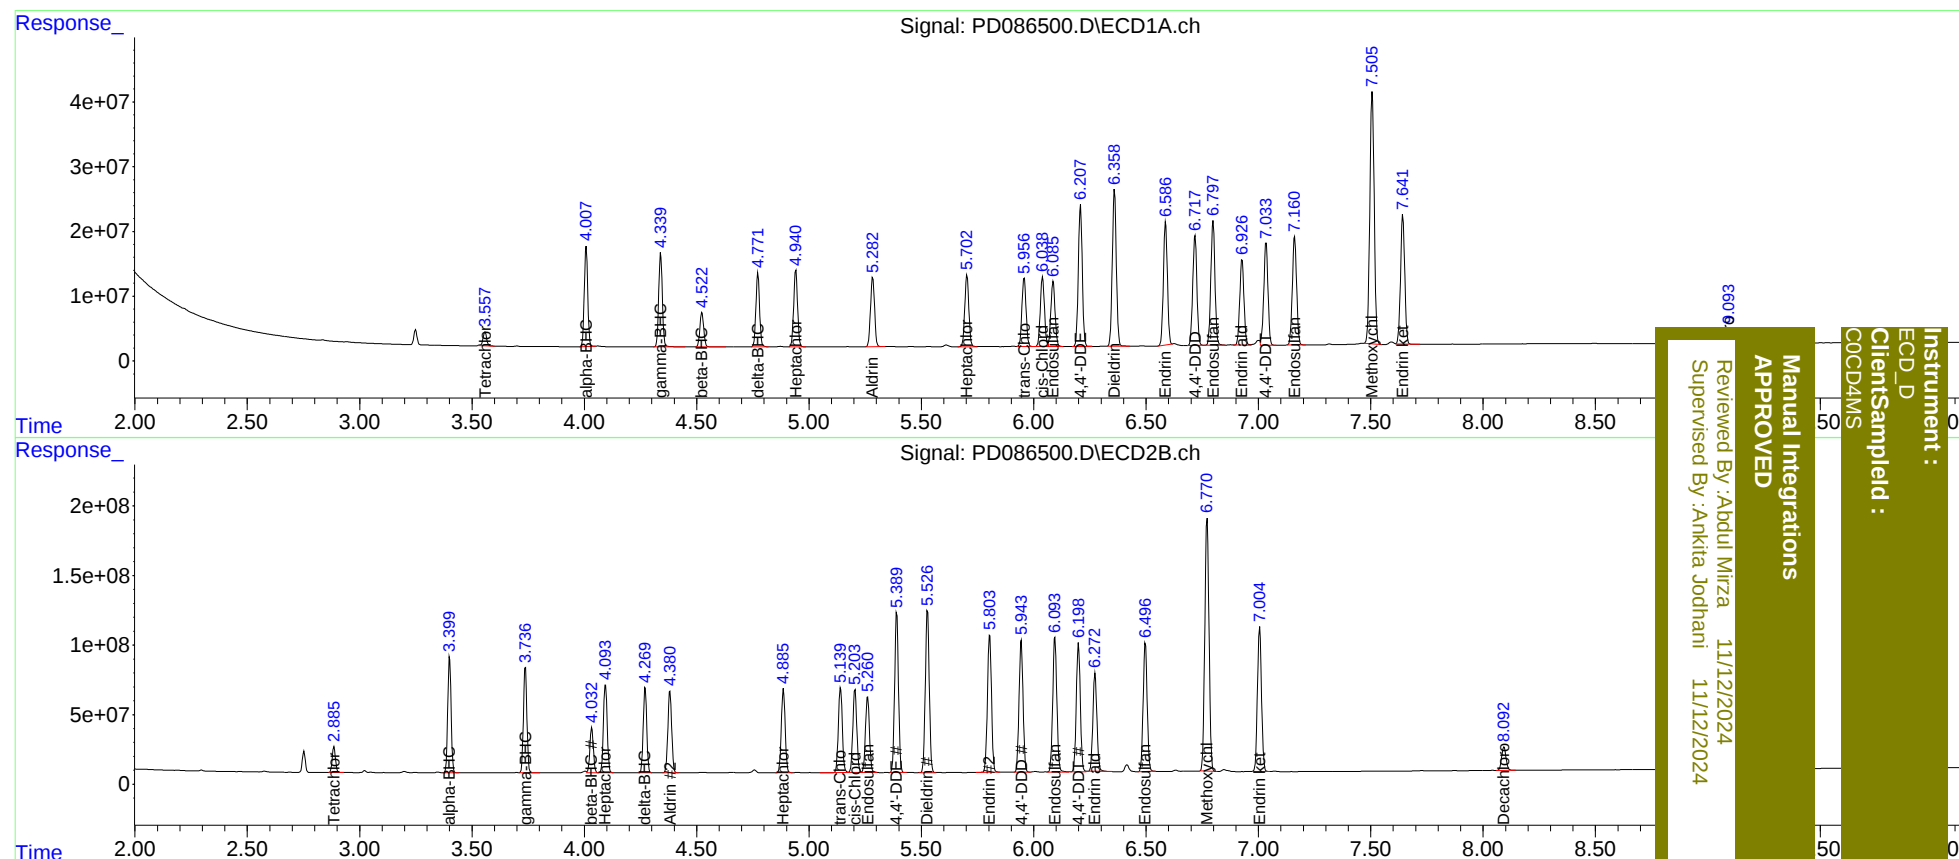

Instrument :
ECD_D
ClientSampled :
C00CD4MS

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 11/12/2024
Supervised By: Ankita Jodhani 11/12/2024