

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110824\
 Data File : PD086455.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Nov 2024 13:42
 Operator : AR\AJ
 Sample : P4636-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CC0P2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/11/2024
 Supervised By :mohammad ahmed 11/11/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 21:16:05 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102524CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 25 14:36:38 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.558	2.886	25659429	163.6E6	19.489m	17.632m
2) SA Decachlor...	9.098	8.095	26976256	179.3E6	15.047	18.957 #
Target Compounds						
8) B Heptachlo...	5.727	4.885	1279759	4960089	0.560m	0.396m#
10) B trans-Chl...	5.959	5.138	10533247	15775068	4.774m	1.199m#
11) B cis-Chlor...	6.052	5.192	24783647	33581655	11.209	2.644m#
17) MA 4,4'-DDT	7.032	6.198	1358531	11198164	0.815m	1.091 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110824\
Data File : PD086455.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Nov 2024 13:42
Operator : AR\AJ
Sample : P4636-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 21:16:05 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102524CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 25 14:36:38 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

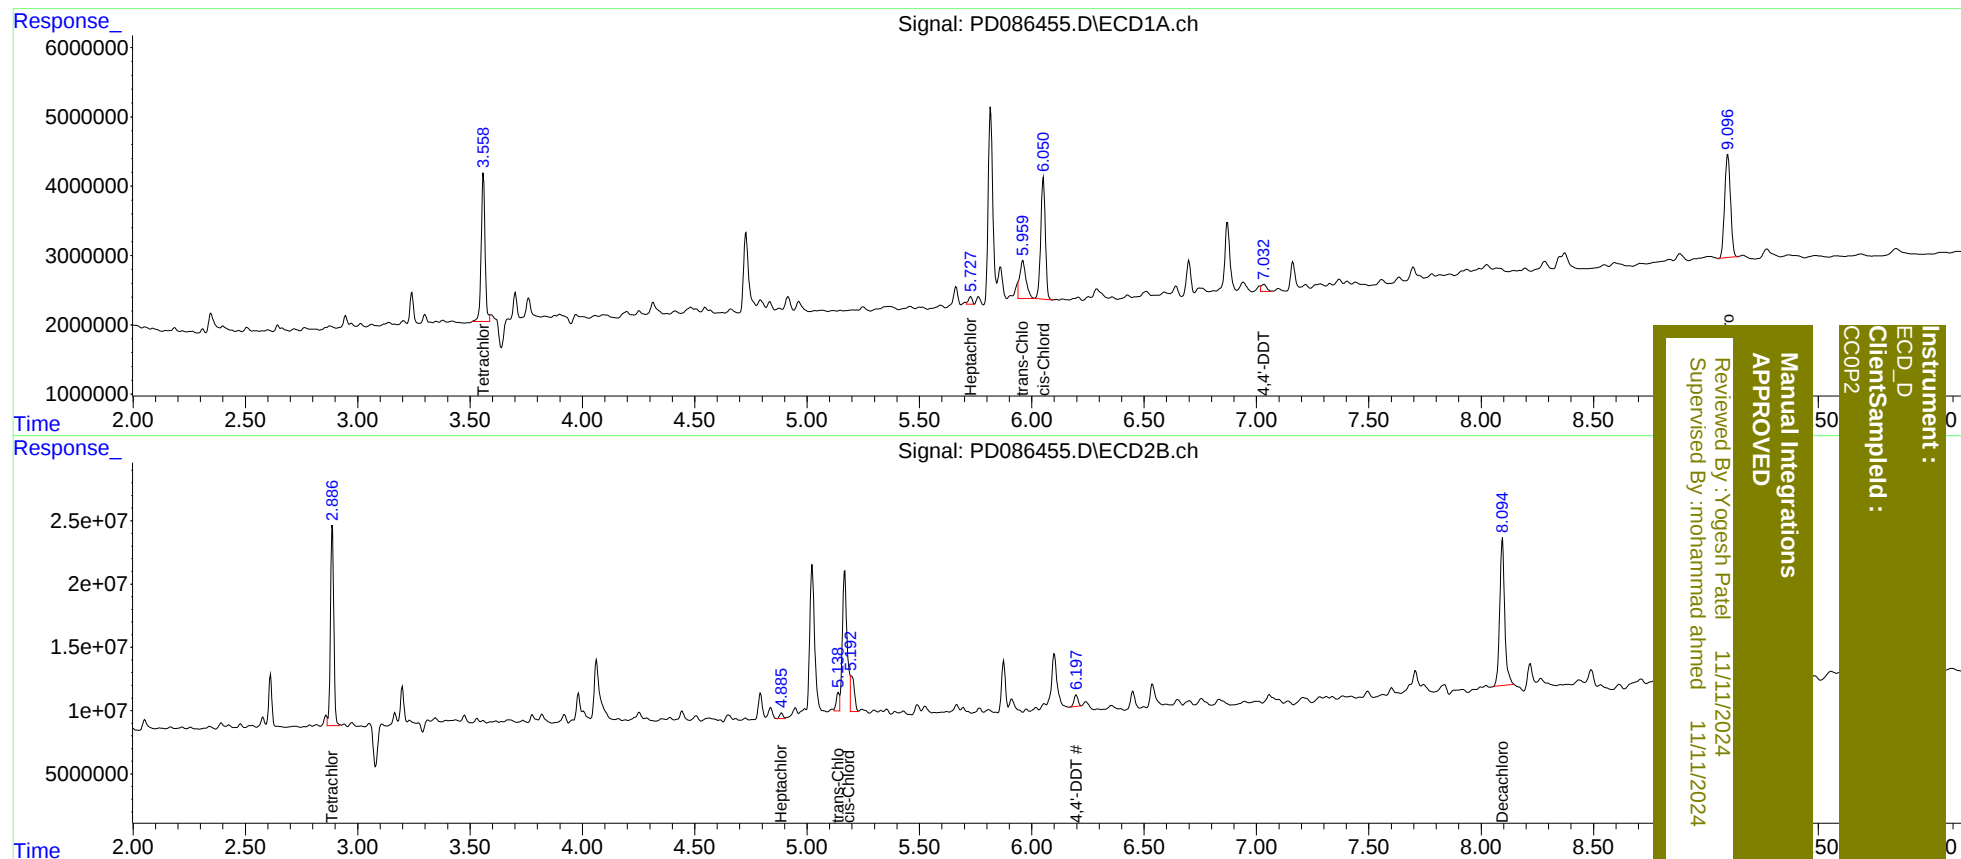

Manual Integrations
APPROVED
Reviewed By : Yogesh Patel 11/11/2024
Supervised By : mohammad ahmed 11/11/2024

Instrument :
ECD_D
ClientSampled :
CC0P2