

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110824\
 Data File : PD086505.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Nov 2024 03:08
 Operator : AR\AJ
 Sample : P4687-24
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0CP8

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/12/2024
 Supervised By : Ankita Jodhani 11/12/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 04:07:32 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102524CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 25 14:36:38 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.559	2.887	27833184	184.1E6	21.140	19.848
2) SA Decachlor...	9.093	8.094	30503448	171.9E6	17.015	18.179
Target Compounds						
7) B delta-BHC	4.788	4.293	2497872	8108826	0.965m	0.578m#
20) A Methoxychlor	7.506	6.770	326473	2691766	0.347m	0.566m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110824\
Data File : PD086505.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Nov 2024 03:08
Operator : AR\AJ
Sample : P4687-24
Misc :
ALS Vial : 57 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 04:07:32 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102524CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 25 14:36:38 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

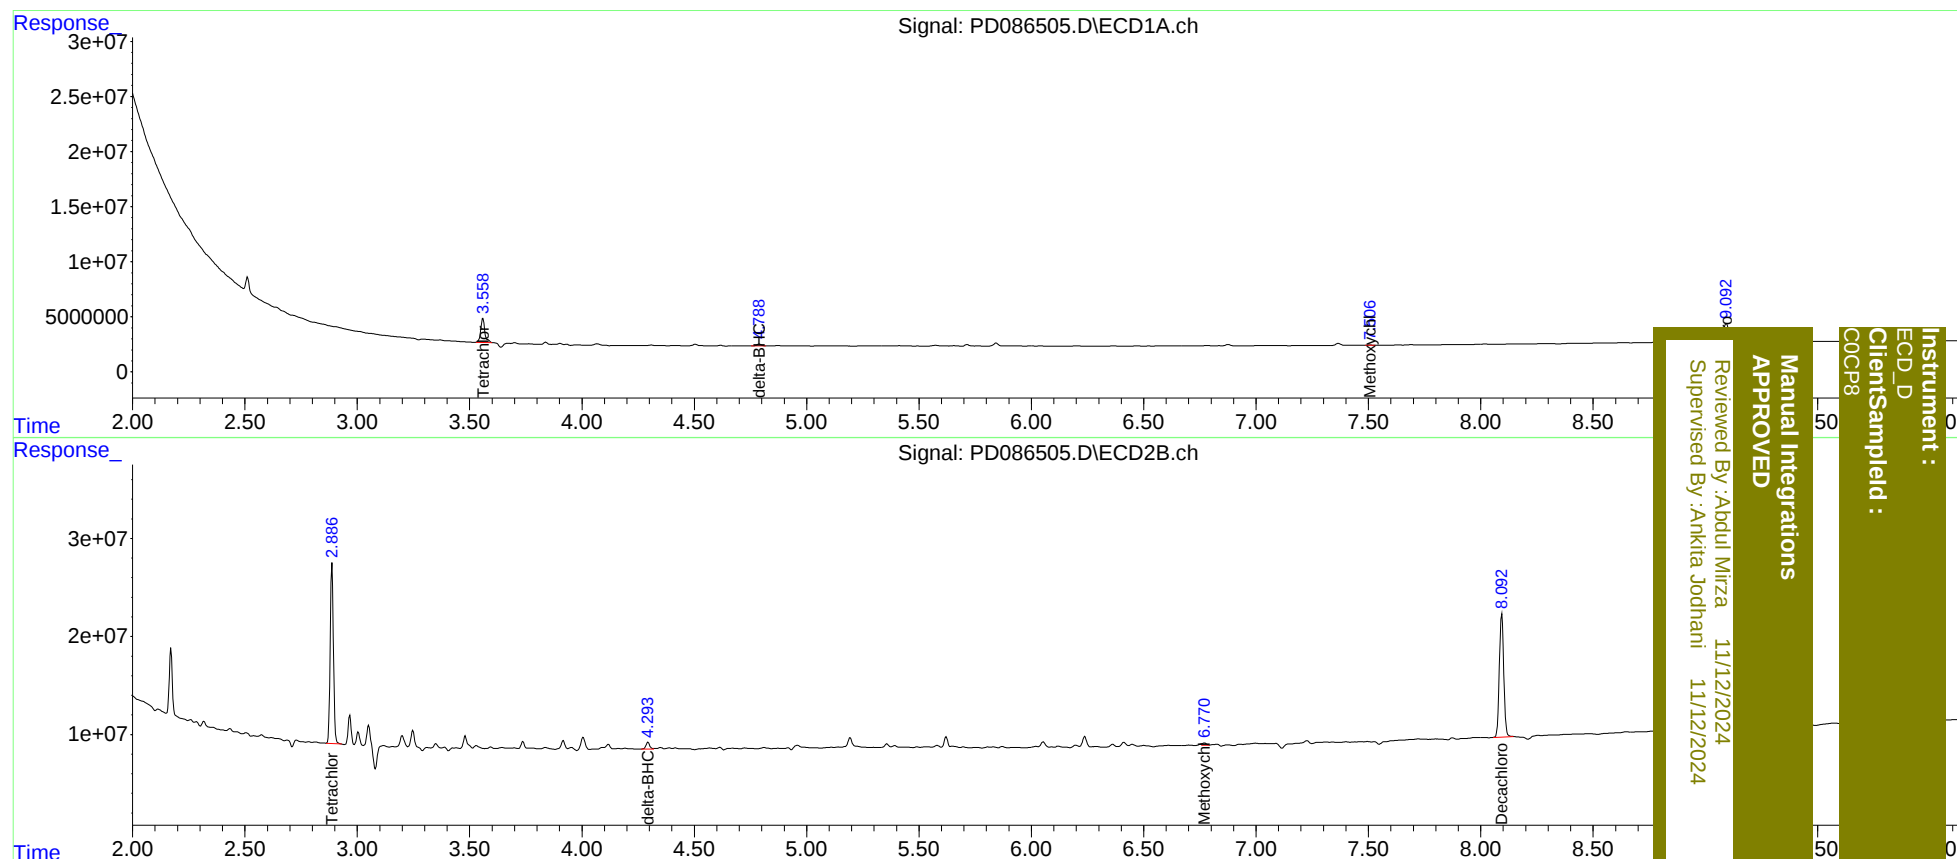

Reviewed By: Abdul Mirza 11/12/2024
Supervised By: Ankita Jodhani 11/12/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
C00CP8