

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD110921\  
 Data File : PD066801.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 09 Nov 2021 08:50  
 Operator : AR\AJ  
 Sample : HEXANE  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 ECD\_D  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Nov 10 05:32:03 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD102821.M  
 Quant Title : GC Extractables  
 QLast Update : Thu Oct 28 02:17:57 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

#### System Monitoring Compounds

| Target Compounds |              |       |        |         |         |               |
|------------------|--------------|-------|--------|---------|---------|---------------|
| 2) A             | alpha-BHC    | 0.000 | 4.377  | 0       | 4311134 | N.D. 0.391 #  |
| 4) MA            | Heptachlor   | 0.000 | 5.134  | 0       | 656116  | N.D. 0.067 #  |
| 5) MB            | Aldrin       | 0.000 | 5.464  | 0       | 488506  | N.D. 0.054 #  |
| 8) B             | Heptachlo... | 0.000 | 5.863f | 0       | 3128132 | N.D. 0.432 #  |
| 15) B            | Endosulfa... | 6.258 | 0.000  | 1941159 | 0       | 0.976 N.D. #  |
| 18) B            | Endrin al... | 0.000 | 7.035f | 0       | 619452  | N.D. 0.109 #  |
| 19) B            | Endosulfa... | 6.627 | 0.000  | 2265803 | 0       | 1.217 N.D. #  |
| 20) A            | Methoxychlor | 0.000 | 7.566  | 0       | 44806   | N.D. 0.011 #  |
| 27)              | Chlordane-5  | 6.258 | 0.000  | 1941159 | 0       | 22.953 N.D. # |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD110921\  
Data File : PD066801.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 09 Nov 2021 08:50  
Operator : AR\AJ  
Sample : HEXANE  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Nov 10 05:32:03 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD102821.M  
Quant Title : GC Extractables  
QLast Update : Thu Oct 28 02:17:57 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

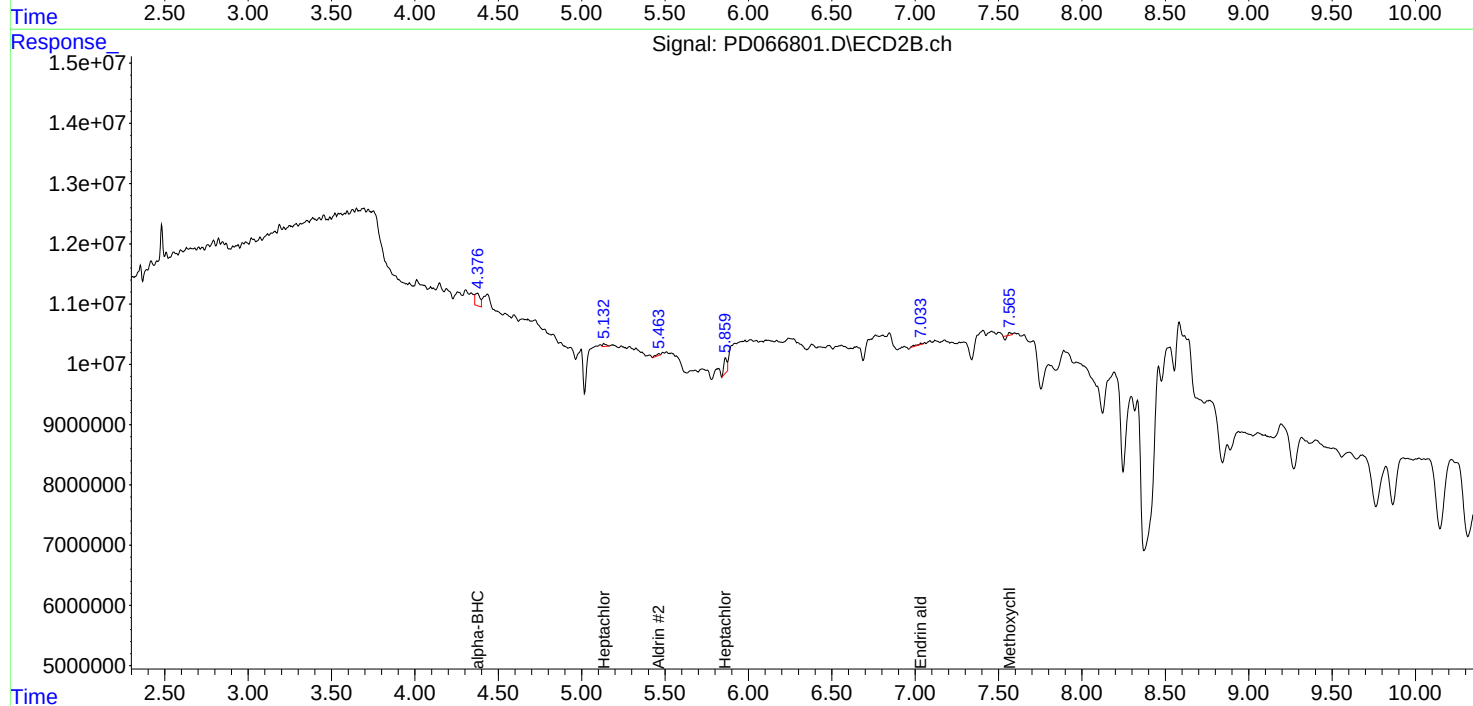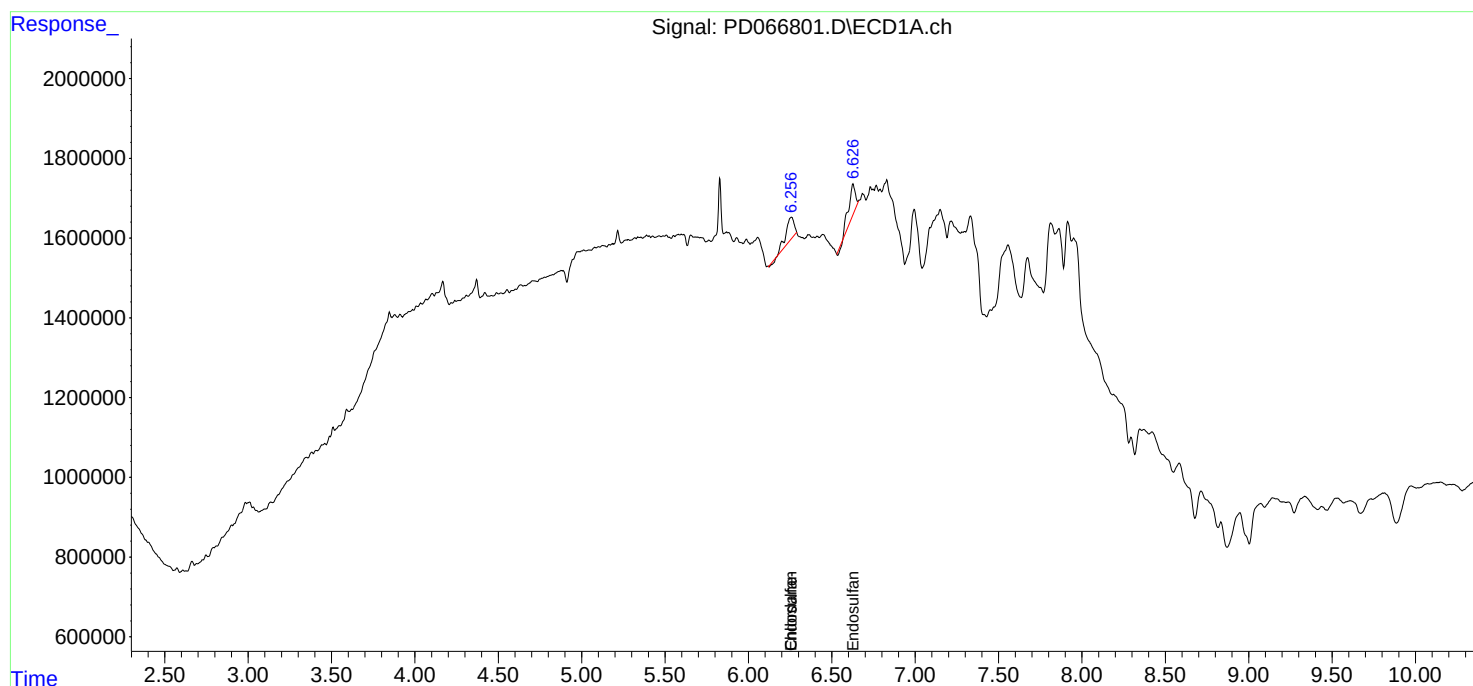


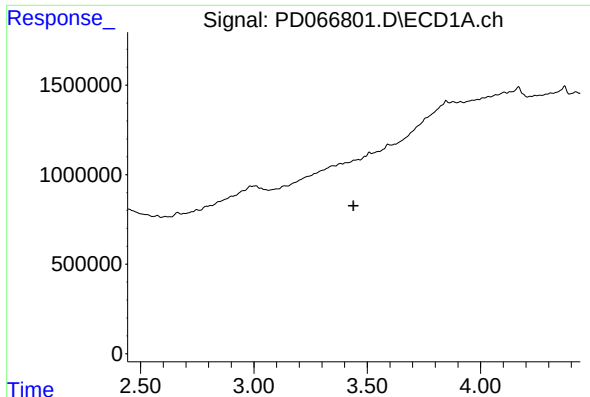

#1 Tetrachloro-m-xylene


R.T.: 0.000 min  
Exp R.T. : 3.440 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_D  
ClientSampleId :

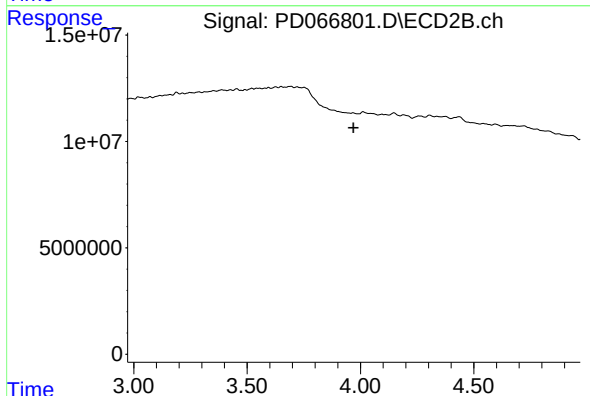


#1 Tetrachloro-m-xylene

R.T.: 0.000 min  
Exp R.T. : 3.970 min  
Response: 0  
Conc: N.D.

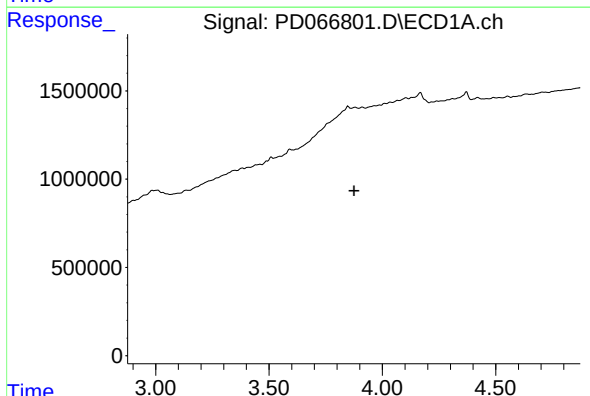


#2 alpha-BHC

R.T.: 0.000 min  
Exp R.T. : 3.876 min  
Response: 0  
Conc: N.D.

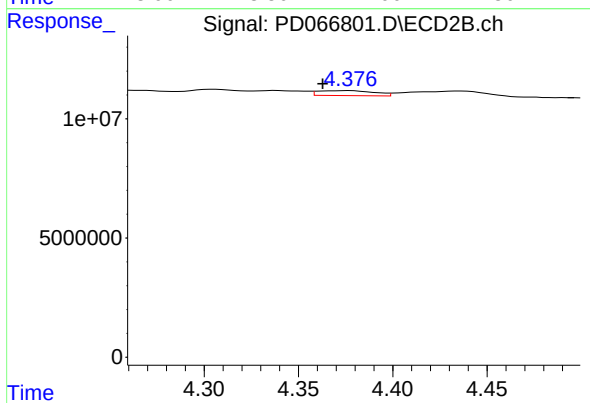

#2 alpha-BHC


R.T.: 4.377 min  
Delta R.T.: 0.014 min  
Response: 4311134  
Conc: 0.39 ng/ml

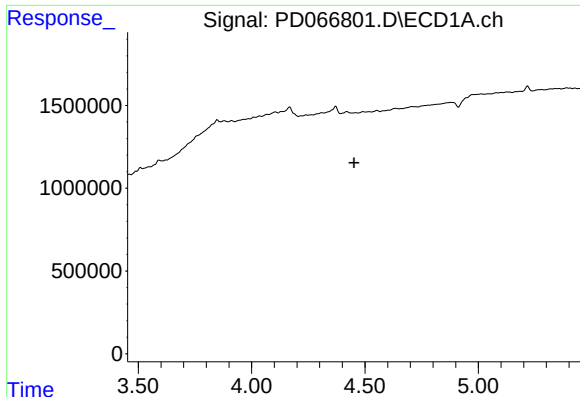

#4 Heptachlor


R.T.: 0.000 min  
Exp R.T.: 4.452 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_D  
ClientSampleId :

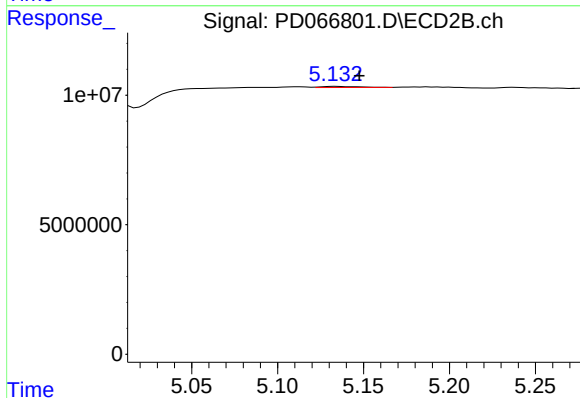


#4 Heptachlor

R.T.: 5.134 min  
Delta R.T.: -0.014 min  
Response: 656116  
Conc: 0.07 ng/ml

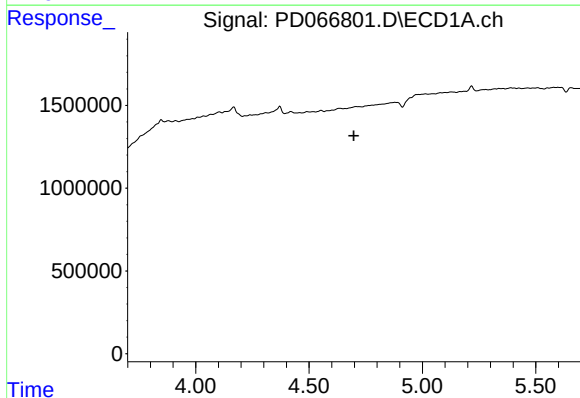


#5 Aldrin

R.T.: 0.000 min  
Exp R.T.: 4.697 min  
Response: 0  
Conc: N.D.

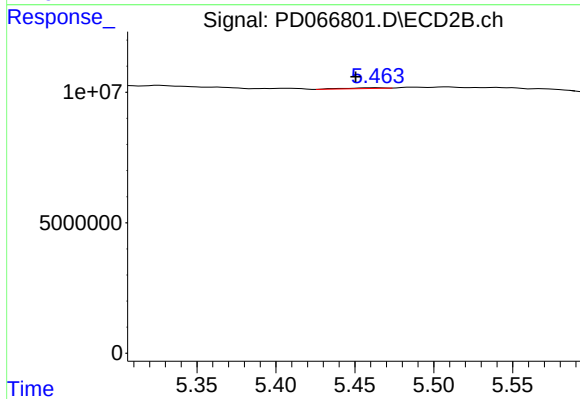

#5 Aldrin


R.T.: 5.464 min  
Delta R.T.: 0.014 min  
Response: 488506  
Conc: 0.05 ng/ml

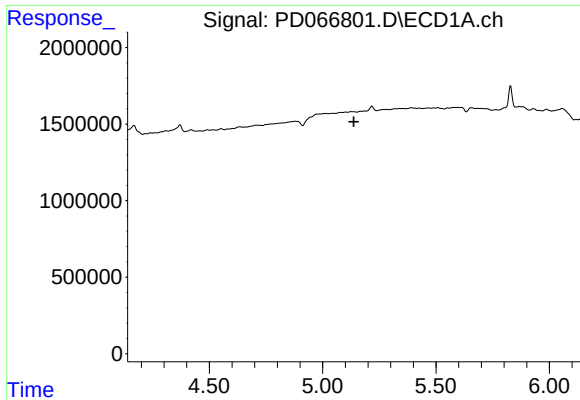

#8 Heptachlor epoxide


R.T.: 0.000 min  
Exp R.T.: 5.138 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_D  
ClientSampleId :

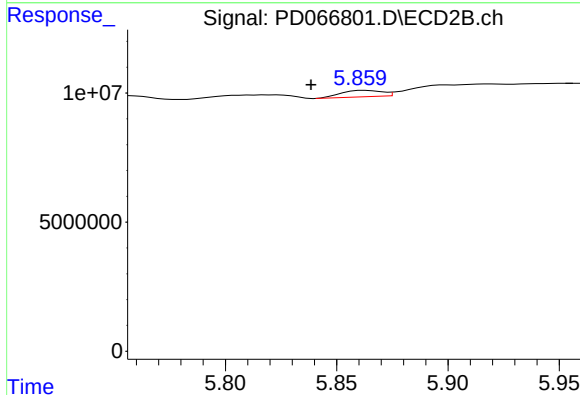


#8 Heptachlor epoxide

R.T.: 5.863 min  
Delta R.T.: 0.024 min  
Response: 3128132  
Conc: 0.43 ng/ml

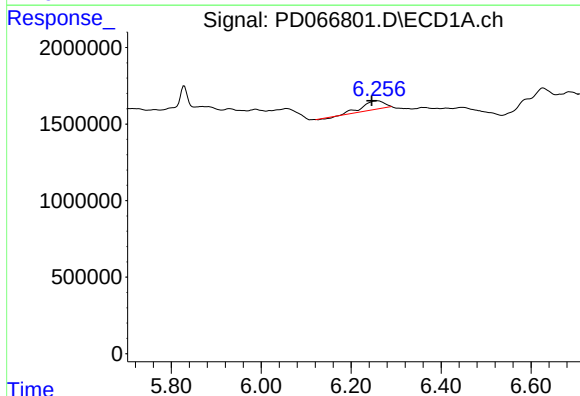


#15 Endosulfan II

R.T.: 6.258 min  
Delta R.T.: 0.013 min  
Response: 1941159  
Conc: 0.98 ng/ml

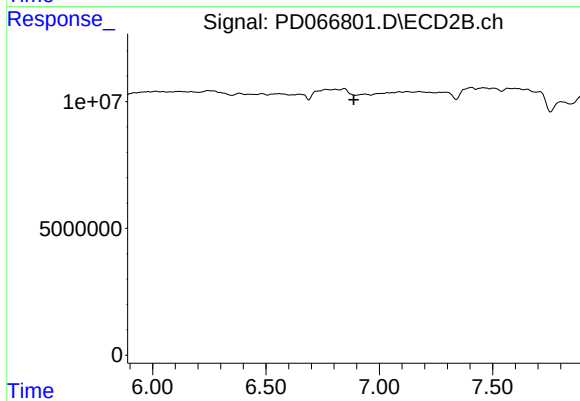

#15 Endosulfan II


R.T.: 0.000 min  
Exp R.T.: 6.888 min  
Response: 0  
Conc: N.D.

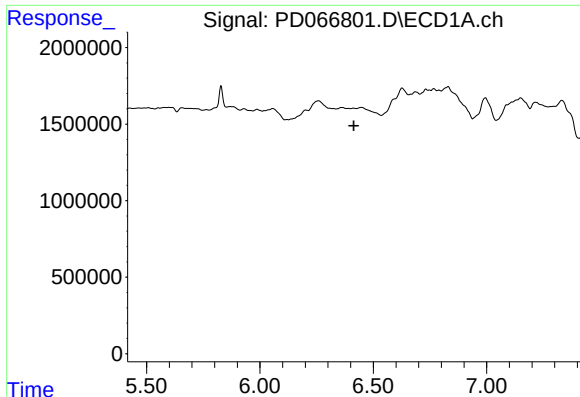

#18 Endrin aldehyde


R.T.: 0.000 min  
Exp R.T.: 6.414 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_D  
ClientSampleId :

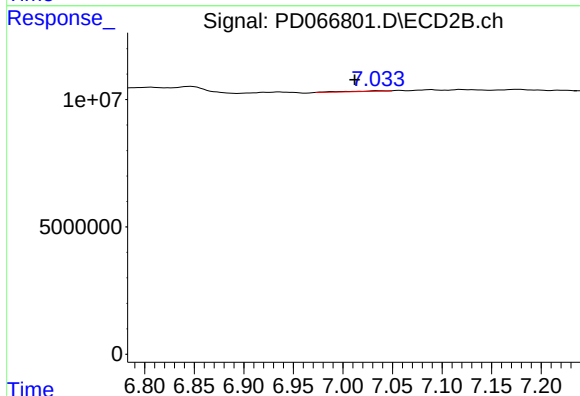


#18 Endrin aldehyde

R.T.: 7.035 min  
Delta R.T.: 0.023 min  
Response: 619452  
Conc: 0.11 ng/ml

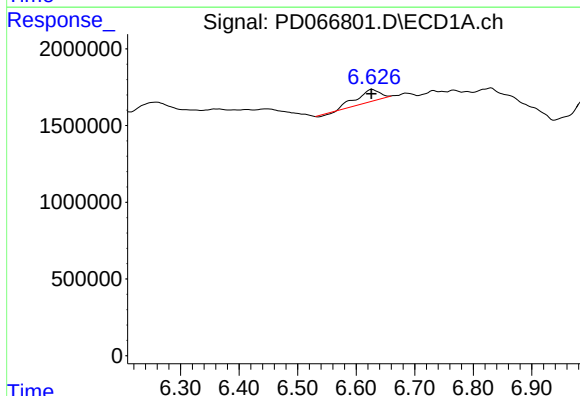


#19 Endosulfan Sulfate

R.T.: 6.627 min  
Delta R.T.: 0.001 min  
Response: 2265803  
Conc: 1.22 ng/ml

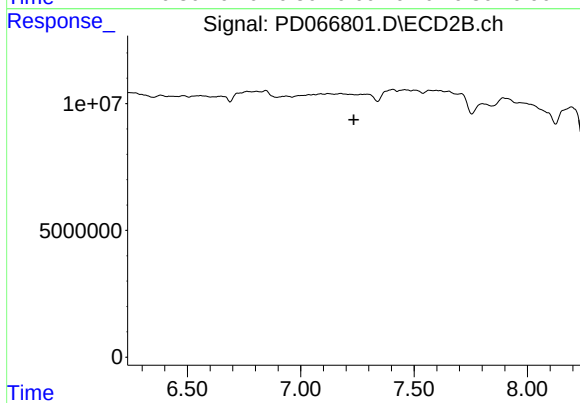

#19 Endosulfan Sulfate


R.T.: 0.000 min  
Exp R.T.: 7.235 min  
Response: 0  
Conc: N.D.

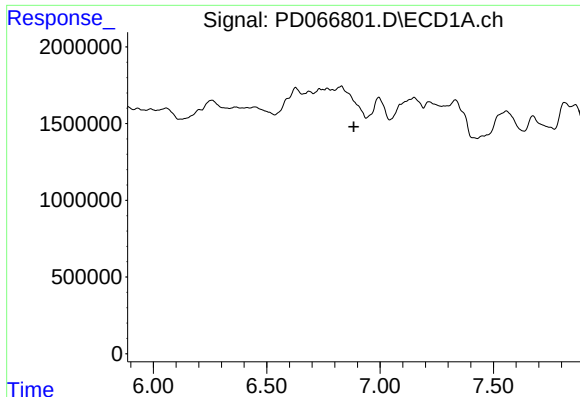

#20 Methoxychlor


R.T.: 0.000 min  
Exp R.T.: 6.884 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_D  
ClientSampleId :

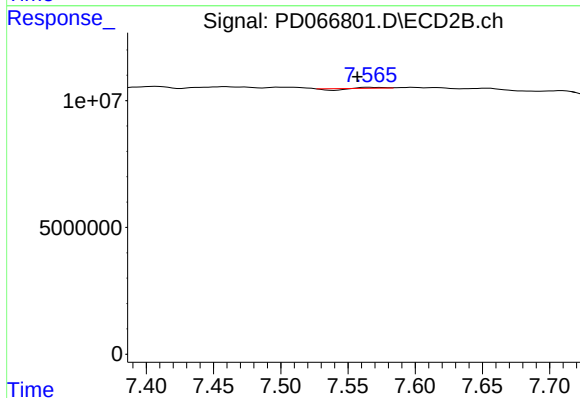


#20 Methoxychlor

R.T.: 7.566 min  
Delta R.T.: 0.009 min  
Response: 44806  
Conc: 0.01 ng/ml

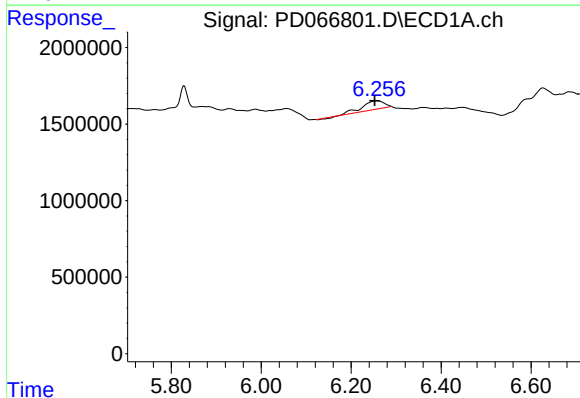


#27 Chlordane-5

R.T.: 6.258 min  
Delta R.T.: 0.006 min  
Response: 1941159  
Conc: 22.95 ng/ml

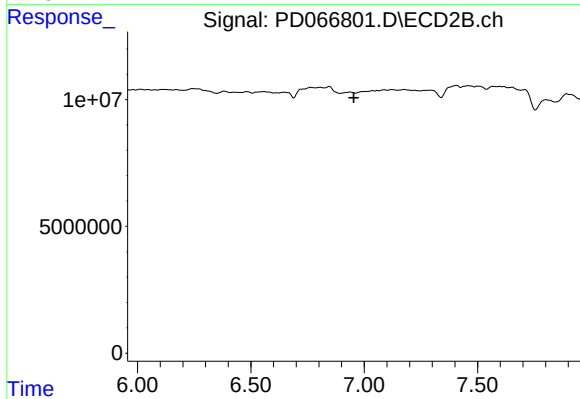

#27 Chlordane-5


R.T.: 0.000 min  
Exp R.T.: 6.955 min  
Response: 0  
Conc: N.D.

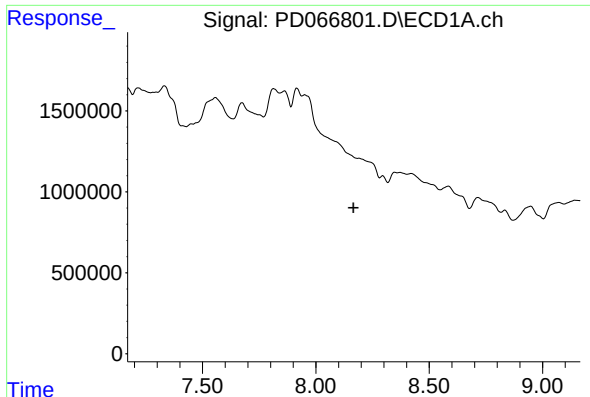

#28 Decachlorobiphenyl

R.T.: 0.000 min  
Exp R.T.: 8.166 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_D  
ClientSampleId :

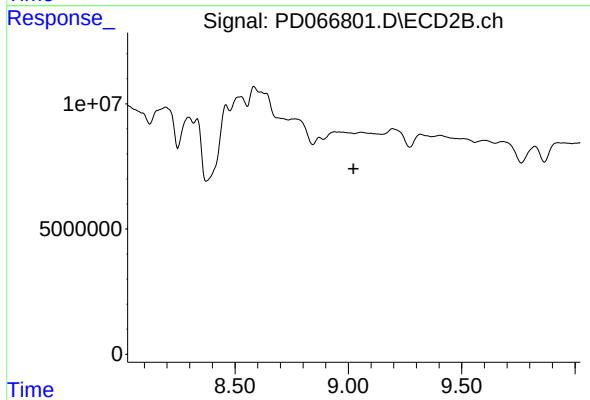

#28 Decachlorobiphenyl

R.T.: 0.000 min  
Exp R.T.: 9.023 min  
Response: 0  
Conc: N.D.