

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110921\
 Data File : PD066825.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Nov 2021 17:50
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 10 05:39:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102821.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 28 02:17:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.438	3.968	33405723	149.2E6	17.904	18.434
28)	SA Decachlor...	8.164	9.026	19847102	99806092	17.177	18.529
Target Compounds							
2)	A alpha-BHC	0.000	4.368	0	604852	N.D.	0.055 #
4)	MA Heptachlor	0.000	5.156	0	448815	N.D.	0.046 #
6)	B beta-BHC	4.414	4.845f	1542011	2613724	1.234	0.561 #
8)	B Heptachlo...	0.000	5.858f	0	4665170	N.D.	0.644 #
14)	MA Endrin	5.982	0.000	1985349	0	0.949	N.D. #
15)	B Endosulfa...	6.261f	6.879	1786441	104827	0.898	0.015 #
18)	B Endrin al...	0.000	7.013	0	2818029	N.D.	0.495 #
21)	B Endrin ke...	0.000	7.730f	0	9845597	N.D.	1.171 #
27)	Chlordane-5	6.261	0.000	1786441	0	21.124	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110921\
Data File : PD066825.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Nov 2021 17:50
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 10 05:39:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102821.M
Quant Title : GC Extractables
QLast Update : Thu Oct 28 02:17:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

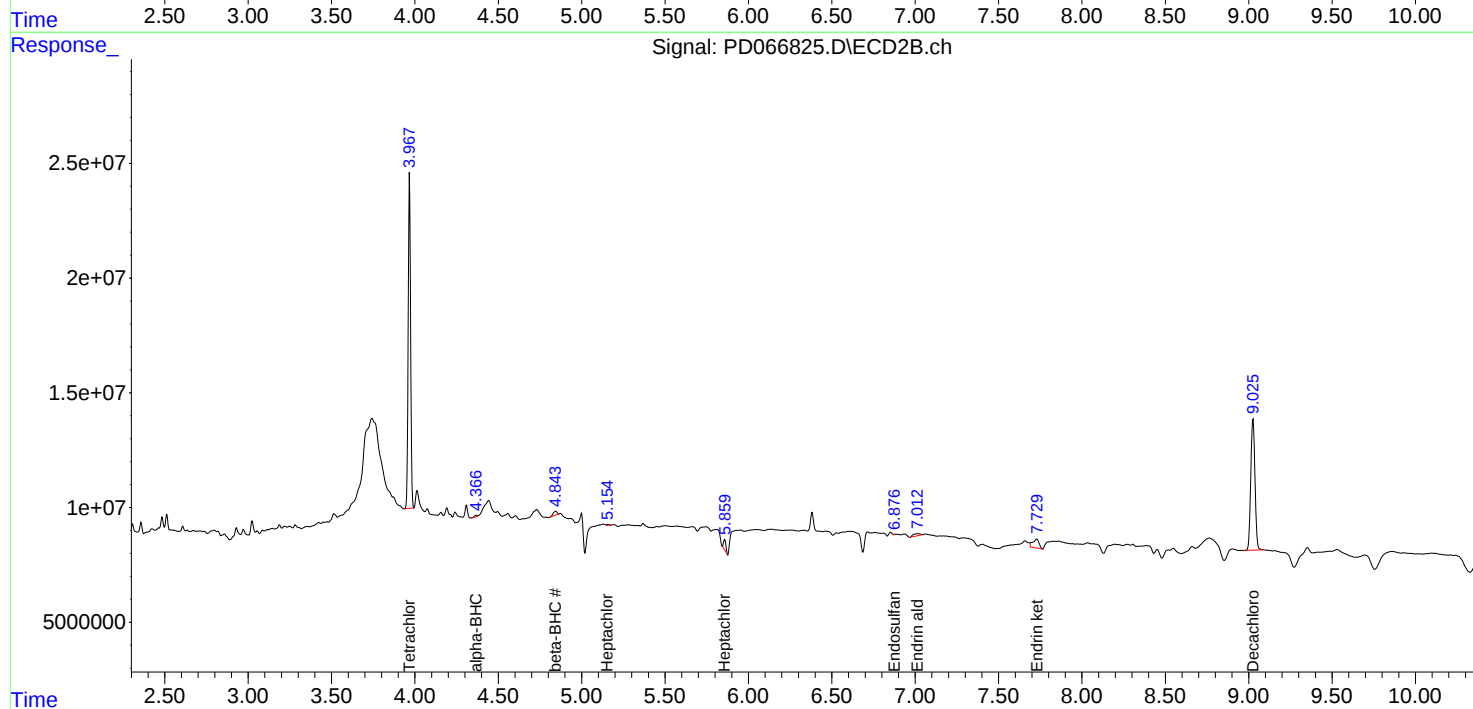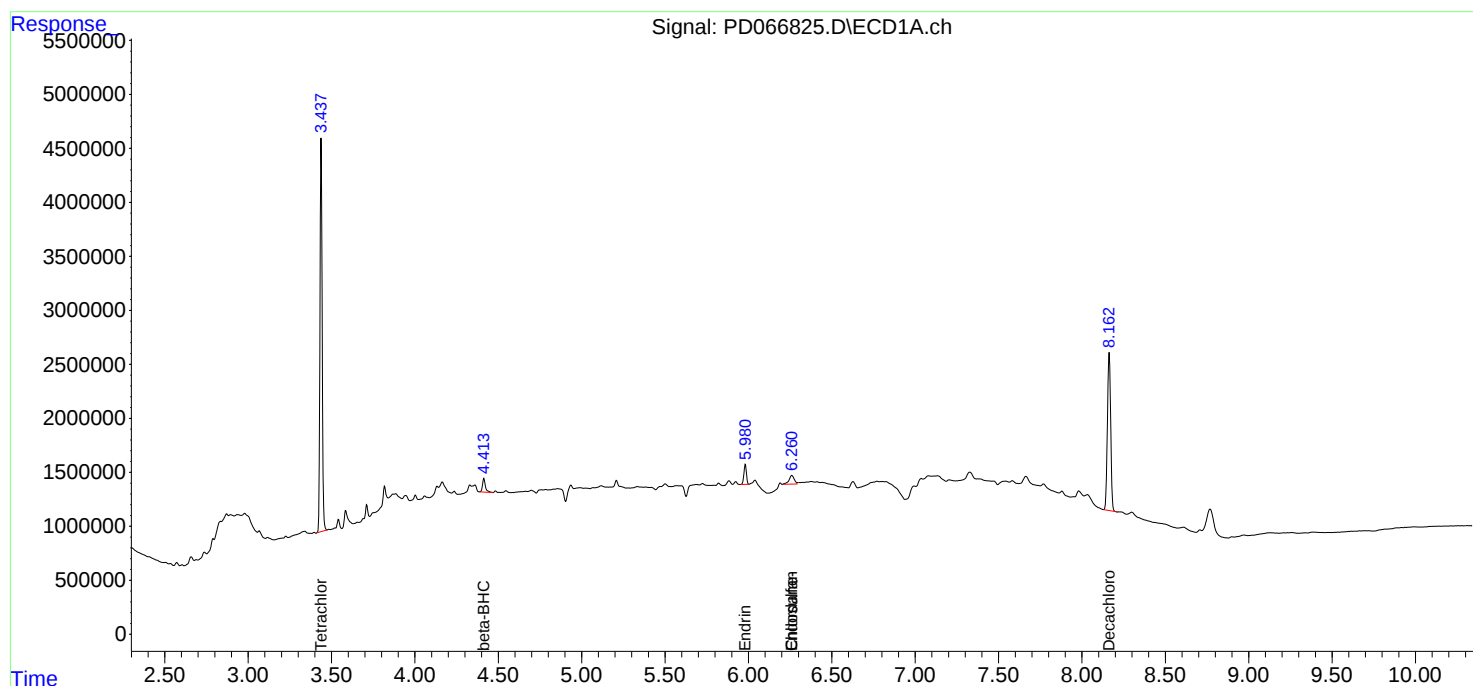


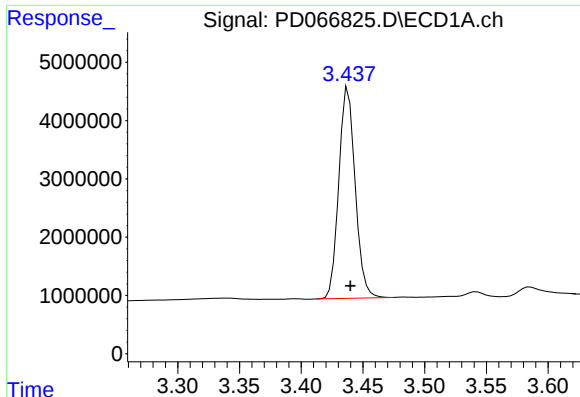

#1 Tetrachloro-m-xylene


R.T.: 3.438 min
Delta R.T.: -0.002 min
Response: 33405723
Conc: 17.90 ng/ml

Instrument :
ECD_D
ClientSampleId :

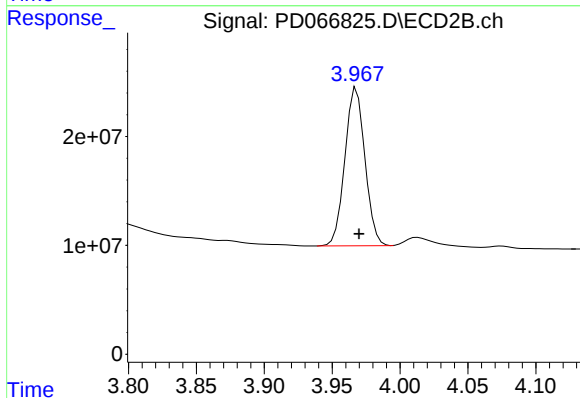


#1 Tetrachloro-m-xylene

R.T.: 3.968 min
Delta R.T.: -0.002 min
Response: 149173331
Conc: 18.43 ng/ml

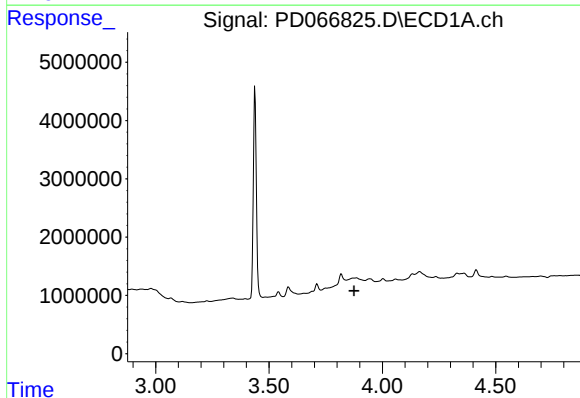


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.876 min
Response: 0
Conc: N.D.

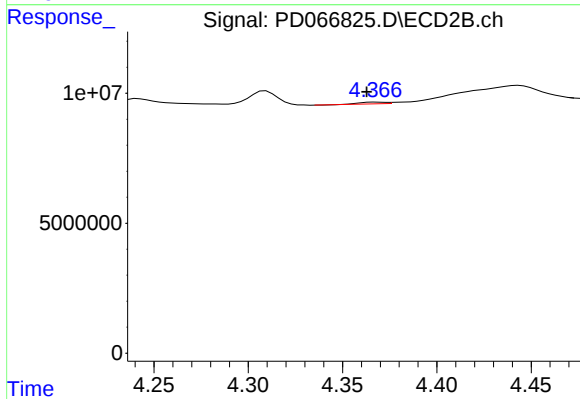

#2 alpha-BHC


R.T.: 4.368 min
Delta R.T.: 0.005 min
Response: 604852
Conc: 0.05 ng/ml

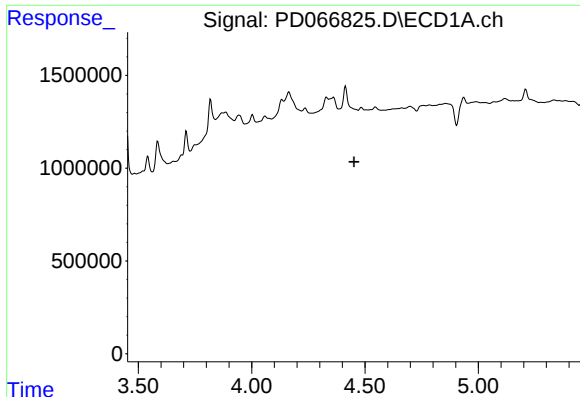

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.452 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

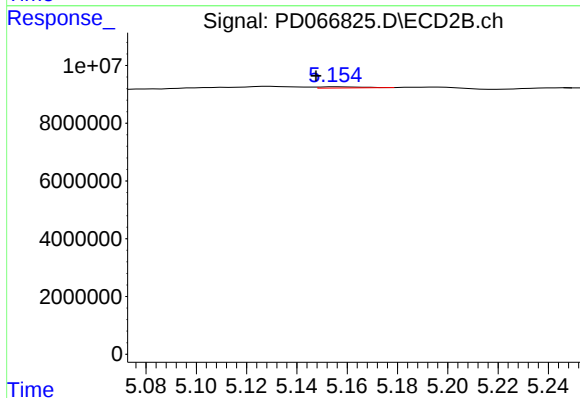


#4 Heptachlor

R.T.: 5.156 min
Delta R.T.: 0.008 min
Response: 448815
Conc: 0.05 ng/ml

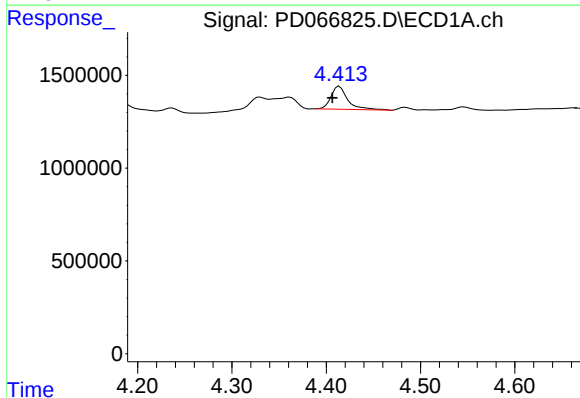


#6 beta-BHC

R.T.: 4.414 min
Delta R.T.: 0.008 min
Response: 1542011
Conc: 1.23 ng/ml

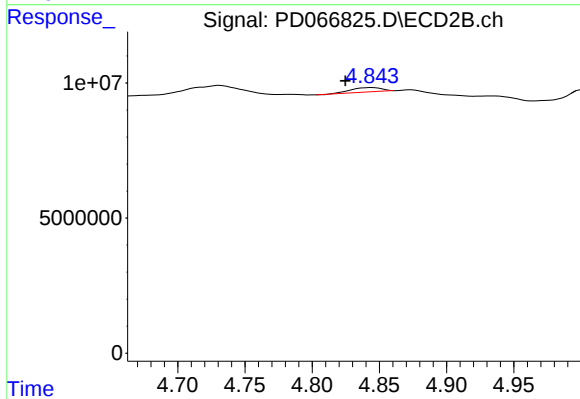

#6 beta-BHC


R.T.: 4.845 min
Delta R.T.: 0.020 min
Response: 2613724
Conc: 0.56 ng/ml

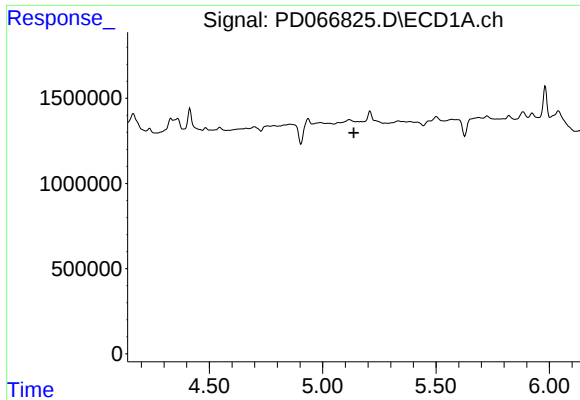

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.138 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

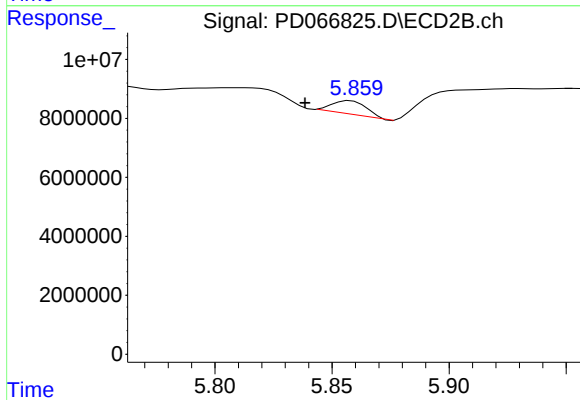


#8 Heptachlor epoxide

R.T.: 5.858 min
Delta R.T.: 0.019 min
Response: 4665170
Conc: 0.64 ng/ml

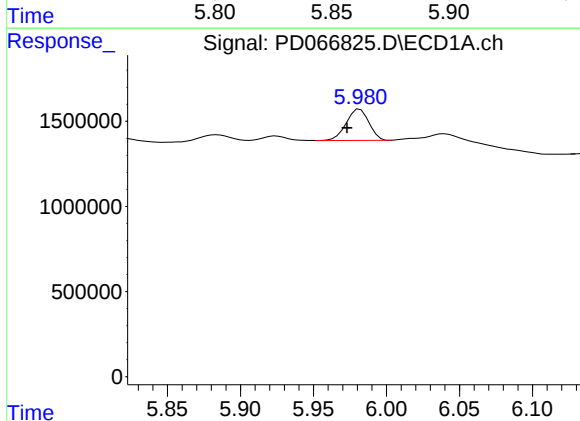


#14 Endrin

R.T.: 5.982 min
Delta R.T.: 0.009 min
Response: 1985349
Conc: 0.95 ng/ml

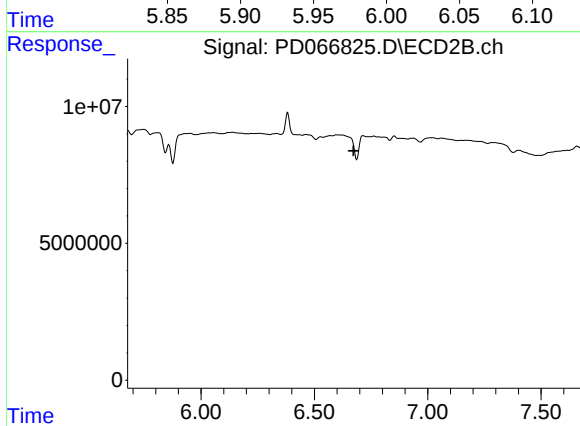

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.673 min
Response: 0
Conc: N.D.

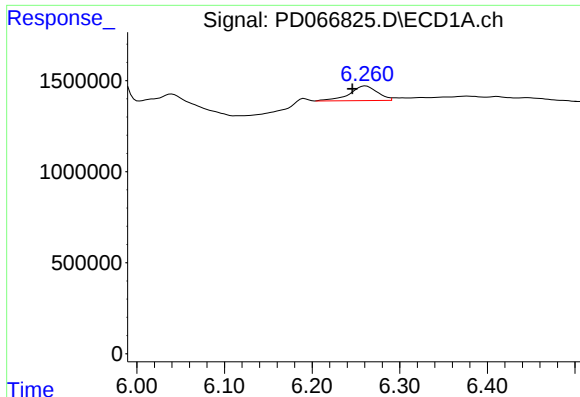

#15 Endosulfan II


R.T.: 6.261 min
Delta R.T.: 0.015 min
Response: 1786441
Conc: 0.90 ng/ml

Instrument :
ECD_D
ClientSampleId :

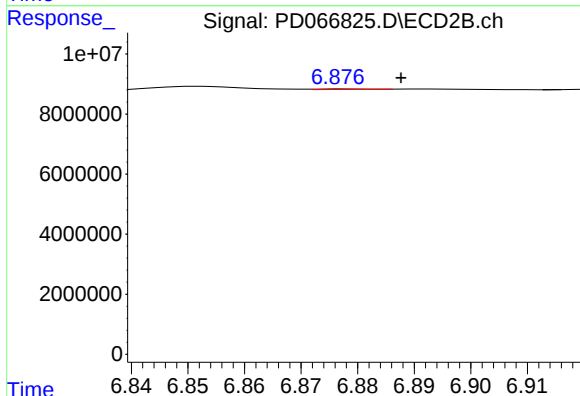


#15 Endosulfan II

R.T.: 6.879 min
Delta R.T.: -0.009 min
Response: 104827
Conc: 0.01 ng/ml

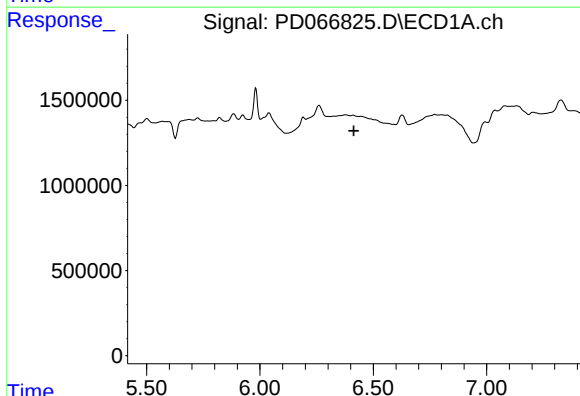


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.414 min
Response: 0
Conc: N.D.

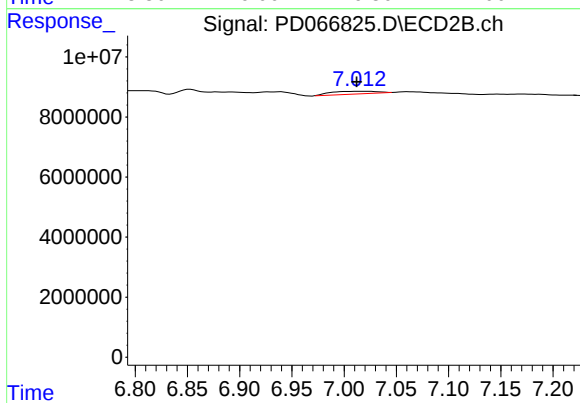

#18 Endrin aldehyde


R.T.: 7.013 min
Delta R.T.: 0.002 min
Response: 2818029
Conc: 0.50 ng/ml

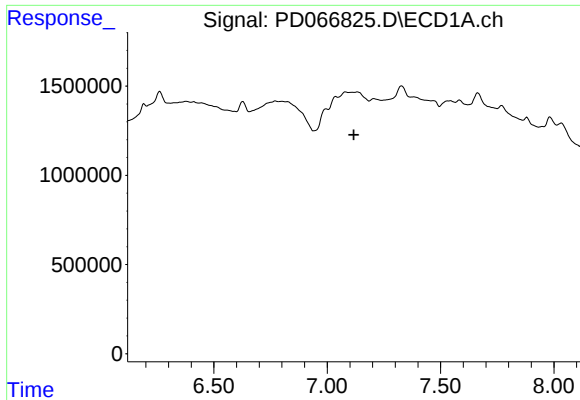

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.118 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

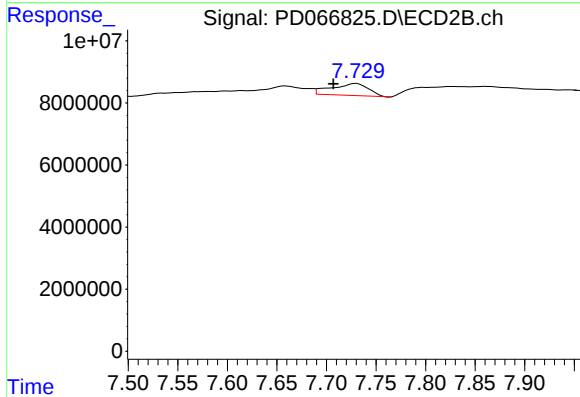


#21 Endrin ketone

R.T.: 7.730 min
Delta R.T.: 0.023 min
Response: 9845597
Conc: 1.17 ng/ml

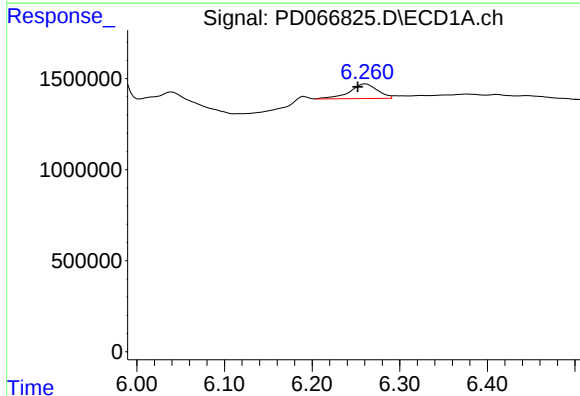


#27 Chlordane-5

R.T.: 6.261 min
Delta R.T.: 0.009 min
Response: 1786441
Conc: 21.12 ng/ml

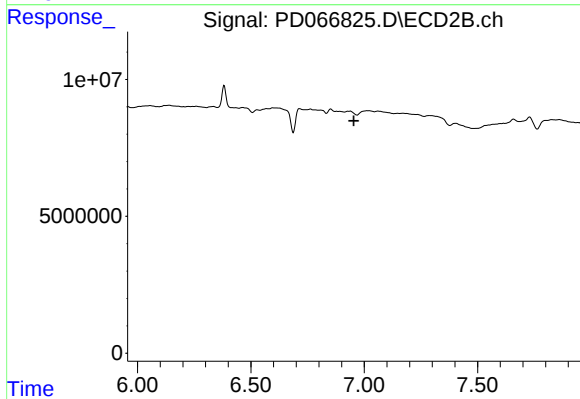

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.955 min
Response: 0
Conc: N.D.

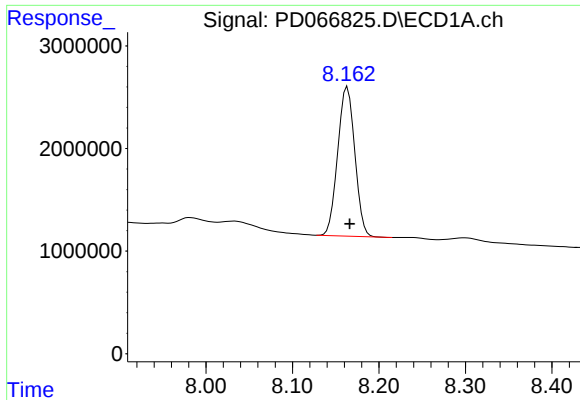

#28 Decachlorobiphenyl

R.T.: 8.164 min
Delta R.T.: -0.003 min
Response: 19847102
Conc: 17.18 ng/ml

Instrument :
ECD_D
ClientSampleId :

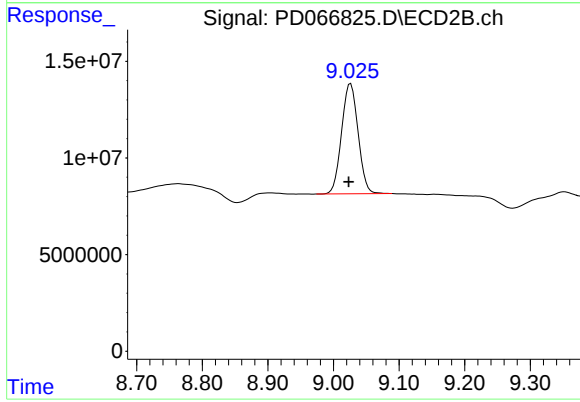

#28 Decachlorobiphenyl

R.T.: 9.026 min
Delta R.T.: 0.003 min
Response: 99806092
Conc: 18.53 ng/ml