

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110921\
 Data File : PD066823.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Nov 2021 17:22
 Operator : AR\AJ
 Sample : M4595-07
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CMC-ICS-001-002

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 10 05:38:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102821.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 28 02:17:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.438	3.969	22909273	110.9E6	12.278	13.707
28) SA Decachlor...	8.163	9.026	15910887	74703615	13.771	13.869

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110921\
Data File : PD066823.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Nov 2021 17:22
Operator : AR\AJ
Sample : M4595-07
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
CMC-ICS-001-002

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 10 05:38:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102821.M
Quant Title : GC Extractables
QLast Update : Thu Oct 28 02:17:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

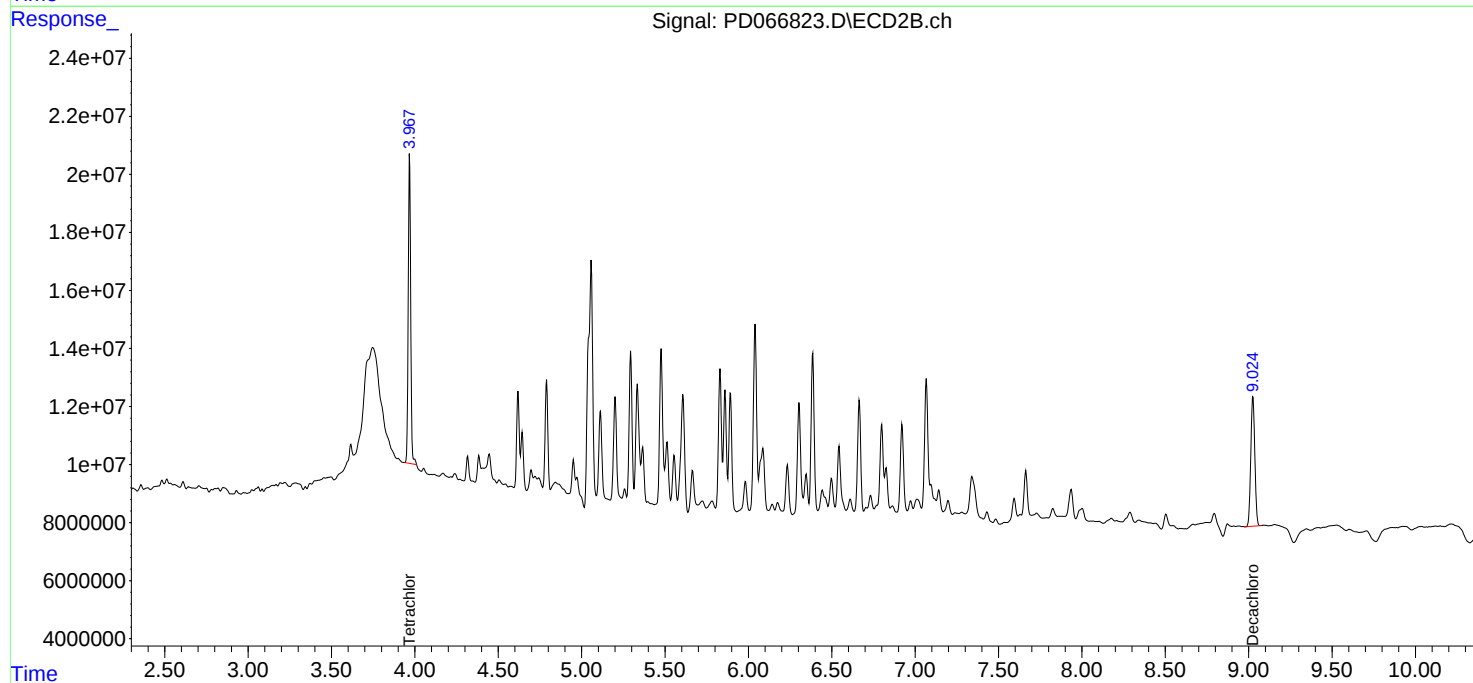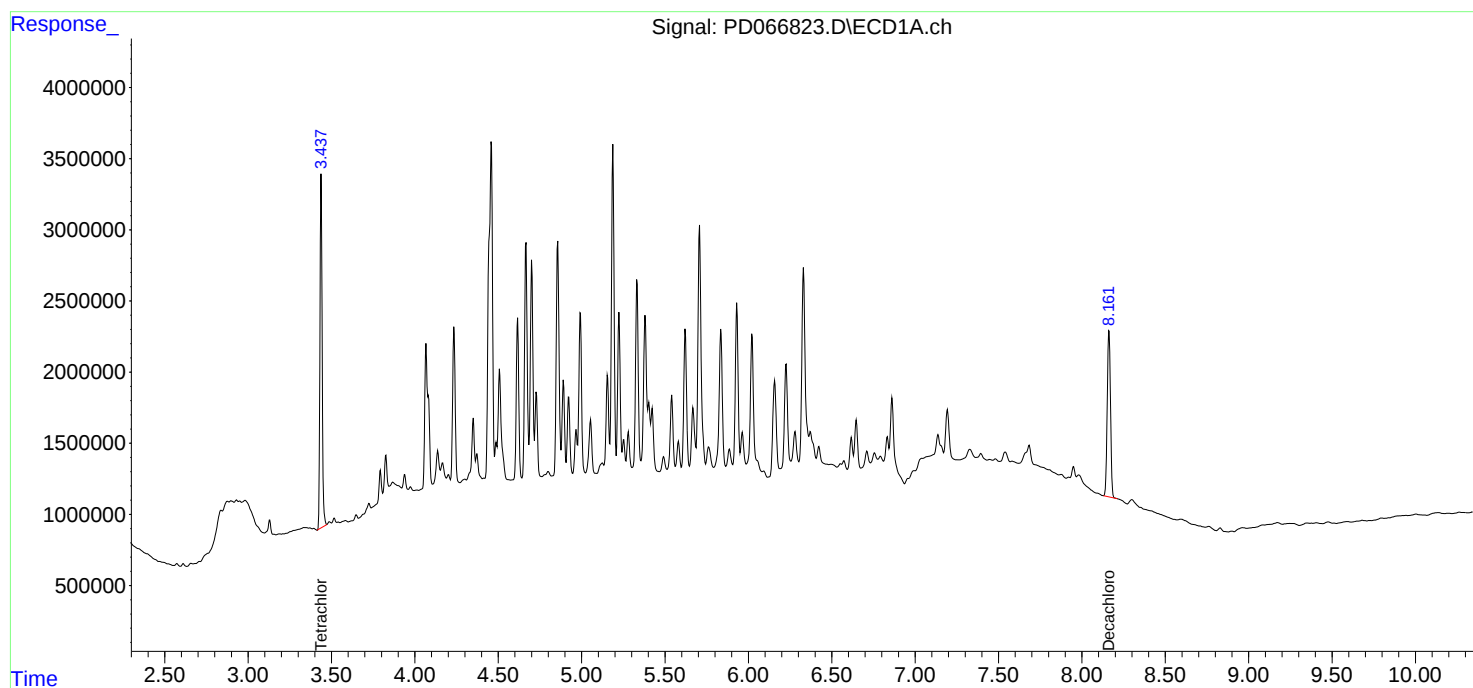


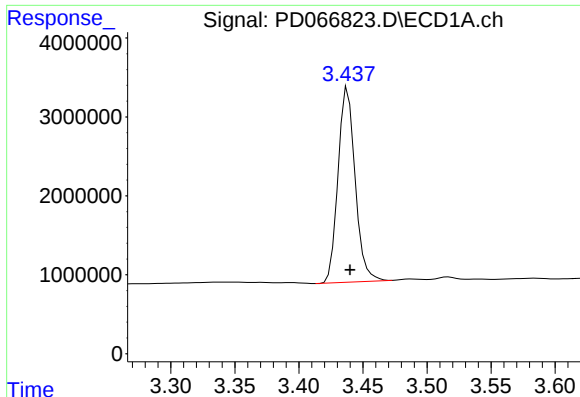

#1 Tetrachloro-m-xylene


R.T.: 3.438 min
Delta R.T.: -0.002 min
Response: 22909273
Conc: 12.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
CMC-ICS-001-002

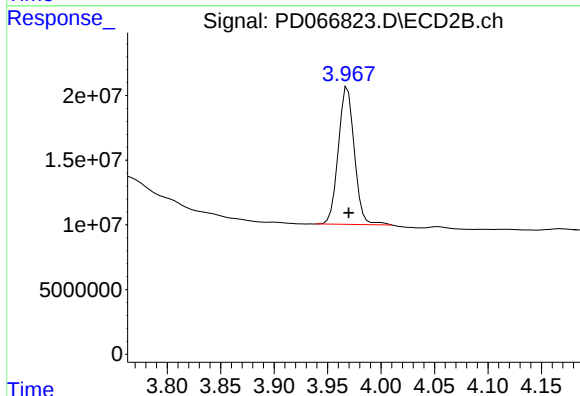


#1 Tetrachloro-m-xylene

R.T.: 3.969 min
Delta R.T.: -0.001 min
Response: 110921543
Conc: 13.71 ng/ml

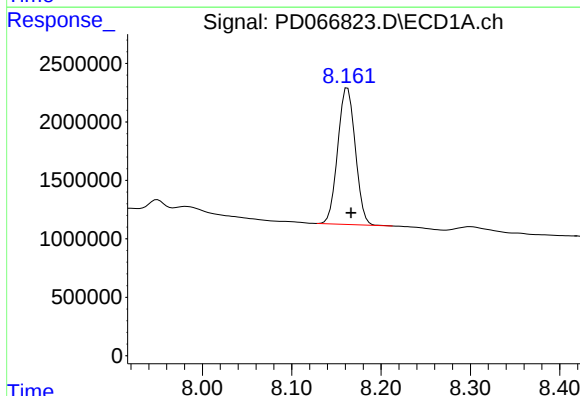

#28 Decachlorobiphenyl

R.T.: 8.163 min
Delta R.T.: -0.004 min
Response: 15910887
Conc: 13.77 ng/ml

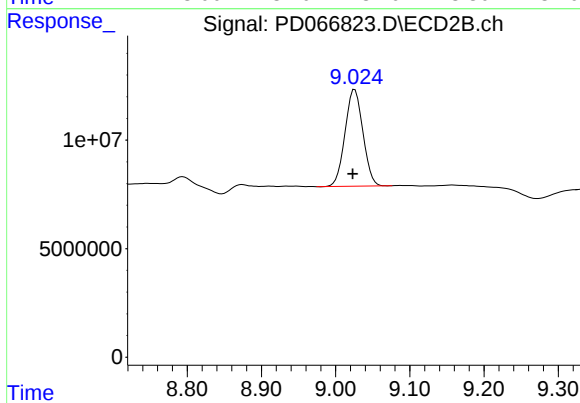

#28 Decachlorobiphenyl

R.T.: 9.026 min
Delta R.T.: 0.003 min
Response: 74703615
Conc: 13.87 ng/ml