

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110923\
 Data File : PD079506.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2023 12:55
 Operator : AR\AJ
 Sample : PIBLK072
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 19:57:42 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 04 07:14:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	2.803	36683330	58522510	25.119	25.586
27)	SA Decachlor...	9.118	7.949	83759661	118.1E6	47.201	49.465
Target Compounds							
2)	A alpha-BHC	0.000	3.294	0	129140	N.D.	<MDL
3)	MA gamma-BHC...	0.000	3.655	0	187662	N.D.	<MDL
4)	MA Heptachlor	0.000	3.942f	0	994047	N.D.	0.298
5)	MB Aldrin	0.000	4.265	0	807220	N.D.	0.248
6)	B beta-BHC	0.000	3.942	0	994047	N.D.	0.607
7)	B delta-BHC	4.793	4.184	4743579	244033	1.904	<MDL #
8)	B Heptachlo...	0.000	4.789	0	722235	N.D.	0.234
9)	A Endosulfan I	0.000	5.096f	0	27170	N.D.	<MDL
10)	B trans-Chl...	6.008	5.022	1559012	148331	0.733	<MDL #
11)	B cis-Chlor...	6.008f	5.096	1559012	27170	0.716	<MDL #
13)	MA Dieldrin	0.000	5.395	0	555927	N.D.	0.175
14)	MA Endrin	0.000	5.687	0	266246	N.D.	<MDL
15)	B Endosulfa...	0.000	5.996	0	275646	N.D.	0.106
18)	B Endrin al...	0.000	6.158	0	138357	N.D.	<MDL
22)	Toxaphene-1	0.000	5.038	0	135272	N.D.	8.090
23)	Toxaphene-2	0.000	5.369	0	612974	N.D.	36.477


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110923\
Data File : PD079506.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2023 12:55
Operator : AR\AJ
Sample : PIBLK072
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 19:57:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 07:14:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

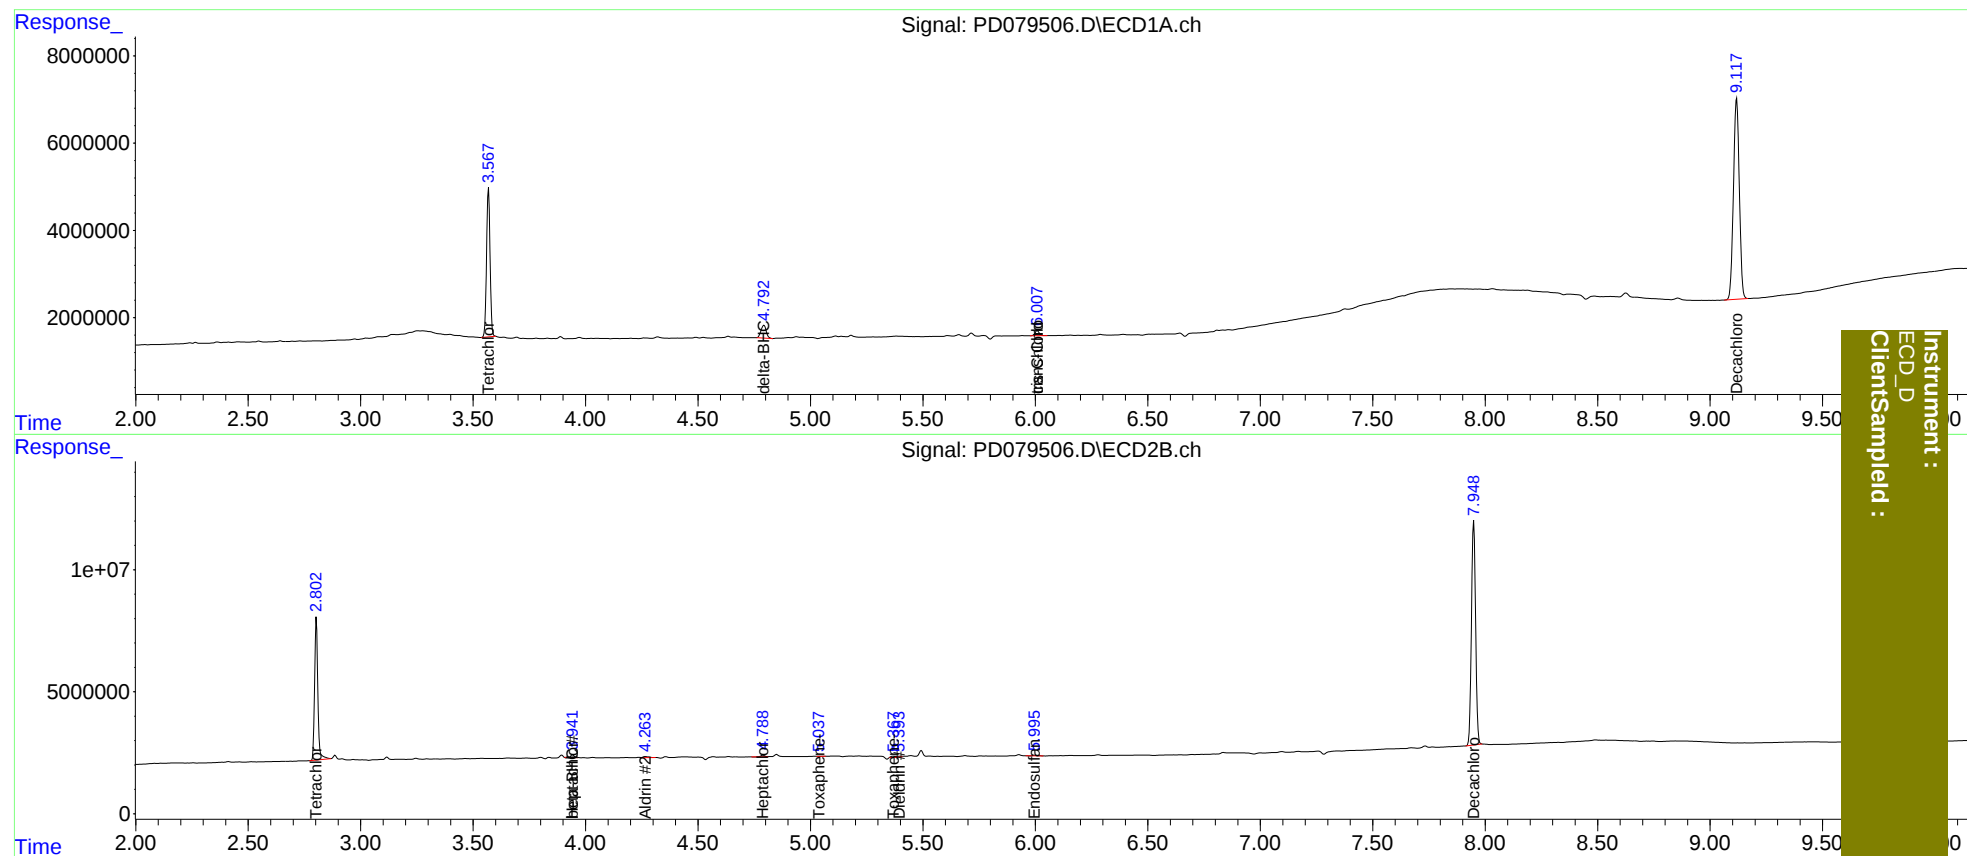


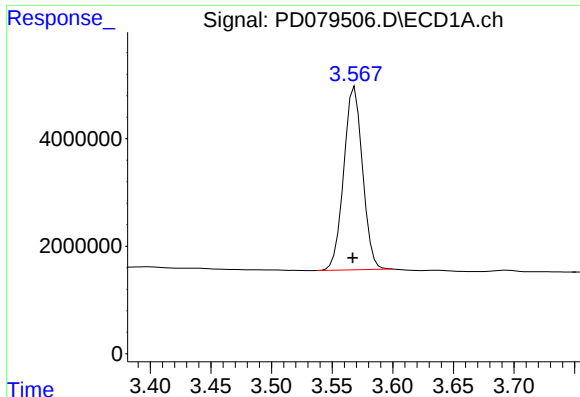

#1 Tetrachloro-m-xylene


R.T.: 3.569 min
Delta R.T.: 0.002 min
Response: 36683330
Conc: 25.12 ng/ml

Instrument :
ECD_D
ClientSampleId :

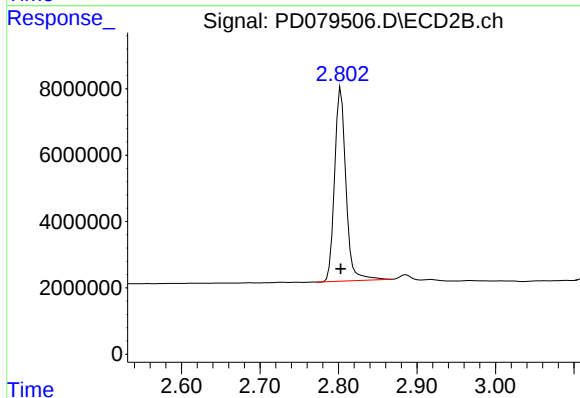


#1 Tetrachloro-m-xylene

R.T.: 2.803 min
Delta R.T.: 0.000 min
Response: 58522510
Conc: 25.59 ng/ml

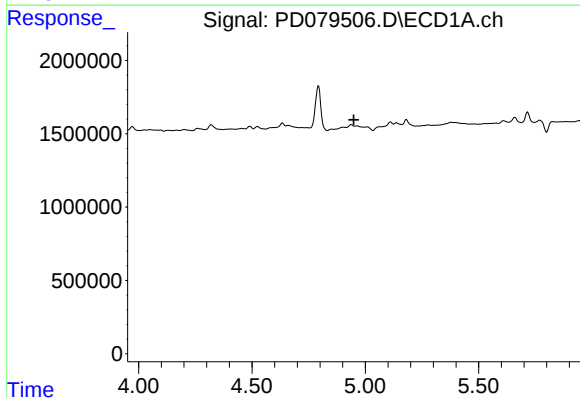


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.950 min
Response: 0
Conc: N.D.

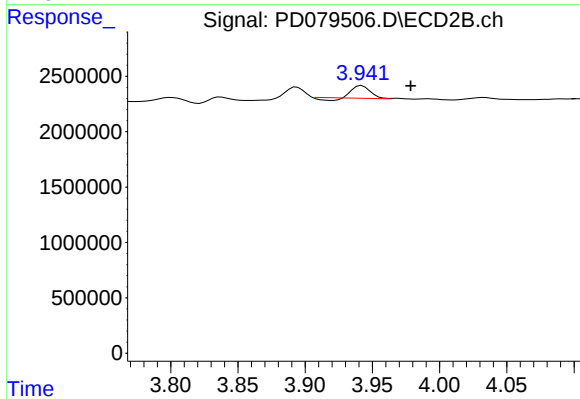

#4 Heptachlor


R.T.: 3.942 min
Delta R.T.: -0.036 min
Response: 994047
Conc: 0.30 ng/ml

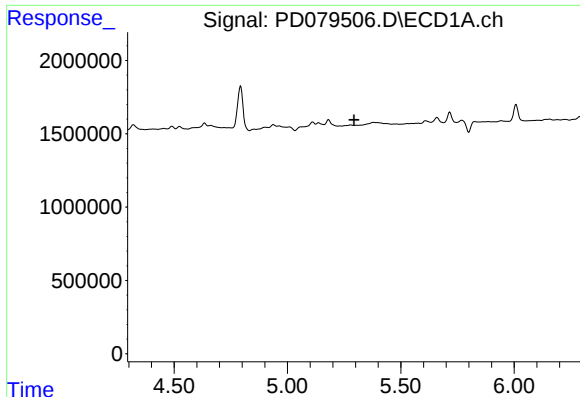

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.294 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

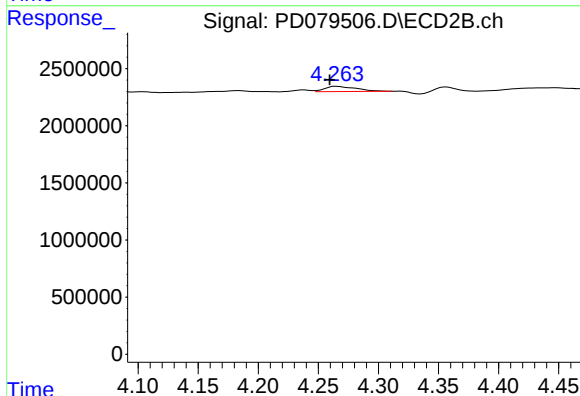


#5 Aldrin

R.T.: 4.265 min
Delta R.T.: 0.005 min
Response: 807220
Conc: 0.25 ng/ml

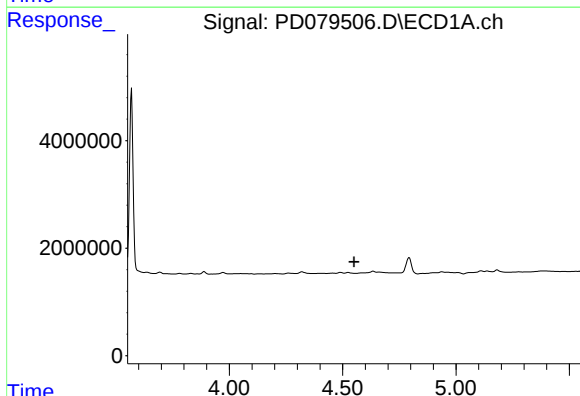


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.551 min
Response: 0
Conc: N.D.

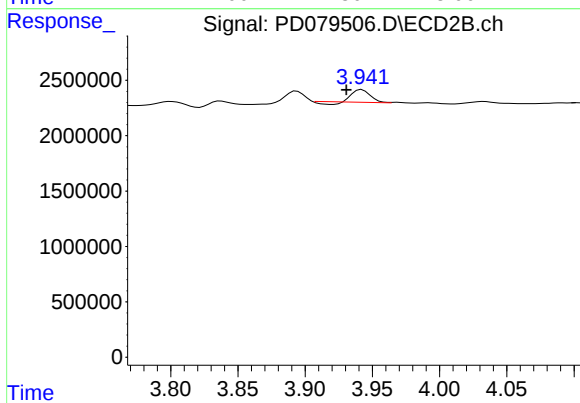

#6 beta-BHC


R.T.: 3.942 min
Delta R.T.: 0.011 min
Response: 994047
Conc: 0.61 ng/ml

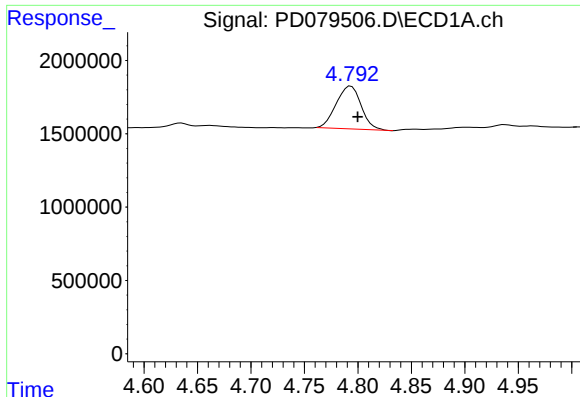

#7 delta-BHC


R.T.: 4.793 min
Delta R.T.: -0.006 min
Response: 4743579
Conc: 1.90 ng/ml

Instrument :
ECD_D
ClientSampleId :

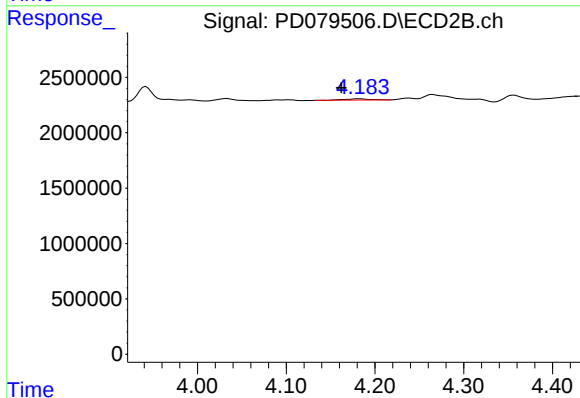


#7 delta-BHC

R.T.: 4.184 min
Delta R.T.: 0.022 min
Response: 244033
Conc: N.D.

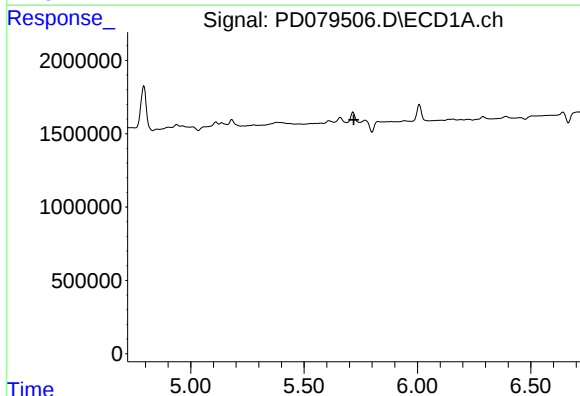


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.720 min
Response: 0
Conc: N.D.

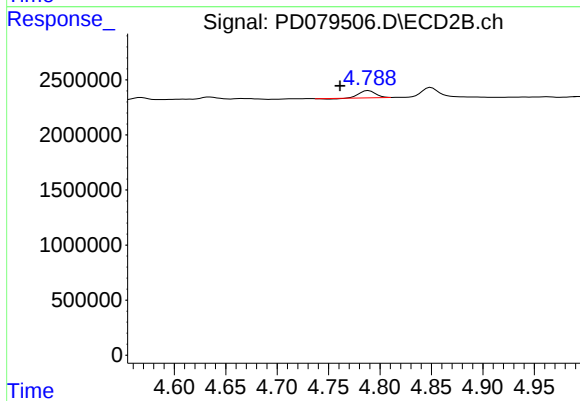

#8 Heptachlor epoxide


R.T.: 4.789 min
Delta R.T.: 0.028 min
Response: 722235
Conc: 0.23 ng/ml

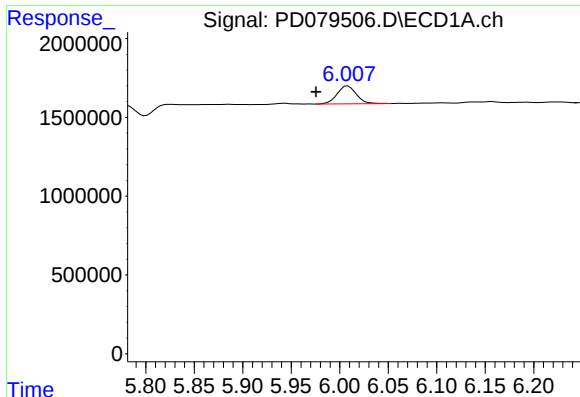

#10 trans-Chlordane


R.T.: 6.008 min
Delta R.T.: 0.033 min
Response: 1559012
Conc: 0.73 ng/ml

Instrument :
ECD_D
ClientSampleId :

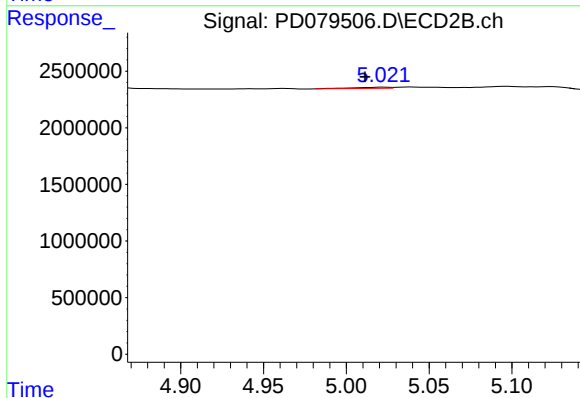


#10 trans-Chlordane

R.T.: 5.022 min
Delta R.T.: 0.011 min
Response: 148331
Conc: N.D.

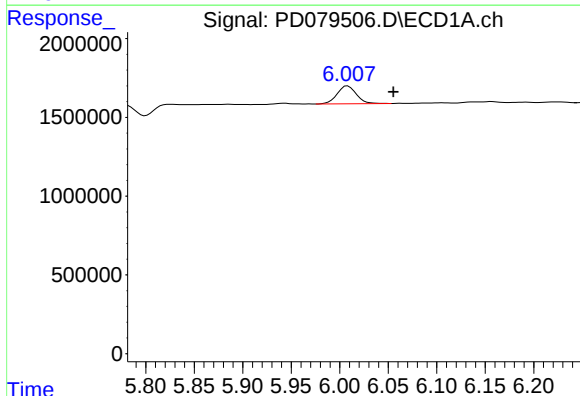


#11 cis-Chlordane

R.T.: 6.008 min
Delta R.T.: -0.047 min
Response: 1559012
Conc: 0.72 ng/ml

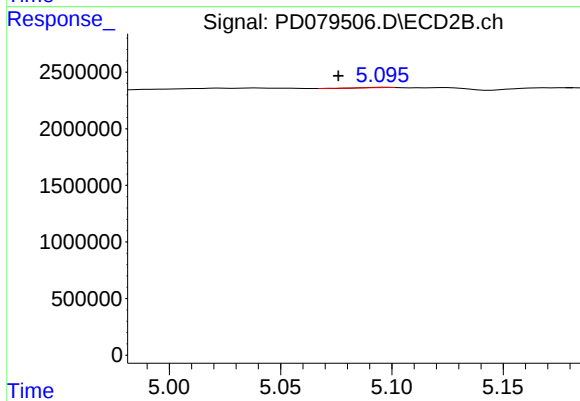

#11 cis-Chlordane


R.T.: 5.096 min
Delta R.T.: 0.020 min
Response: 27170
Conc: N.D.

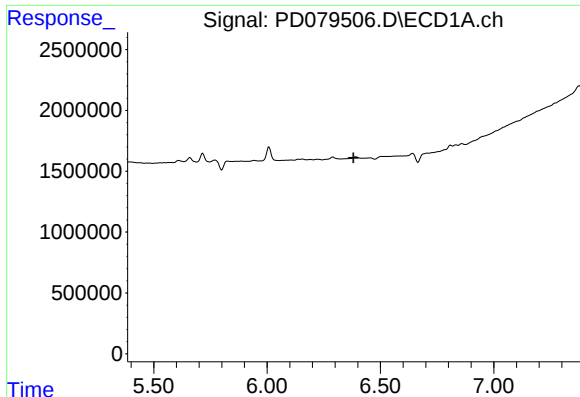

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

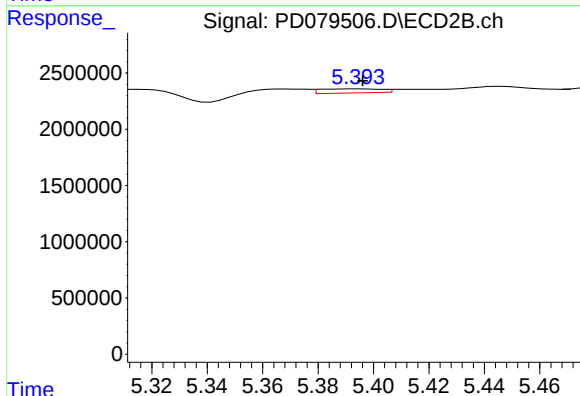


#13 Dieldrin

R.T.: 5.395 min
Delta R.T.: -0.001 min
Response: 555927
Conc: 0.17 ng/ml

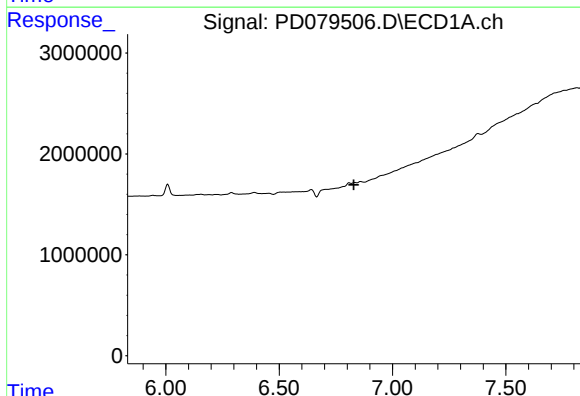


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.830 min
Response: 0
Conc: N.D.

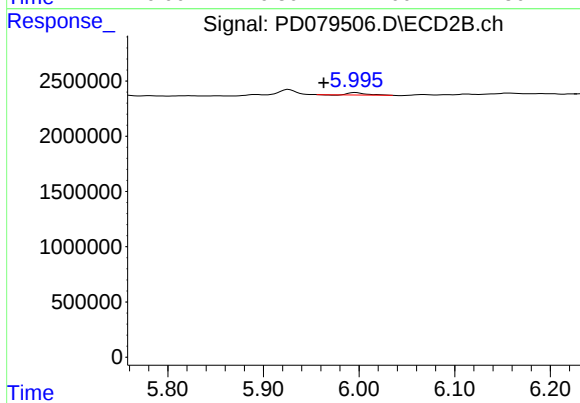

#15 Endosulfan II


R.T.: 5.996 min
Delta R.T.: 0.033 min
Response: 275646
Conc: 0.11 ng/ml

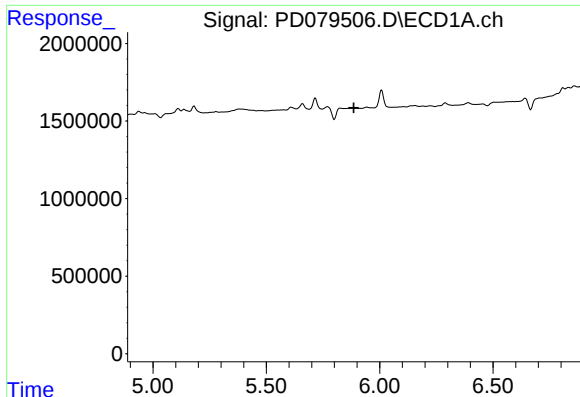

#22 Toxaphene-1


R.T.: 0.000 min
Exp R.T.: 5.886 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

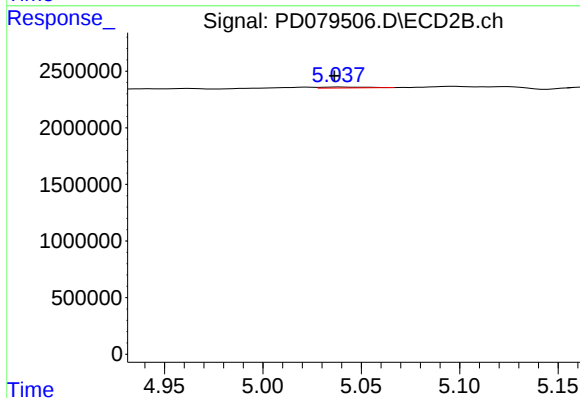


#22 Toxaphene-1

R.T.: 5.038 min
Delta R.T.: 0.002 min
Response: 135272
Conc: 8.09 ng/ml

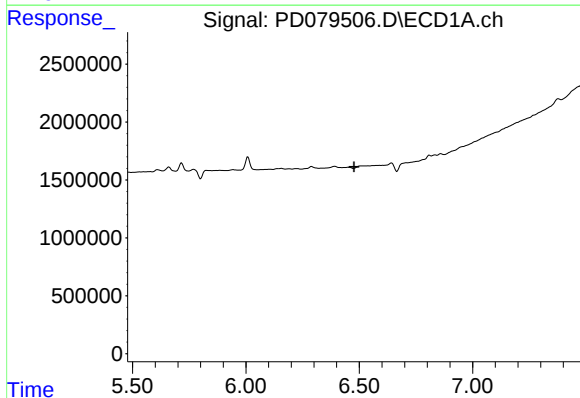


#23 Toxaphene-2

R.T.: 0.000 min
Exp R.T.: 6.477 min
Response: 0
Conc: N.D.

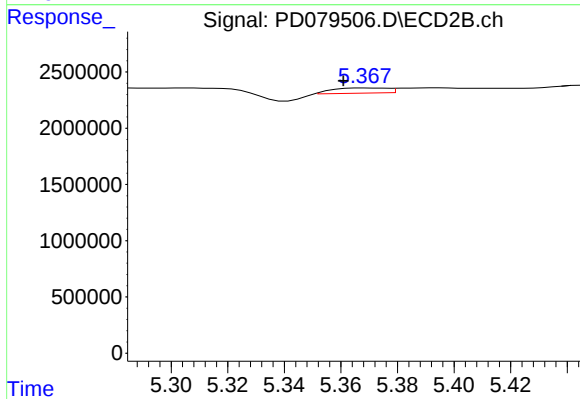

#23 Toxaphene-2


R.T.: 5.369 min
Delta R.T.: 0.008 min
Response: 612974
Conc: 36.48 ng/ml

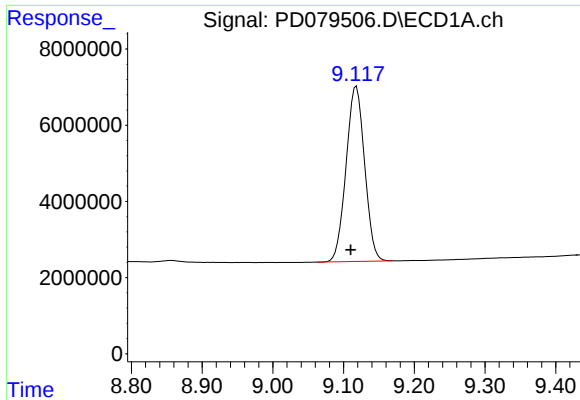

#27 Decachlorobiphenyl

R.T.: 9.118 min
Delta R.T.: 0.008 min
Response: 83759661
Conc: 47.20 ng/ml

Instrument :
ECD_D
ClientSampleId :

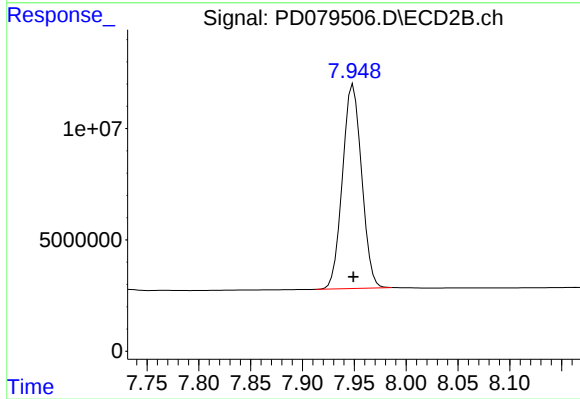

#27 Decachlorobiphenyl

R.T.: 7.949 min
Delta R.T.: 0.000 min
Response: 118095572
Conc: 49.46 ng/ml