

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111020\
 Data File : PD060079.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Nov 2020 10:00
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 11 03:19:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 04 04:05:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

3) MA	gamma-BHC...	4.246	0.000	1193476	0	0.976	N.D.	#
4) MA	Heptachlor	4.577f	0.000	214284	0	0.183	N.D.	#
6) B	beta-BHC	4.502	0.000	723083	0	1.365	N.D.	#
19) B	Endosulfa...	6.812f	0.000	18345284	0	20.992	N.D.	#
20) A	Methoxychlor	0.000	7.675f	0	5122021	N.D.	3.644	
26)	Toxaphene-5	7.144	7.675	1281115	5122021	75.746	150.647	#


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111020\
Data File : PD060079.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Nov 2020 10:00
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 11 03:19:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 04 04:05:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

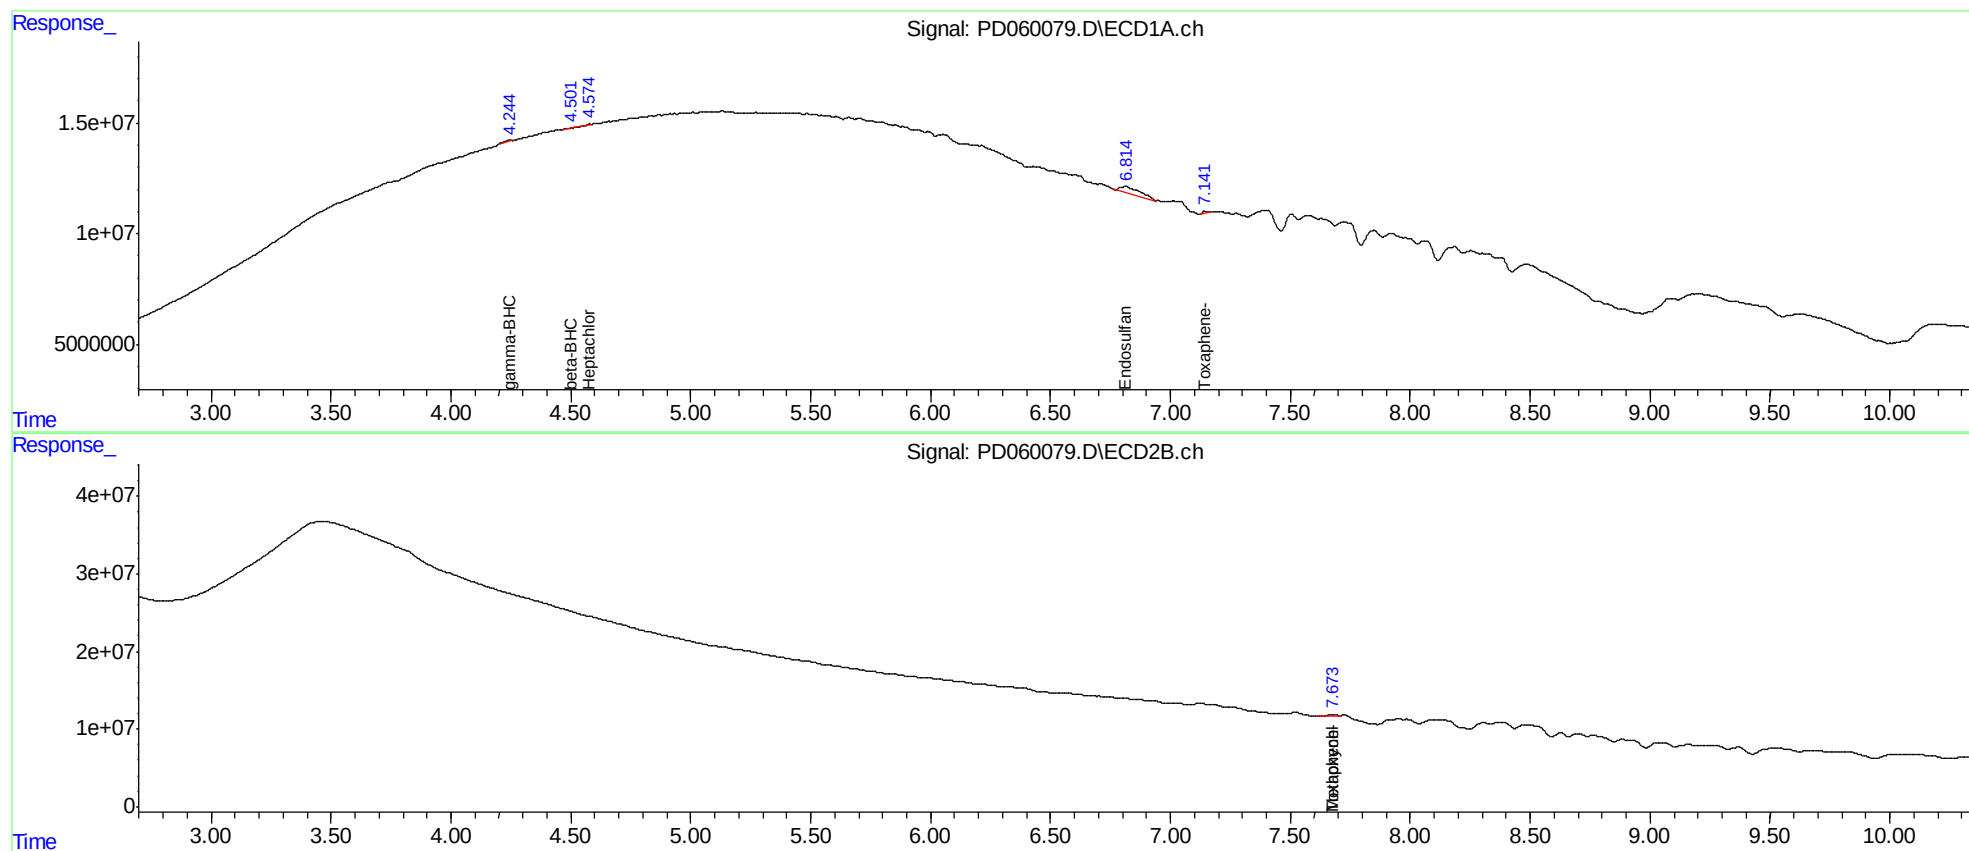


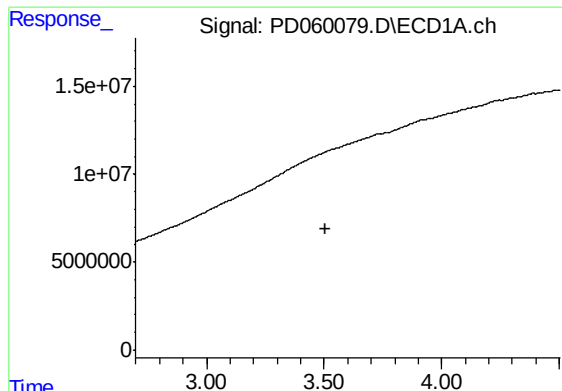

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.506 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

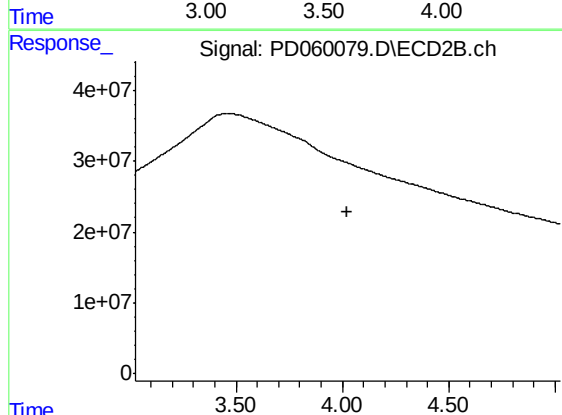


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.024 min
Response: 0
Conc: N.D.

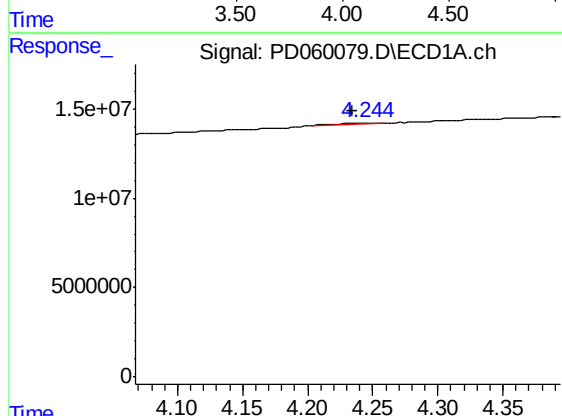


#3 gamma-BHC (Lindane)

R.T.: 4.246 min
Delta R.T.: 0.012 min
Response: 1193476
Conc: 0.98 ng/ml

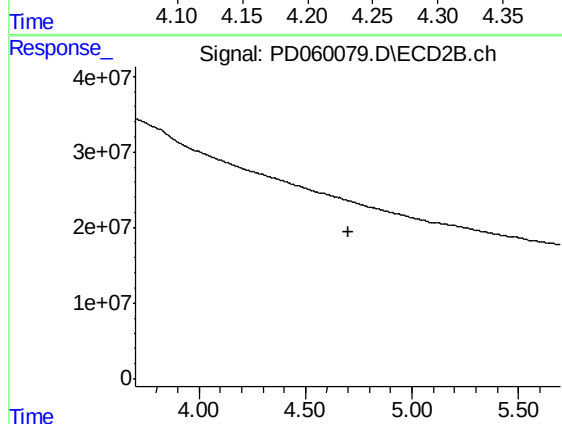

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.701 min
Response: 0
Conc: N.D.

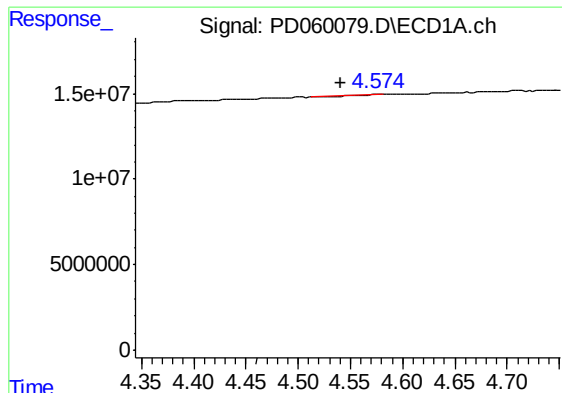

#4 Heptachlor


R.T.: 4.577 min
Delta R.T.: 0.035 min
Response: 214284
Conc: 0.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

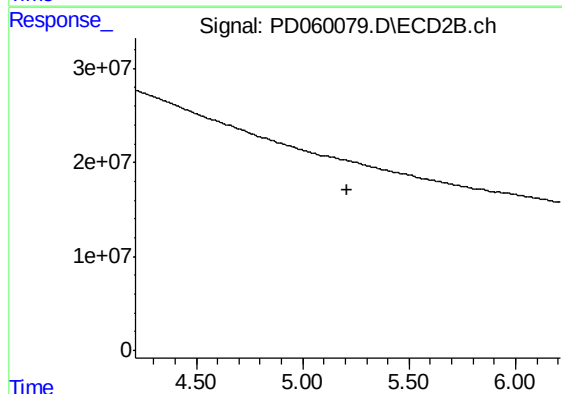


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 5.213 min
Response: 0
Conc: N.D.

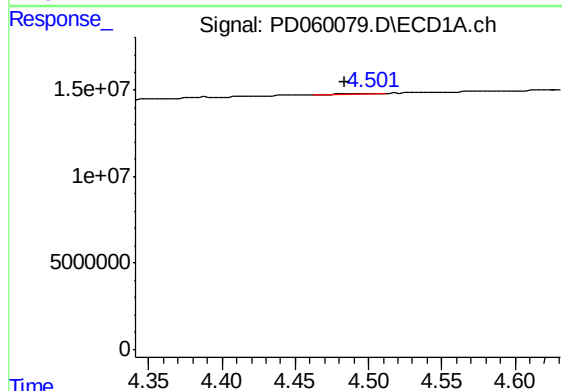


#6 beta-BHC

R.T.: 4.502 min
Delta R.T.: 0.019 min
Response: 723083
Conc: 1.36 ng/ml

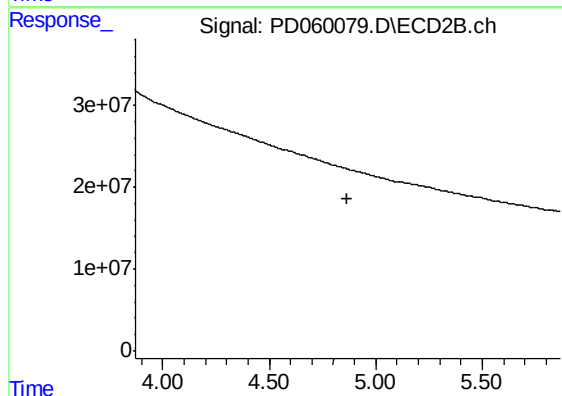

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.868 min
Response: 0
Conc: N.D.

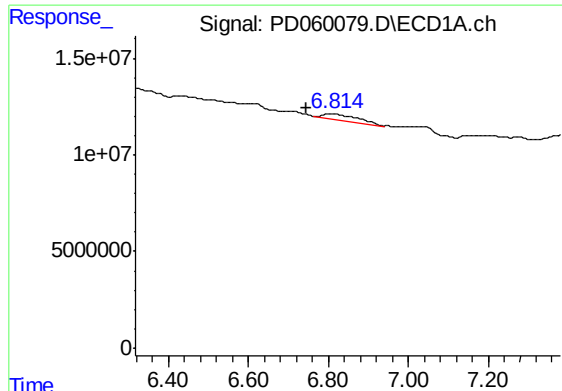

#19 Endosulfan Sulfate


R.T.: 6.812 min
Delta R.T.: 0.068 min
Response: 18345284
Conc: 20.99 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

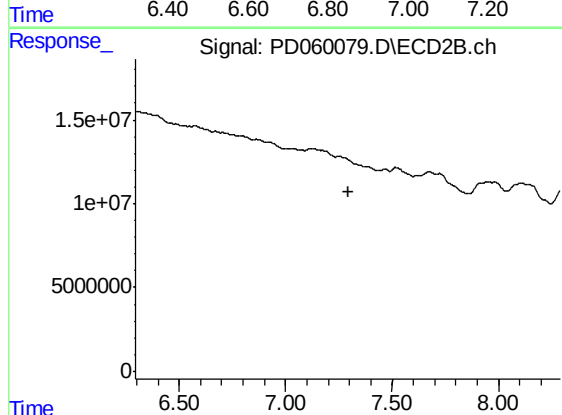


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.294 min
Response: 0
Conc: N.D.

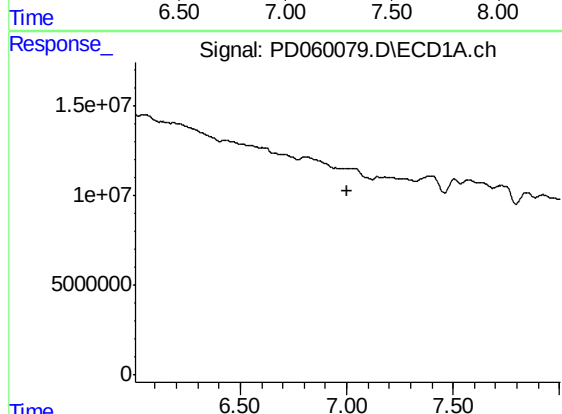


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.005 min
Response: 0
Conc: N.D.

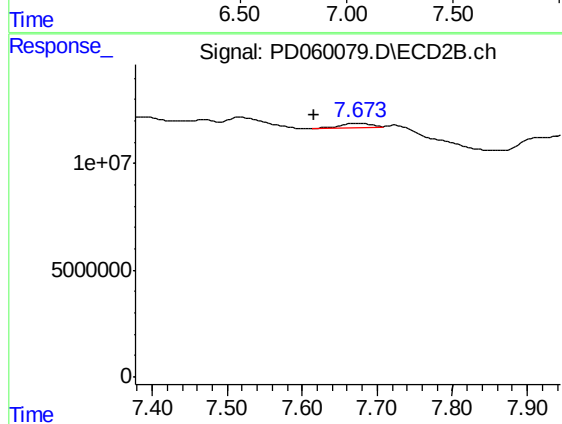

#20 Methoxychlor


R.T.: 7.675 min
Delta R.T.: 0.059 min
Response: 5122021
Conc: 3.64 ng/ml

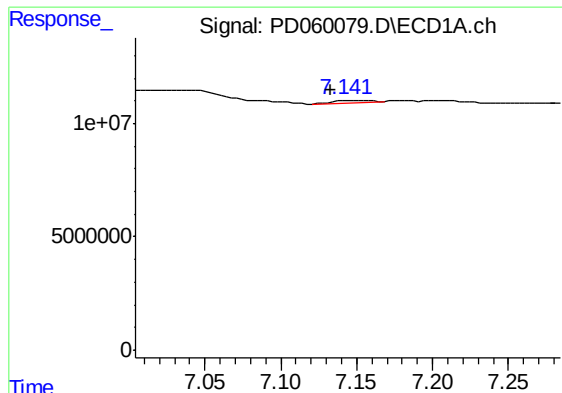

#26 Toxaphene-5


R.T.: 7.144 min
Delta R.T.: 0.011 min
Response: 1281115
Conc: 75.75 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

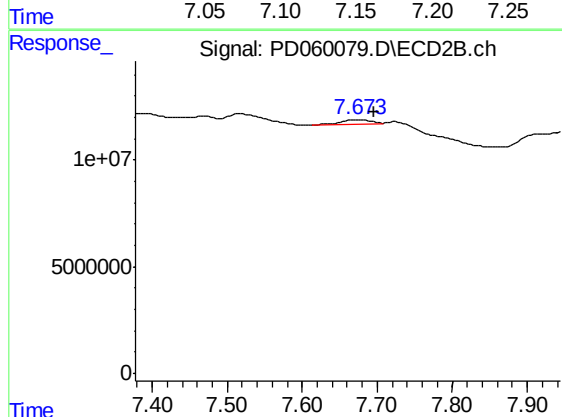


#26 Toxaphene-5

R.T.: 7.675 min
Delta R.T.: -0.021 min
Response: 5122021
Conc: 150.65 ng/ml

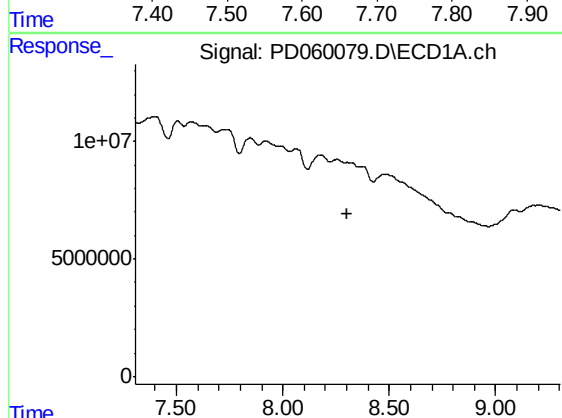

#27 Decachlorobiphenyl

R.T.: 8.253 min
Delta R.T.: -0.052 min
Response: -374996
Conc: N.D.

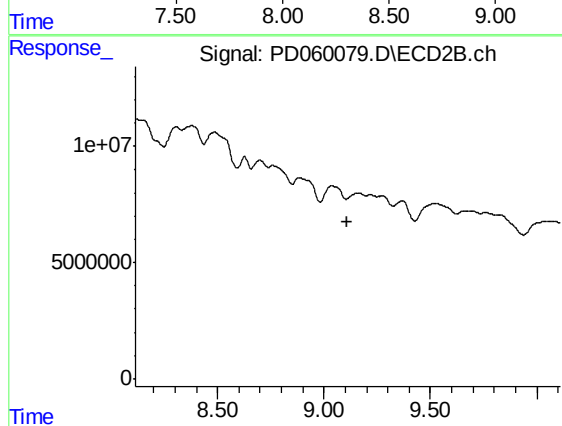

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.112 min
Response: 0
Conc: N.D.