

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111021\
 Data File : PD066849.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Nov 2021 17:56
 Operator : AR\AJ
 Sample : M4419-08MSD
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0HF5MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/11/2021
 Supervised By : mohammad ahmed 11/11/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 11 02:09:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 27 16:50:52 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.431	3.970	292.5E6	86858933	151.306	10.029 #
27)	SA Decachlor...	8.163	9.024	19695491	114.6E6	16.810	21.974 #
Target Compounds							
2)	A alpha-BHC	3.875	4.362	4881.5E6	11489.5E6	1667.713	1050.791 #
3)	MA gamma-BHC...	4.156	4.647	868.7E6	2180.0E6	313.766	215.725 #
4)	MA Heptachlor	4.451	5.123	118.4E6	1896.3E6	41.611	193.470m#
5)	MB Aldrin	4.691	5.451	1082.2E6	293.2E6	375.866	31.119 #
6)	B beta-BHC	4.405	4.824	297.8E6	1036.6E6	237.125	210.386
7)	B delta-BHC	4.608	5.040	9578.7E6	16536.2E6	3613.822	1671.496 #
9)	A Endosulfan I	5.472	6.194	229.6E6	277.4E6	100.148	35.456m#
10)	B trans-Chl...	5.359	6.070	291.5E6	549.1E6	112.776m	63.763m#
11)	B cis-Chlor...	5.417	6.143	212.8E6	474.2E6	83.527m	55.265 #
12)	B 4,4'-DDE	5.582	6.302	312.5E6	840.6E6	136.811	110.392m
13)	MA Dieldrin	5.714	6.452	295.7E6	683.4E6	118.495m	85.666m#
14)	MA Endrin	5.970	6.673	587.4E6	486.1E6	277.634	71.634 #
15)	B Endosulfa...	6.243	6.886	187.7E6	586.1E6	90.416	81.734
16)	A 4,4'-DDD	6.096	6.798	745.5E6	2091.9E6	411.855	324.022
17)	MA 4,4'-DDT	6.335	7.096	2233.4E6	7126.4E6	1181.237	1078.750
18)	B Endrin al...	6.413	7.012	126.8E6	431.6E6	87.010	81.121
19)	B Endosulfa...	6.623	7.234	119.5E6	439.8E6	65.519	63.823
20)	A Methoxychlor	6.882	7.557	308.7E6	1247.2E6	329.403	385.925
21)	B Endrin ke...	7.116	7.708	167.9E6	597.0E6	81.465	76.167

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111021\
Data File : PD066849.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Nov 2021 17:56
Operator : AR\AJ
Sample : M4419-08MSD
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 11 02:09:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 27 16:50:52 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

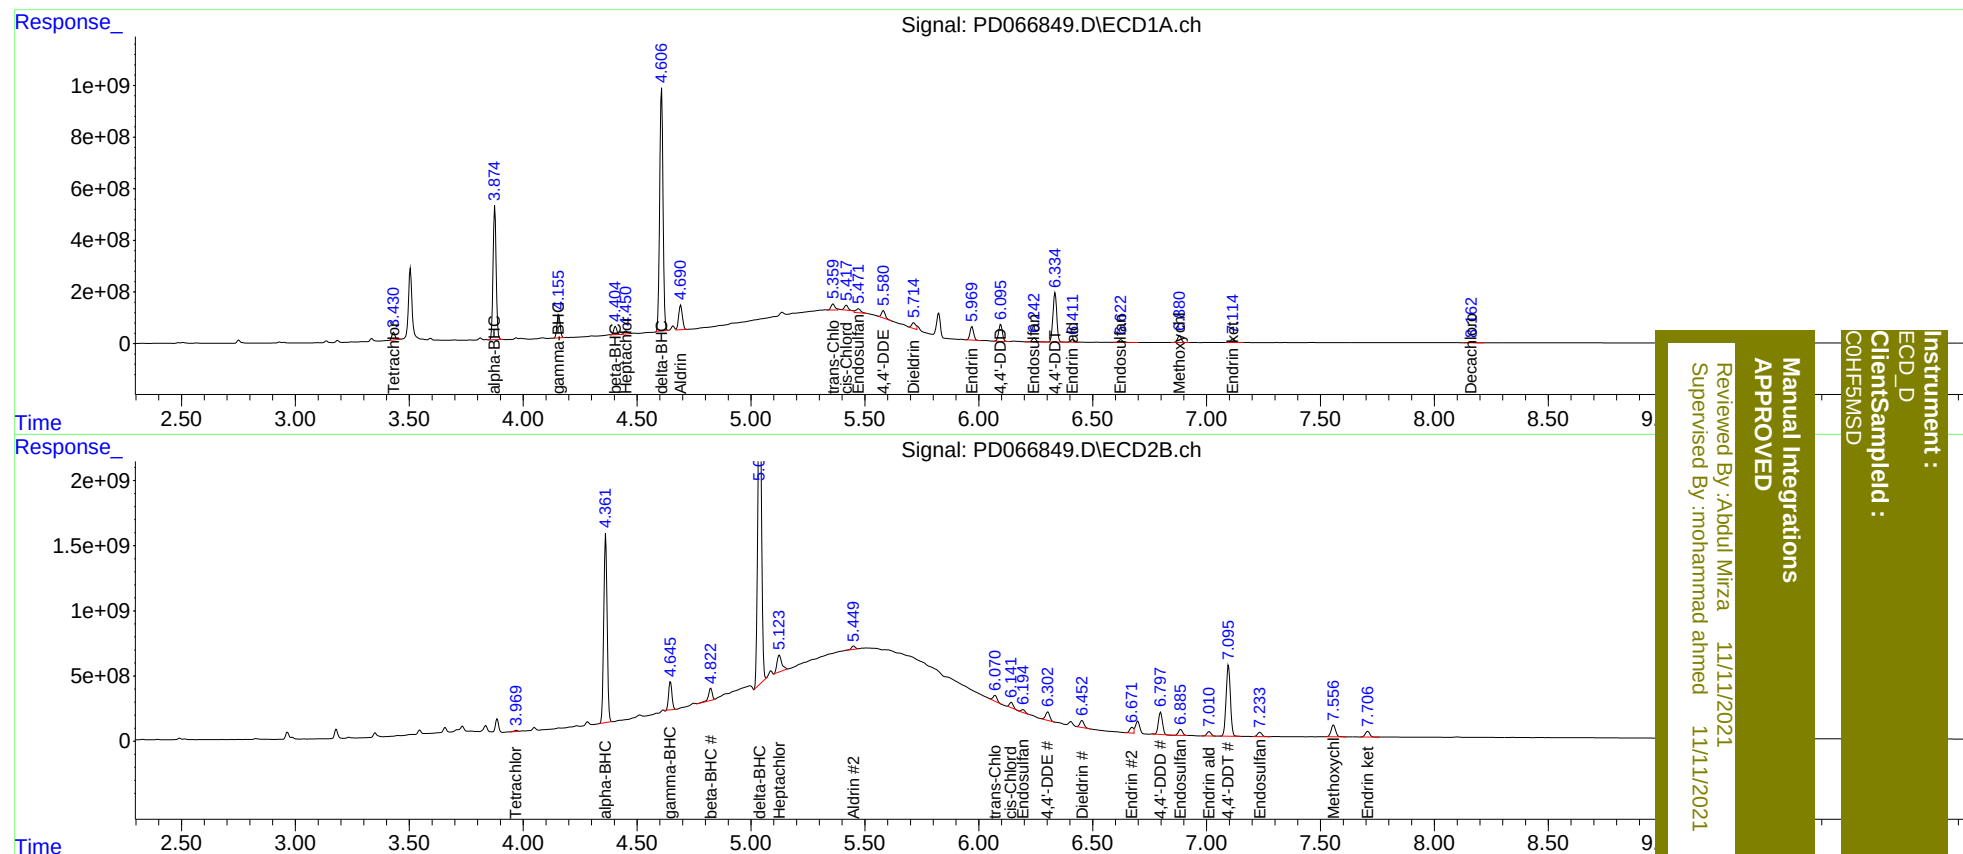

Instrument :
ECD_D
ClientSampled :
COHFSMSD

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 11/11/2021
Supervised By: mohammad ahmed 11/11/2021