

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111021\
 Data File : PD066842.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Nov 2021 16:20
 Operator : AR\AJ
 Sample : M4419-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 COHF0

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/11/2021
 Supervised By :mohammad ahmed 11/11/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 11 02:08:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 27 16:50:52 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.435	3.966	58449761	97821908	30.237	11.295m#
27)	SA Decachlor...	8.163	9.026	26764457	130.6E6	22.843	25.037
Target Compounds							
2)	A alpha-BHC	3.876	4.362	3024.8E6	8326.0E6	1033.412	761.472 #
5)	MB Aldrin	4.696	5.449	107.0E6	59084510	37.160	6.271 #
6)	B beta-BHC	4.405	4.824	402.3E6	1092.4E6	320.284	221.709 #
7)	B delta-BHC	4.607	5.038	638.1E6	1698.5E6	240.752	171.685 #
9)	A Endosulfan I	5.475	6.207	165.9E6	308.1E6	72.393	39.373 #
10)	B trans-Chl...	5.359	6.073	489.4E6	908.6E6	189.329m	105.517 #
11)	B cis-Chlor...	5.419	6.144	322.4E6	793.9E6	126.559	92.516 #
12)	B 4,4'-DDE	5.582	6.303	785.2E6	2014.4E6	343.803	264.528
16)	A 4,4'-DDD	6.100	6.799	12359.9E6	25596.0E6	6828.302	3964.739 #
17)	MA 4,4'-DDT	6.336	7.097	8895.0E6	16342.5E6	4704.473	2473.842 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111021\
Data File : PD066842.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Nov 2021 16:20
Operator : AR\AJ
Sample : M4419-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 11 02:08:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 27 16:50:52 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

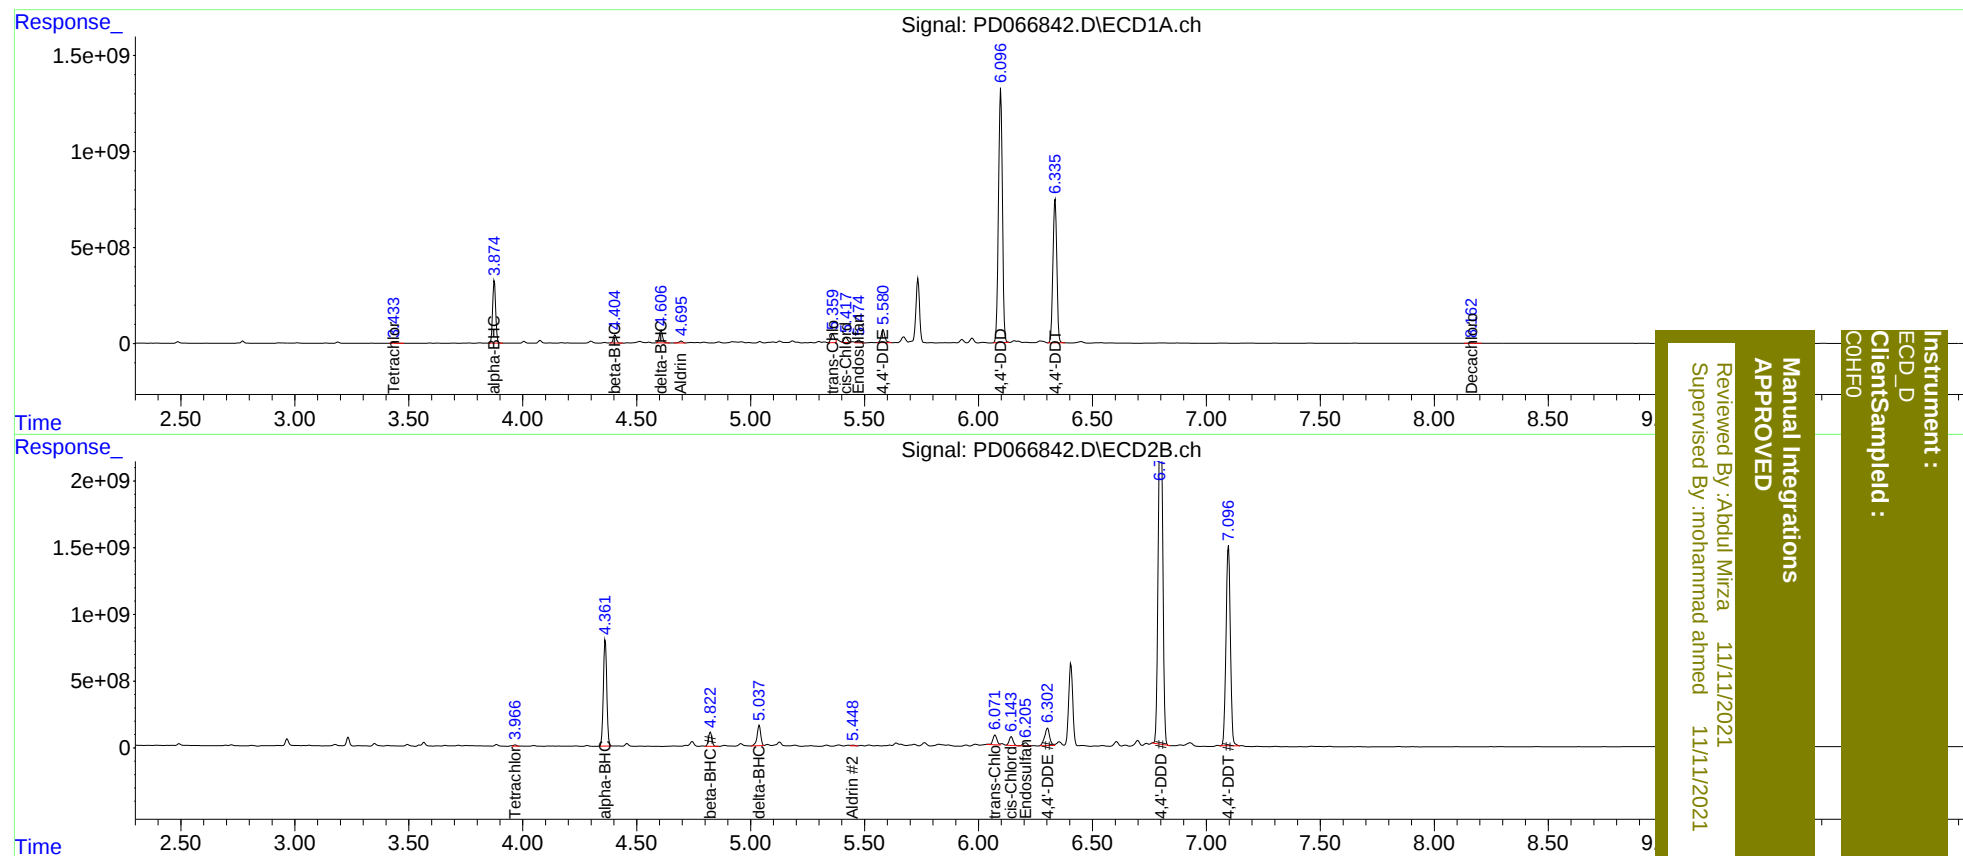

Reviewed By: Abdul Mirza 11/11/2021
Supervised By: mohammad ahmed 11/11/2021

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
COHF0