

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111021\
 Data File : PD066848.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Nov 2021 17:42
 Operator : AR\AJ
 Sample : M4419-07MS
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 COHF5MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/11/2021
 Supervised By :mohammad ahmed 11/11/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 11 02:09:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 27 16:50:52 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.431	3.970	309.7E6	92270021	160.217	10.654 #
27)	SA Decachlor...	8.163	9.023	20678741	118.0E6	17.649	22.623 #
Target Compounds							
2)	A alpha-BHC	3.875	4.363	4721.7E6	10908.6E6	1613.126	997.661 #
3)	MA gamma-BHC...	4.157	4.647	866.3E6	2192.3E6	312.899	216.940 #
4)	MA Heptachlor	4.451	5.123	125.5E6	1881.2E6	44.113	191.926m#
5)	MB Aldrin	4.691	5.451	1166.0E6	291.7E6	404.946	30.961 #
6)	B beta-BHC	4.405	4.823	301.2E6	1098.9E6	239.801	223.028
7)	B delta-BHC	4.607	5.040	10370.3E6	16898.1E6	3912.457	1708.070 #
9)	A Endosulfan I	5.472	6.196	245.2E6	267.9E6	106.966	34.242m#
10)	B trans-Chl...	5.359	6.070	304.1E6	613.4E6	117.645m	71.237m#
11)	B cis-Chlor...	5.417	6.143	222.3E6	543.4E6	87.277m	63.321m#
12)	B 4,4'-DDE	5.582	6.301	317.5E6	847.0E6	139.011	111.224m
13)	MA Dieldrin	5.713	6.452	244.1E6	679.9E6	97.815m	85.224m
14)	MA Endrin	5.970	6.673	585.6E6	506.3E6	276.784	74.609 #
15)	B Endosulfa...	6.243	6.885	188.6E6	578.6E6	90.841	80.685
16)	A 4,4'-DDD	6.096	6.797	792.7E6	2258.2E6	437.940	349.784m
17)	MA 4,4'-DDT	6.334	7.095	2113.1E6	6602.0E6	1117.612	999.373
18)	B Endrin al...	6.412	7.011	128.5E6	430.5E6	88.204	80.918
19)	B Endosulfa...	6.624	7.234	118.0E6	436.7E6	64.705	63.374
20)	A Methoxychlor	6.881	7.557	323.1E6	1202.2E6	344.724	371.990
21)	B Endrin ke...	7.115	7.707	169.4E6	594.6E6	82.228	75.855

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111021\
Data File : PD066848.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Nov 2021 17:42
Operator : AR\AJ
Sample : M4419-07MS
Misc :
ALS Vial : 21 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 11 02:09:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 27 16:50:52 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

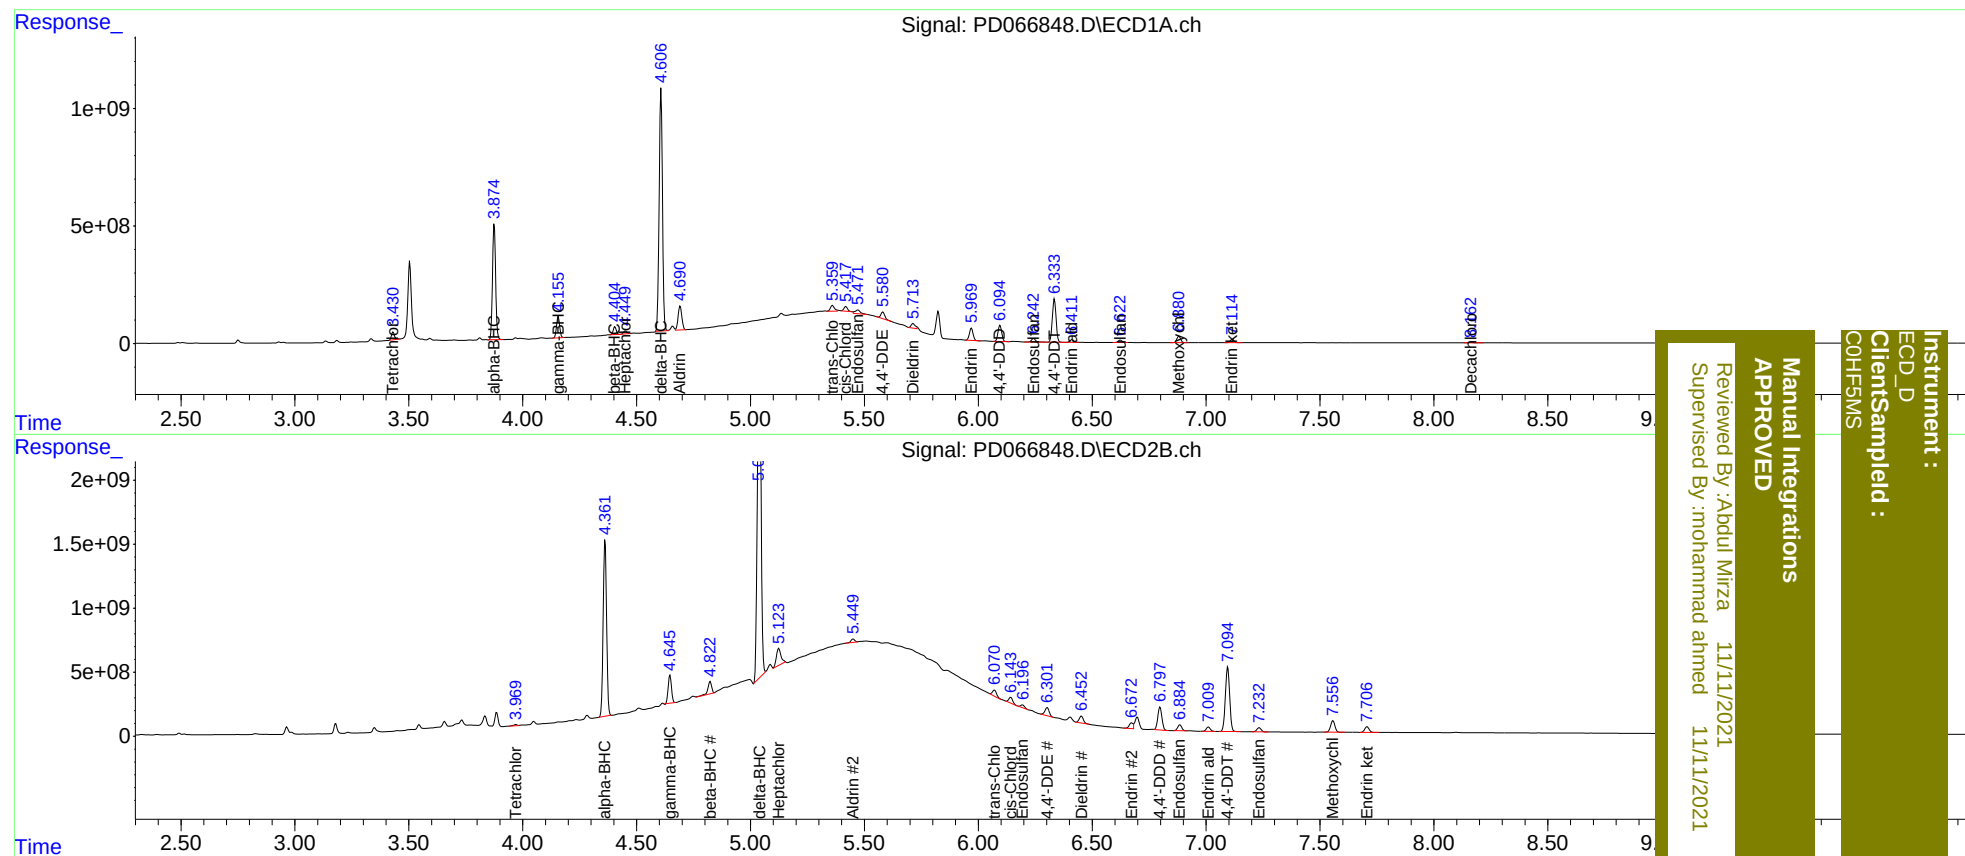

Instrument :
ECD_D
ClientSampled :
COHFSMS

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 11/11/2021
Supervised By: mohammad ahmed 11/11/2021