

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111023\
 Data File : PD079518.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2023 19:14
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 01:04:36 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111023CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 08 01:02:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	2.803	7546532	11452123	5.492	5.360
27)	SA Decachlor...	9.117	7.950	17740405	25495562	10.769	11.090
Target Compounds							
2)	A alpha-BHC	4.026	3.306	11448155	17056859	5.036	5.025
3)	MA gamma-BHC...	4.359	3.636	11223353	16031786	5.164	5.053
4)	MA Heptachlor	4.953	3.979	12536233	16239202	5.427	5.237
9)	A Endosulfan I	6.109	5.131	10639214	14064064	5.448	5.302
13)	MA Dieldrin	6.385	5.396	21230997	29824301	10.394	9.997
14)	MA Endrin	6.615	5.671	17818395	26488845	10.504	10.148
16)	A 4,4'-DDD	6.746	5.819	15708807	22807429	10.390	10.146
17)	MA 4,4'-DDT	7.062	6.070	15900730	22160217	10.134	9.720
20)	A Methoxychlor	7.536	6.645	46535673	66719274	54.319	53.521


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111023\
Data File : PD079518.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2023 19:14
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 01:04:36 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111023CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 08 01:02:54 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

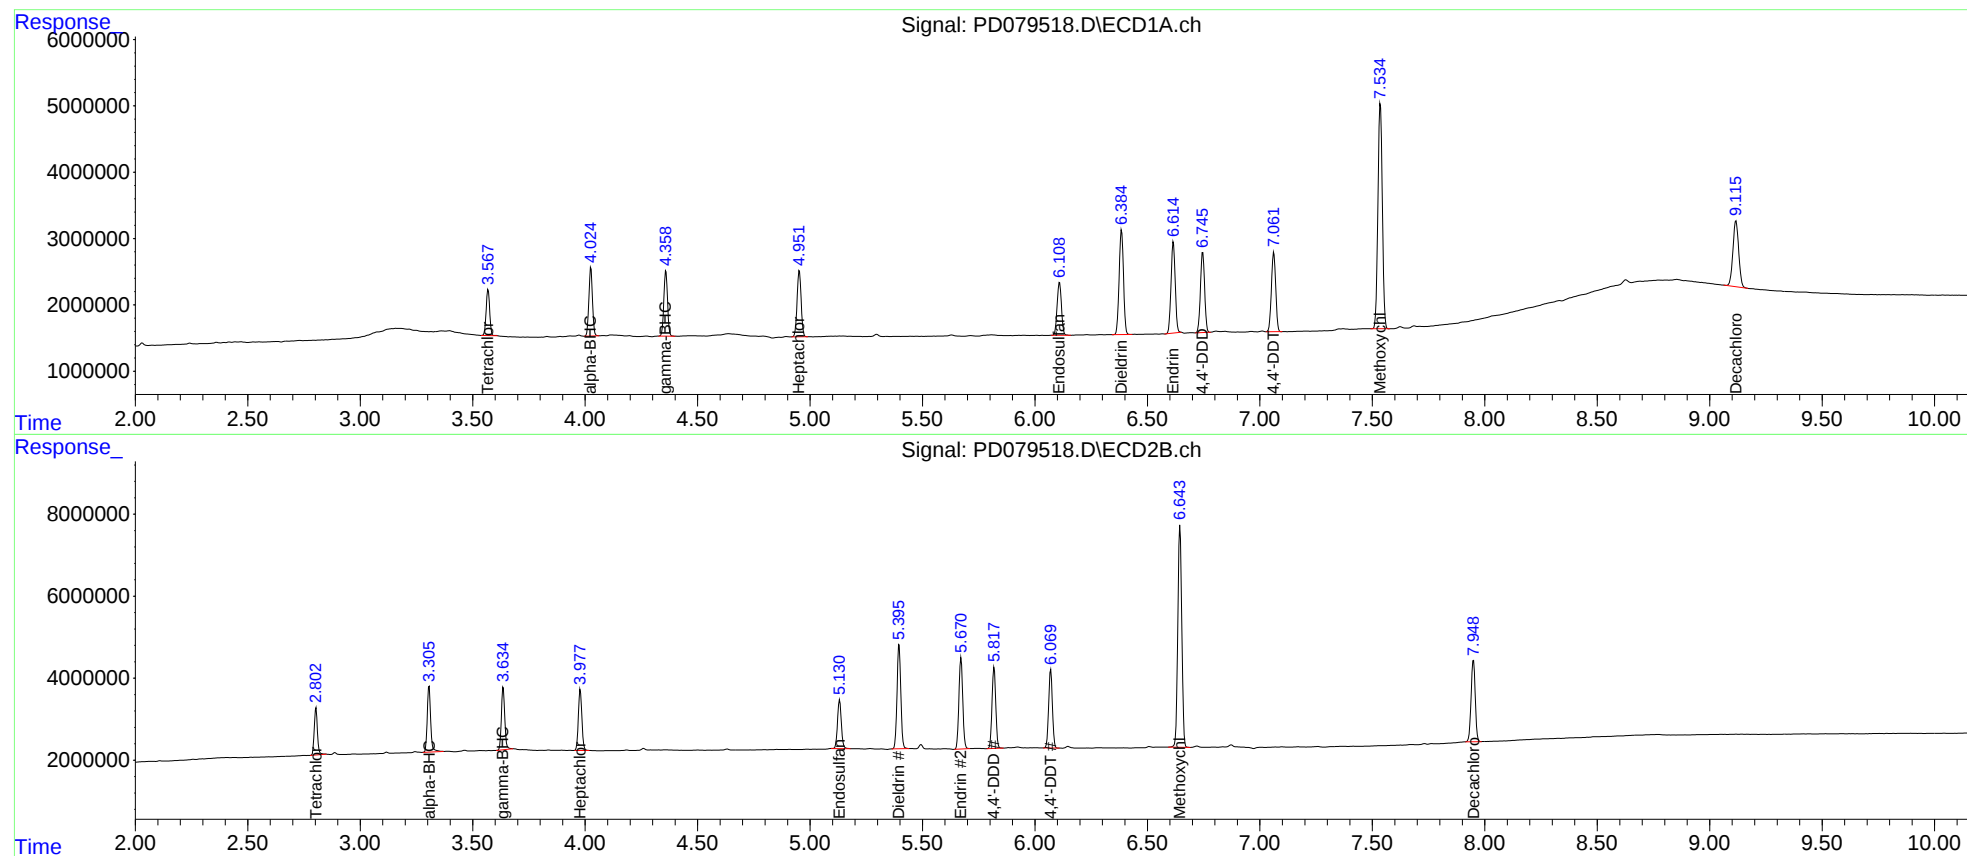

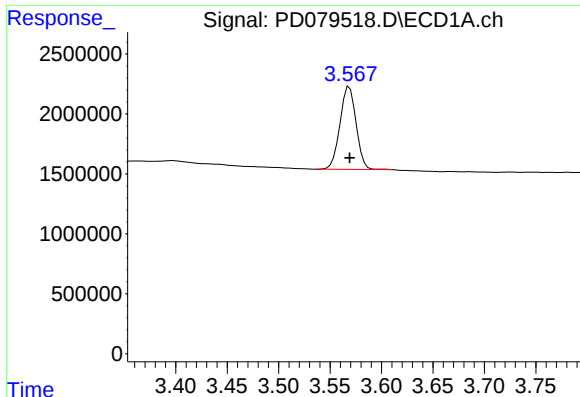


#1 Tetrachloro-m-xylene

R.T.: 3.569 min
Delta R.T.: 0.000 min
Response: 7546532
Conc: 5.49 ng/ml

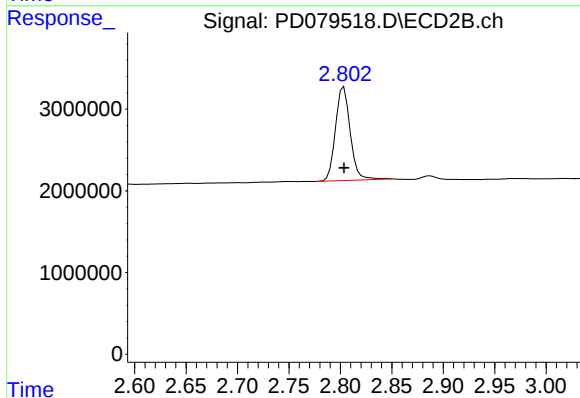


#1 Tetrachloro-m-xylene

R.T.: 2.803 min
Delta R.T.: 0.000 min
Response: 11452123
Conc: 5.36 ng/ml

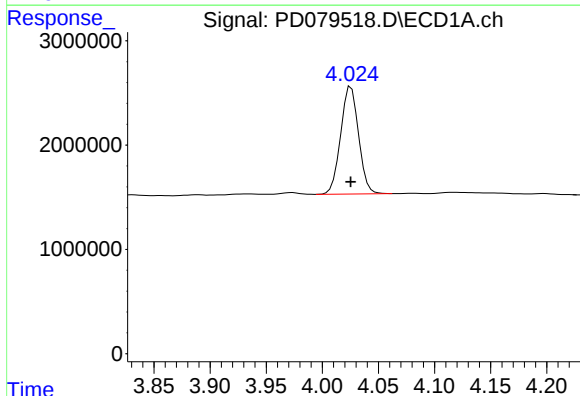


#2 alpha-BHC

R.T.: 4.026 min
Delta R.T.: 0.000 min
Response: 11448155
Conc: 5.04 ng/ml

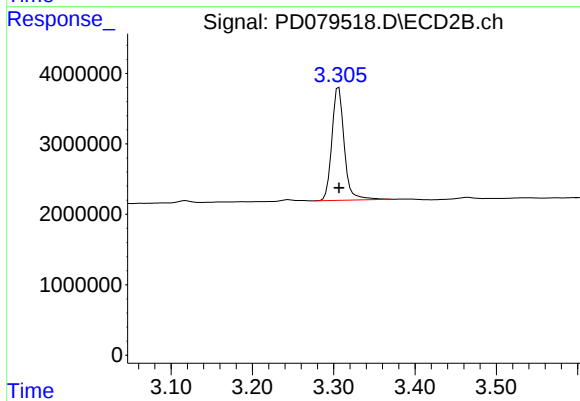


#2 alpha-BHC

R.T.: 3.306 min
Delta R.T.: 0.000 min
Response: 17056859
Conc: 5.02 ng/ml

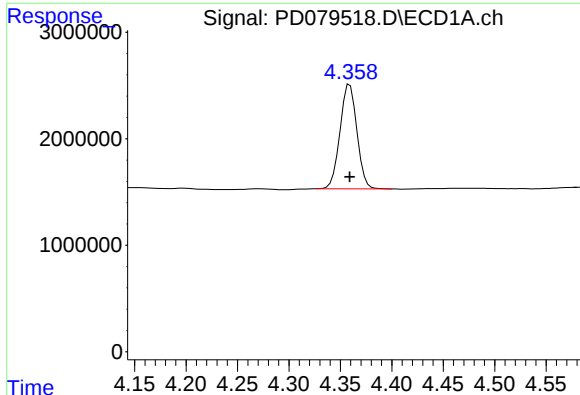


#3 gamma-BHC (Lindane)

R.T.: 4.359 min
Delta R.T.: 0.000 min
Response: 11223353
Conc: 5.16 ng/ml

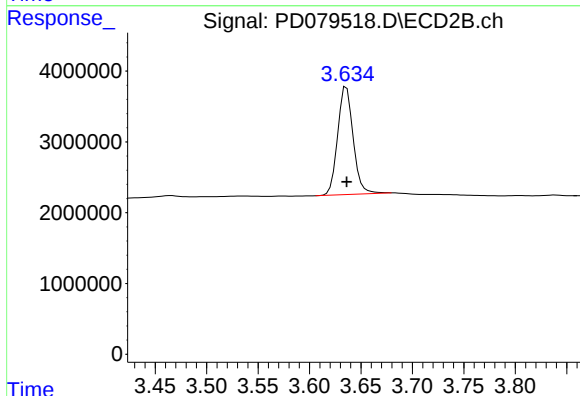


#3 gamma-BHC (Lindane)

R.T.: 3.636 min
Delta R.T.: 0.000 min
Response: 16031786
Conc: 5.05 ng/ml

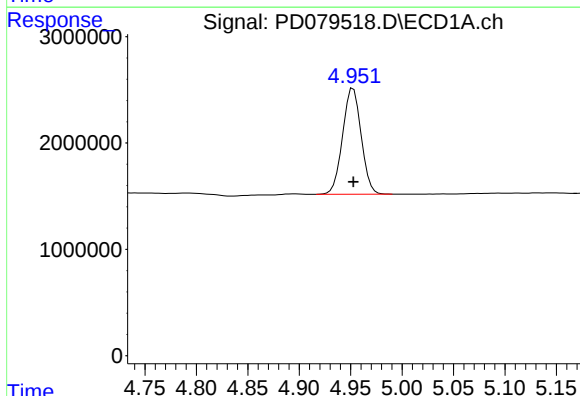


#4 Heptachlor

R.T.: 4.953 min
Delta R.T.: 0.000 min
Response: 12536233
Conc: 5.43 ng/ml

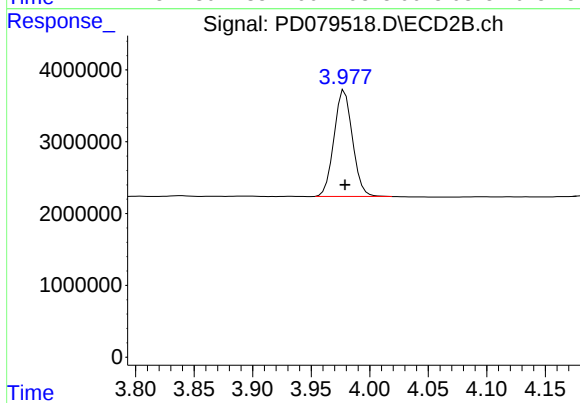


#4 Heptachlor

R.T.: 3.979 min
Delta R.T.: 0.000 min
Response: 16239202
Conc: 5.24 ng/ml

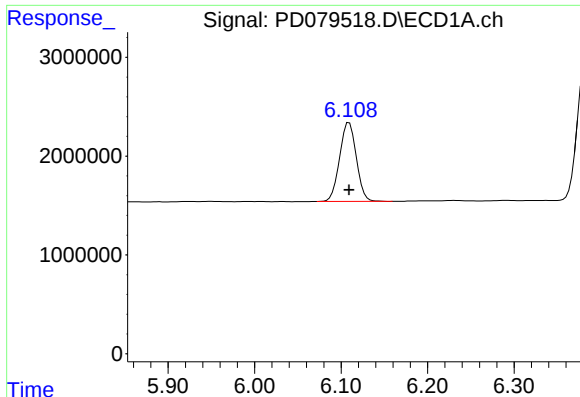


#9 Endosulfan I

R.T.: 6.109 min
Delta R.T.: 0.000 min
Response: 10639214
Conc: 5.45 ng/ml

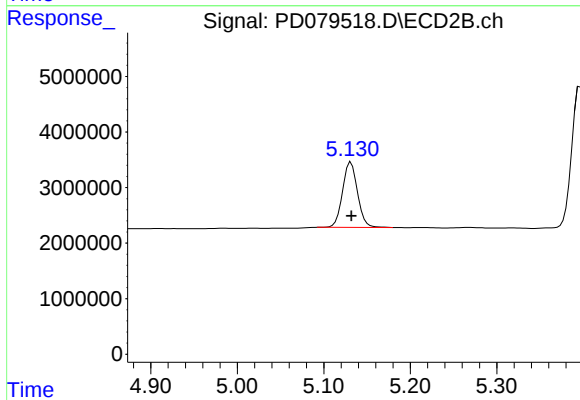


#9 Endosulfan I

R.T.: 5.131 min
Delta R.T.: 0.000 min
Response: 14064064
Conc: 5.30 ng/ml

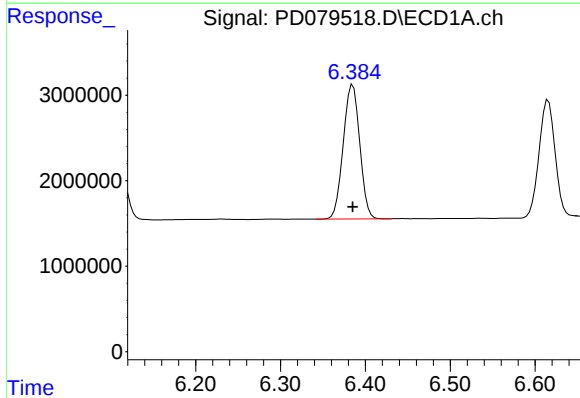


#13 Dieldrin

R.T.: 6.385 min
Delta R.T.: 0.000 min
Response: 21230997
Conc: 10.39 ng/ml

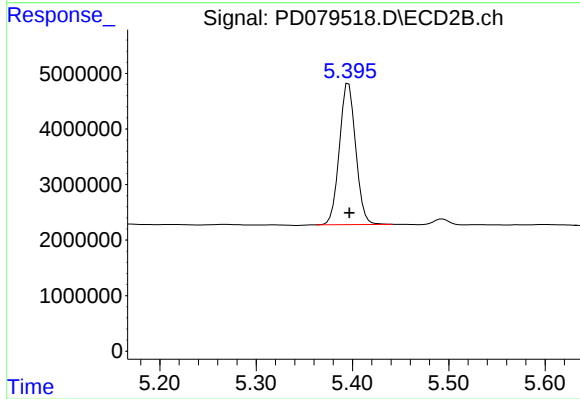


#13 Dieldrin

R.T.: 5.396 min
Delta R.T.: 0.000 min
Response: 29824301
Conc: 10.00 ng/ml

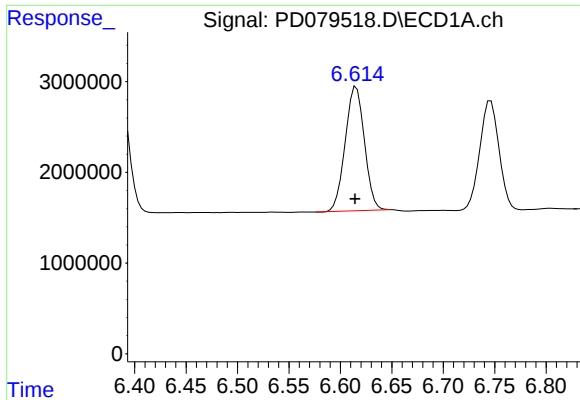


#14 Endrin

R.T.: 6.615 min
Delta R.T.: 0.001 min
Response: 17818395
Conc: 10.50 ng/ml

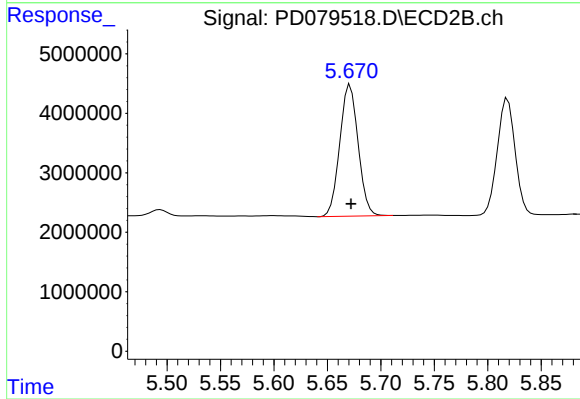


#14 Endrin

R.T.: 5.671 min
Delta R.T.: 0.000 min
Response: 26488845
Conc: 10.15 ng/ml

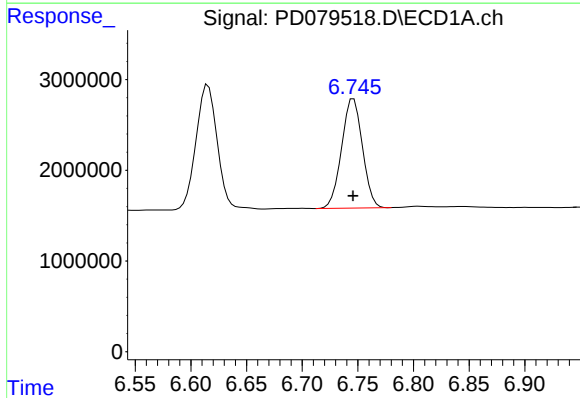


#16 4,4'-DDD

R.T.: 6.746 min
Delta R.T.: 0.000 min
Response: 15708807
Conc: 10.39 ng/ml

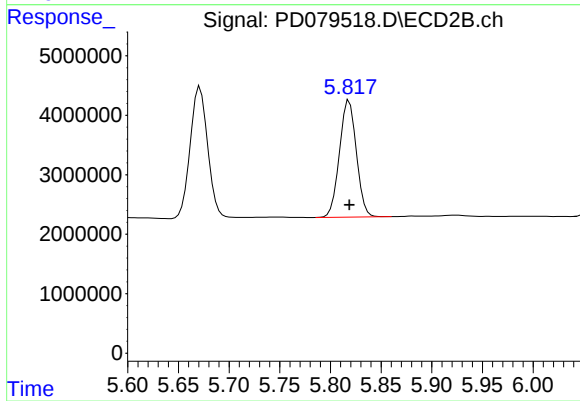


#16 4,4'-DDD

R.T.: 5.819 min
Delta R.T.: 0.000 min
Response: 22807429
Conc: 10.15 ng/ml

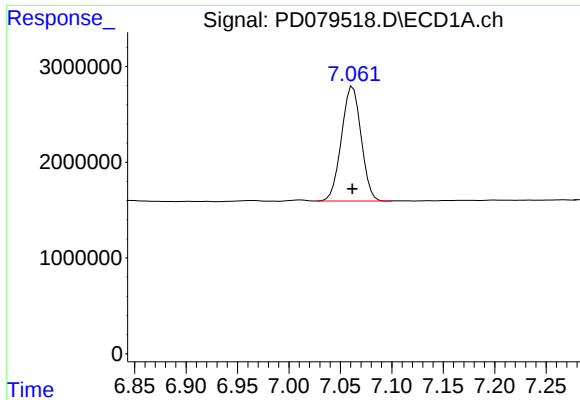


#17 4,4'-DDT

R.T.: 7.062 min
Delta R.T.: 0.000 min
Response: 15900730
Conc: 10.13 ng/ml

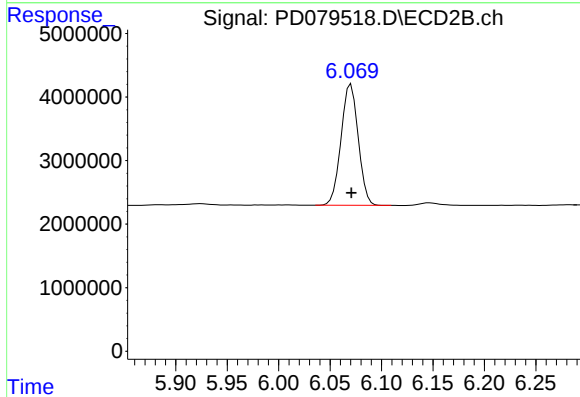


#17 4,4'-DDT

R.T.: 6.070 min
Delta R.T.: 0.000 min
Response: 22160217
Conc: 9.72 ng/ml

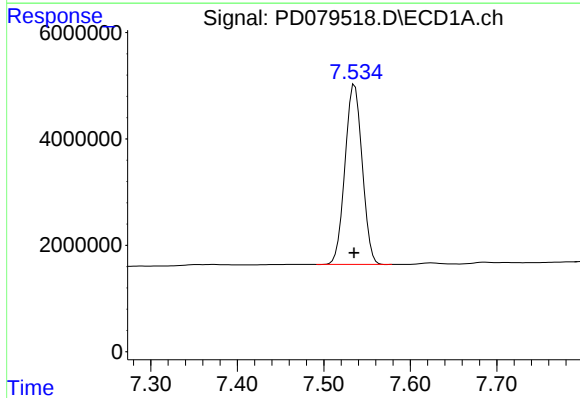


#20 Methoxychlor

R.T.: 7.536 min
Delta R.T.: 0.000 min
Response: 46535673
Conc: 54.32 ng/ml

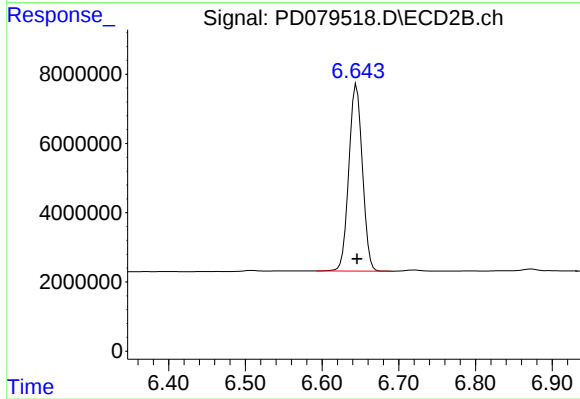


#20 Methoxychlor

R.T.: 6.645 min
Delta R.T.: 0.000 min
Response: 66719274
Conc: 53.52 ng/ml

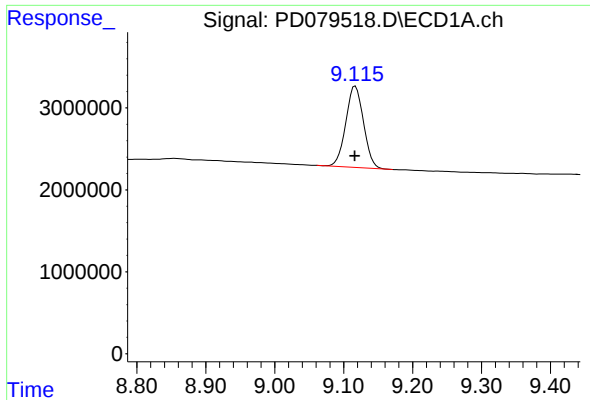

#27 Decachlorobiphenyl

R.T.: 9.117 min
Delta R.T.: 0.000 min
Response: 17740405
Conc: 10.77 ng/ml

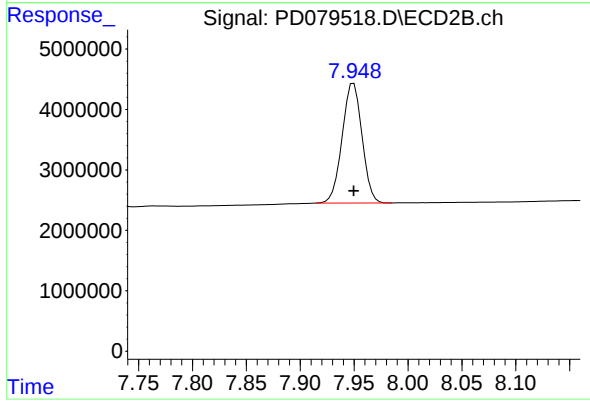

#27 Decachlorobiphenyl

R.T.: 7.950 min
Delta R.T.: 0.000 min
Response: 25495562
Conc: 11.09 ng/ml