

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111023\
 Data File : PD079520.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2023 19:40
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 01:04:51 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111023CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 08 01:02:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	2.804	14483355	22276218	10.540	10.425
27)	SA Decachlor...	9.117	7.950	34732865	48620455	21.084	21.149
Target Compounds							
2)	A alpha-BHC	4.026	3.307	22730614	34089584	10.000	10.042
3)	MA gamma-BHC...	4.359	3.636	22058976	31973921	10.150	10.078
4)	MA Heptachlor	4.952	3.979	24078597	32210563	10.424	10.388
9)	A Endosulfan I	6.109	5.132	20311899	27469526	10.402	10.355
13)	MA Dieldrin	6.385	5.397	41918973	60020441	20.521	20.118
14)	MA Endrin	6.615	5.672	34922831	52762528	20.587	20.214
16)	A 4,4'-DDD	6.746	5.819	31117940	45737770	20.582	20.347
17)	MA 4,4'-DDT	7.061	6.071	31807134	45347650	20.271	19.890
20)	A Methoxychlor	7.536	6.645	89315175	130.3E6	104.254	104.518


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111023\
Data File : PD079520.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2023 19:40
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 01:04:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111023CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 08 01:02:54 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

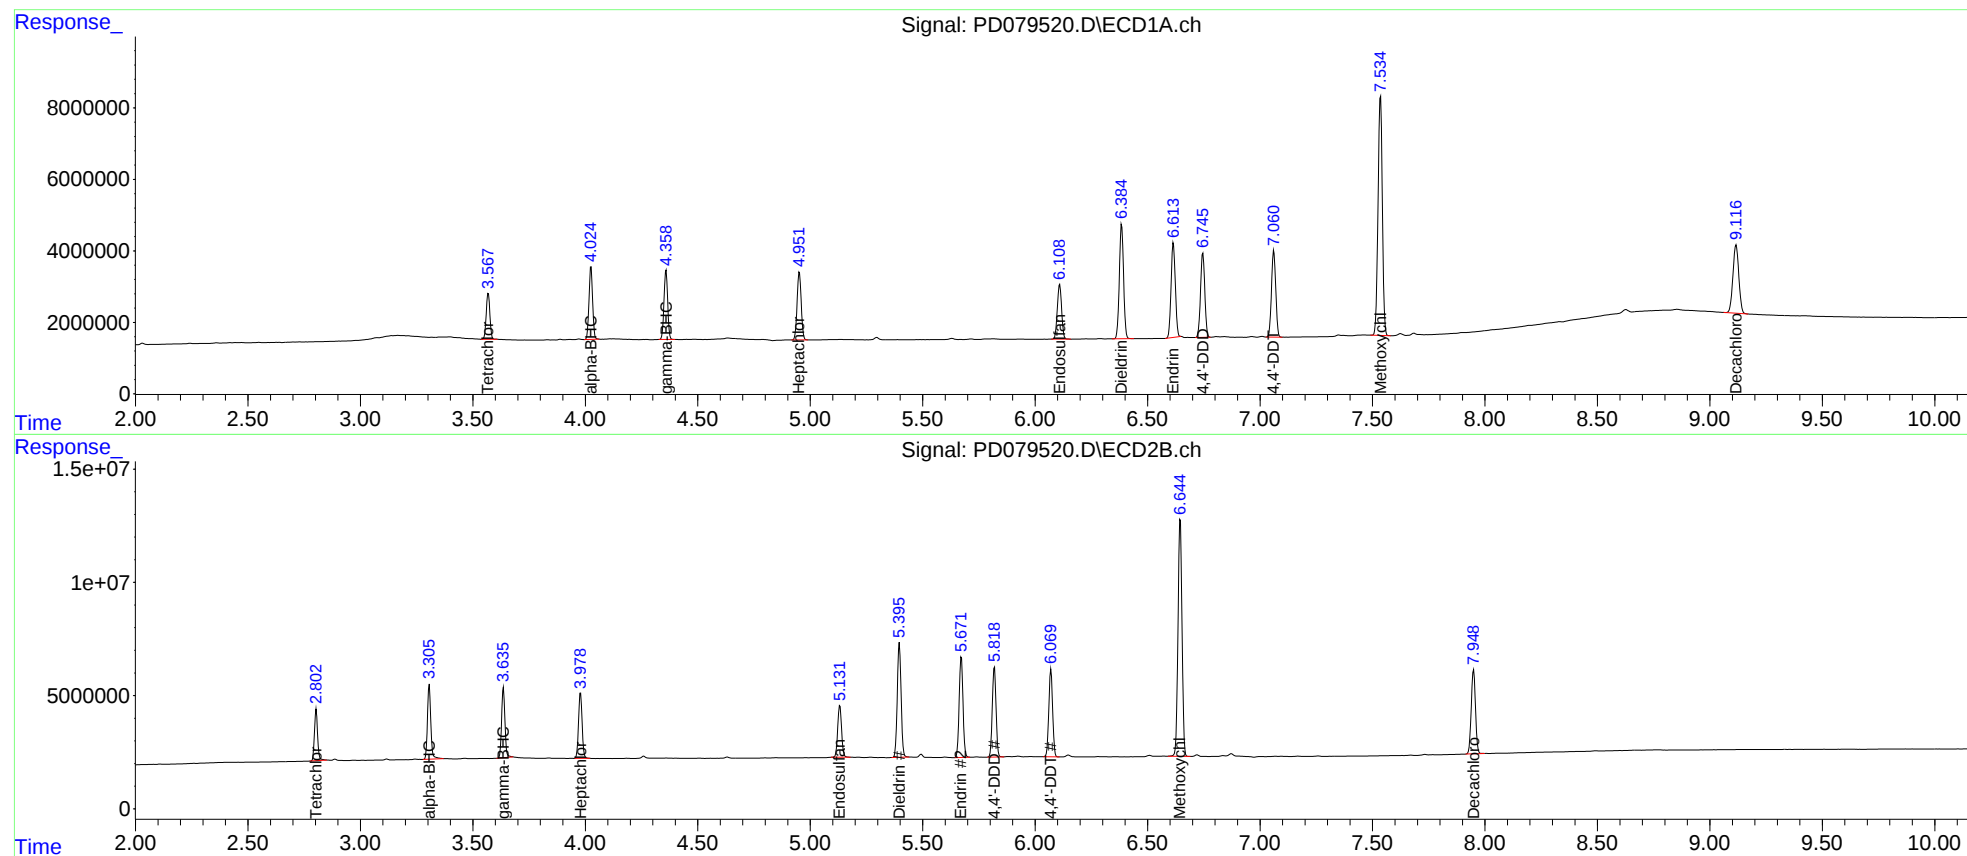

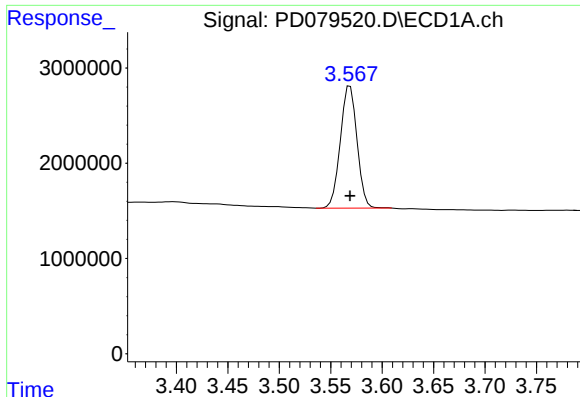


#1 Tetrachloro-m-xylene

R.T.: 3.569 min
Delta R.T.: 0.000 min
Response: 14483355
Conc: 10.54 ng/ml

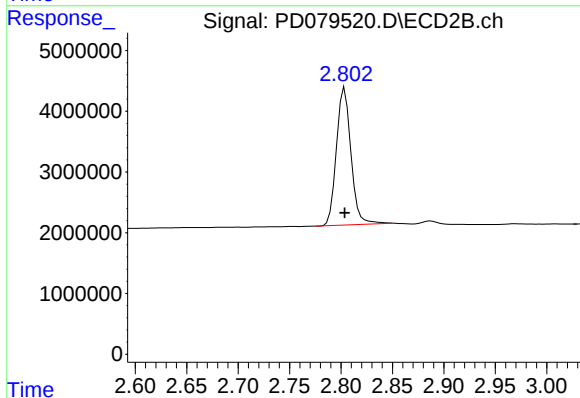


#1 Tetrachloro-m-xylene

R.T.: 2.804 min
Delta R.T.: 0.000 min
Response: 22276218
Conc: 10.43 ng/ml

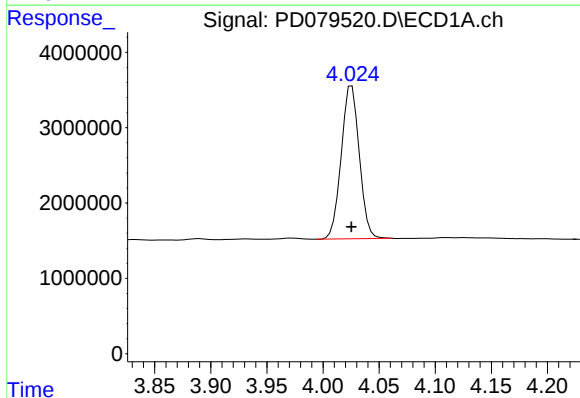


#2 alpha-BHC

R.T.: 4.026 min
Delta R.T.: 0.000 min
Response: 22730614
Conc: 10.00 ng/ml

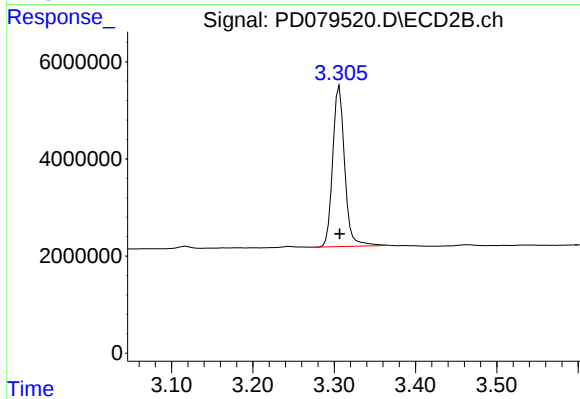


#2 alpha-BHC

R.T.: 3.307 min
Delta R.T.: 0.000 min
Response: 34089584
Conc: 10.04 ng/ml

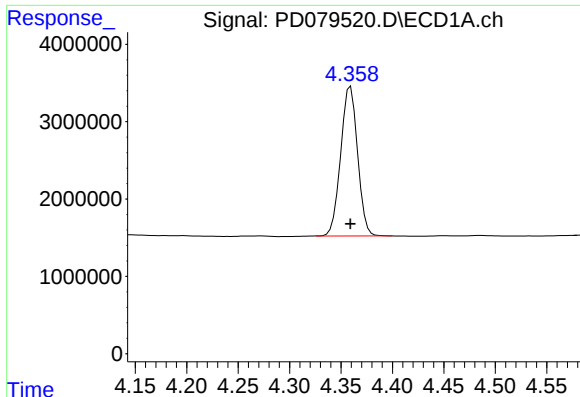


#3 gamma-BHC (Lindane)

R.T.: 4.359 min
Delta R.T.: 0.000 min
Response: 22058976
Conc: 10.15 ng/ml

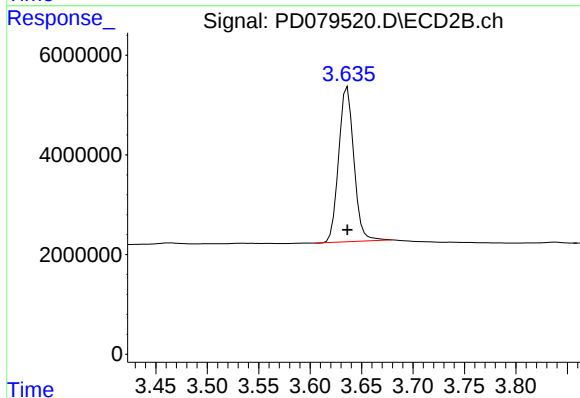


#3 gamma-BHC (Lindane)

R.T.: 3.636 min
Delta R.T.: 0.000 min
Response: 31973921
Conc: 10.08 ng/ml

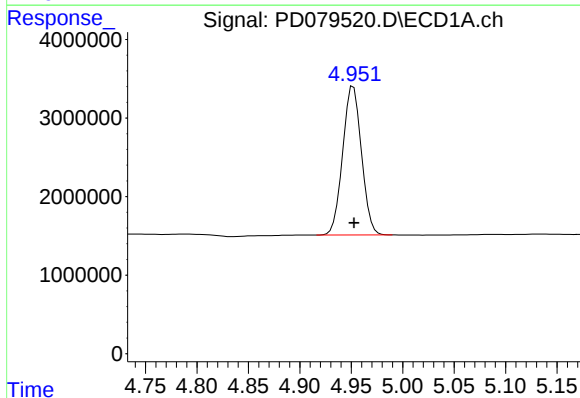


#4 Heptachlor

R.T.: 4.952 min
Delta R.T.: 0.000 min
Response: 24078597
Conc: 10.42 ng/ml

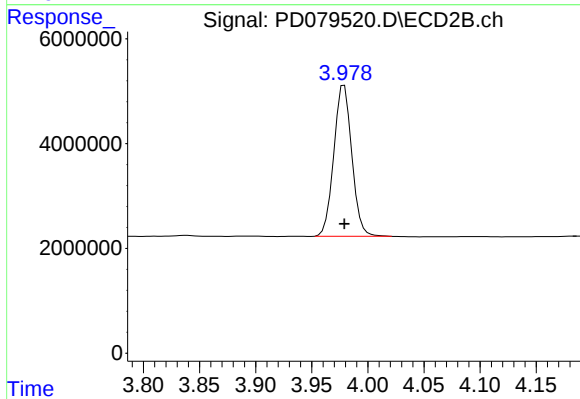


#4 Heptachlor

R.T.: 3.979 min
Delta R.T.: 0.000 min
Response: 32210563
Conc: 10.39 ng/ml

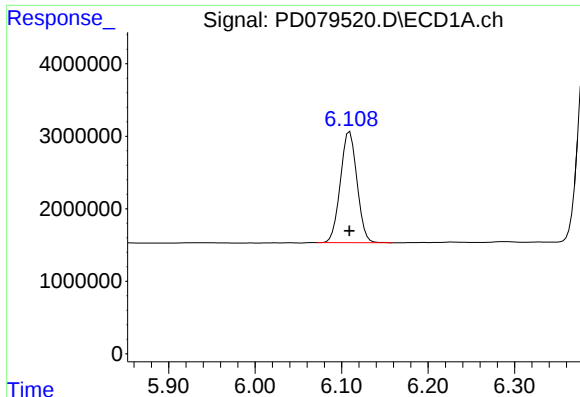


#9 Endosulfan I

R.T.: 6.109 min
Delta R.T.: 0.000 min
Response: 20311899
Conc: 10.40 ng/ml

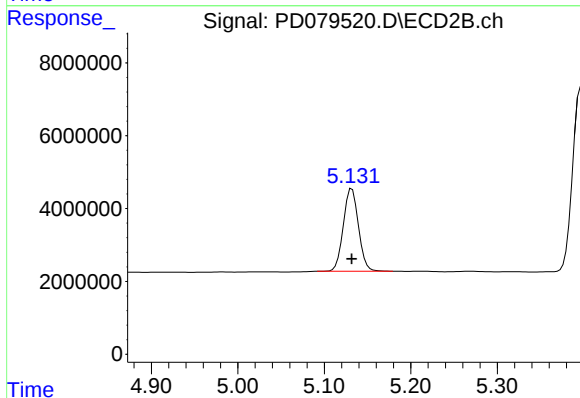


#9 Endosulfan I

R.T.: 5.132 min
Delta R.T.: 0.000 min
Response: 27469526
Conc: 10.36 ng/ml

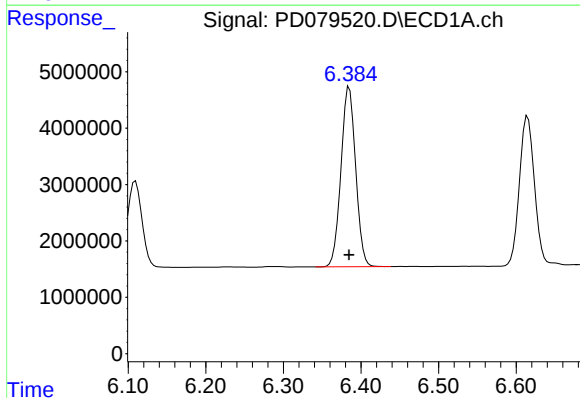


#13 Dieldrin

R.T.: 6.385 min
Delta R.T.: 0.000 min
Response: 41918973
Conc: 20.52 ng/ml

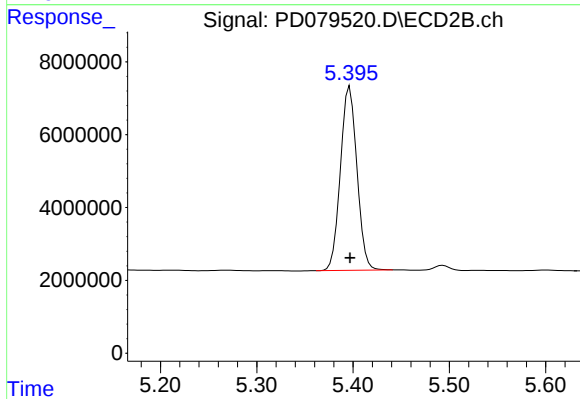


#13 Dieldrin

R.T.: 5.397 min
Delta R.T.: 0.000 min
Response: 60020441
Conc: 20.12 ng/ml

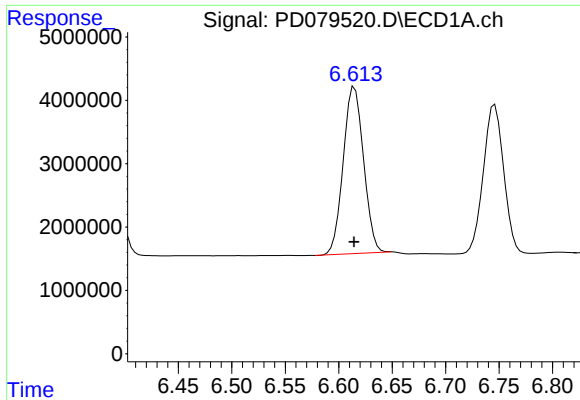


#14 Endrin

R.T.: 6.615 min
Delta R.T.: 0.000 min
Response: 34922831
Conc: 20.59 ng/ml

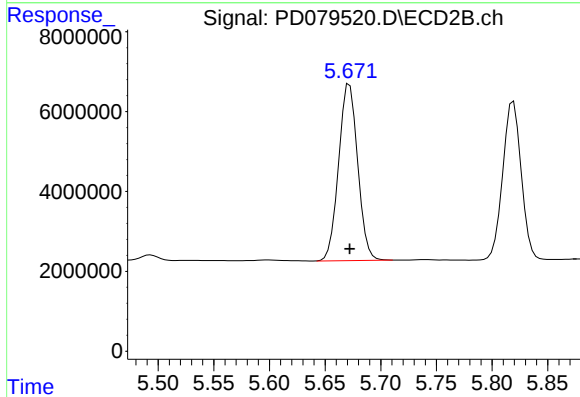


#14 Endrin

R.T.: 5.672 min
Delta R.T.: 0.000 min
Response: 52762528
Conc: 20.21 ng/ml

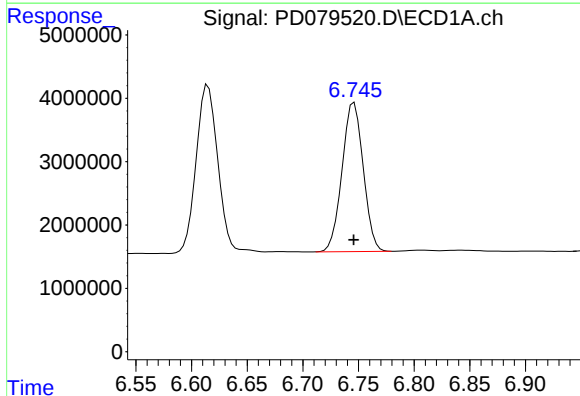


#16 4,4'-DDD

R.T.: 6.746 min
Delta R.T.: 0.000 min
Response: 31117940
Conc: 20.58 ng/ml

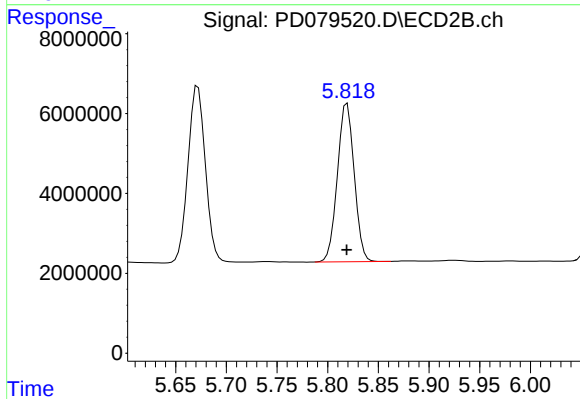


#16 4,4'-DDD

R.T.: 5.819 min
Delta R.T.: 0.000 min
Response: 45737770
Conc: 20.35 ng/ml

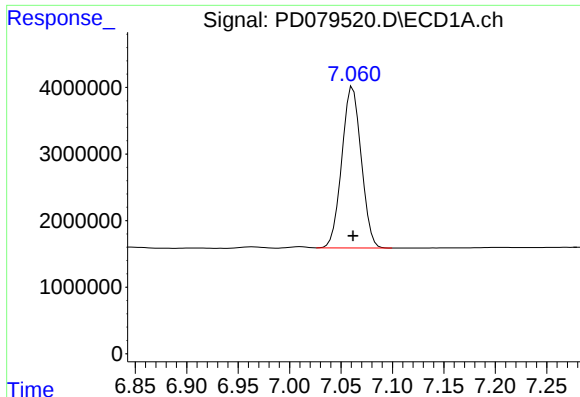


#17 4,4'-DDT

R.T.: 7.061 min
Delta R.T.: 0.000 min
Response: 31807134
Conc: 20.27 ng/ml

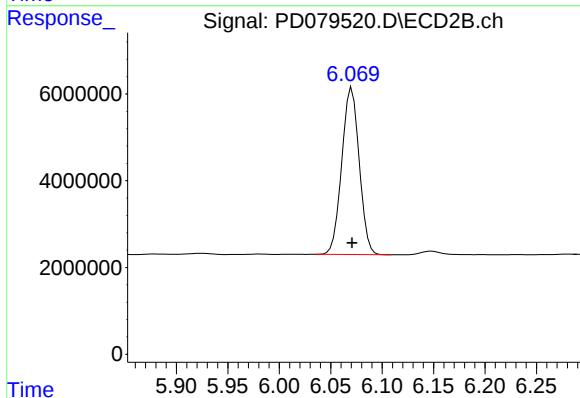


#17 4,4'-DDT

R.T.: 6.071 min
Delta R.T.: 0.000 min
Response: 45347650
Conc: 19.89 ng/ml

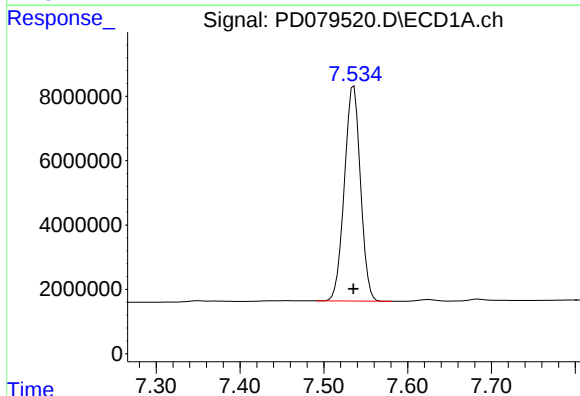


#20 Methoxychlor

R.T.: 7.536 min
Delta R.T.: 0.000 min
Response: 89315175
Conc: 104.25 ng/ml

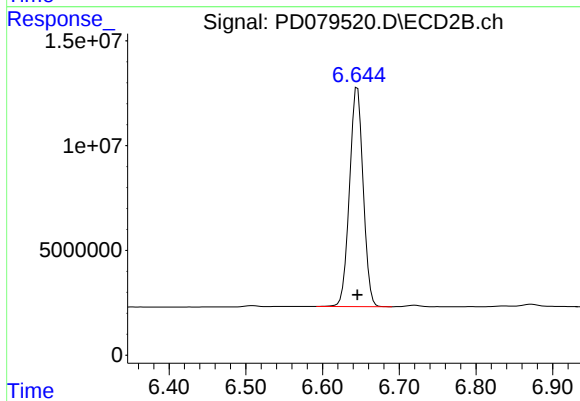


#20 Methoxychlor

R.T.: 6.645 min
Delta R.T.: 0.000 min
Response: 130293175
Conc: 104.52 ng/ml

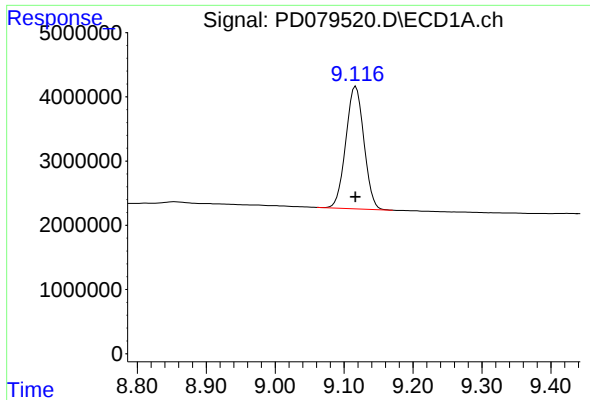

#27 Decachlorobiphenyl

R.T.: 9.117 min
Delta R.T.: 0.000 min
Response: 34732865
Conc: 21.08 ng/ml

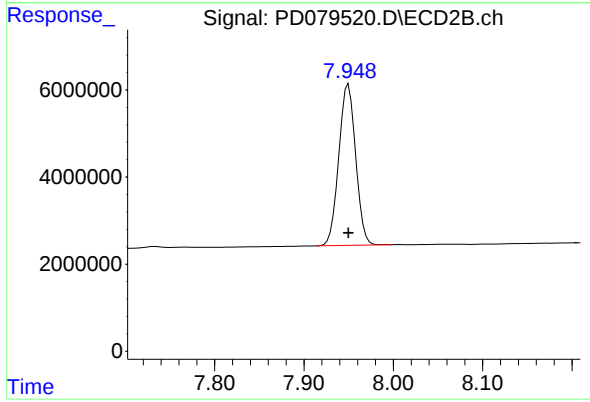

#27 Decachlorobiphenyl

R.T.: 7.950 min
Delta R.T.: 0.000 min
Response: 48620455
Conc: 21.15 ng/ml