

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111023\
 Data File : PD079522.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2023 20:07
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 01:05:06 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111023CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 08 01:02:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	2.804	27481570	42734245	20.000	20.000
27)	SA Decachlor...	9.116	7.950	65894726	91957837	40.000	40.000
Target Compounds							
2)	A alpha-BHC	4.025	3.307	45462857	67894730	20.000	20.000
3)	MA gamma-BHC...	4.359	3.636	43466157	63451141	20.000	20.000
4)	MA Heptachlor	4.953	3.979	46199817	62012376	20.000	20.000
9)	A Endosulfan I	6.109	5.132	39054713	53053263	20.000	20.000
13)	MA Dieldrin	6.385	5.397	81707513	119.3E6	40.000	40.000
14)	MA Endrin	6.614	5.672	67853324	104.4E6	40.000	40.000
16)	A 4,4'-DDD	6.746	5.819	60476280	89914075	40.000	40.000
17)	MA 4,4'-DDT	7.062	6.071	62764383	91198915	40.000	40.000
20)	A Methoxychlor	7.535	6.645	171.3E6	249.3E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111023\
Data File : PD079522.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2023 20:07
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 01:05:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111023CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 08 01:02:54 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

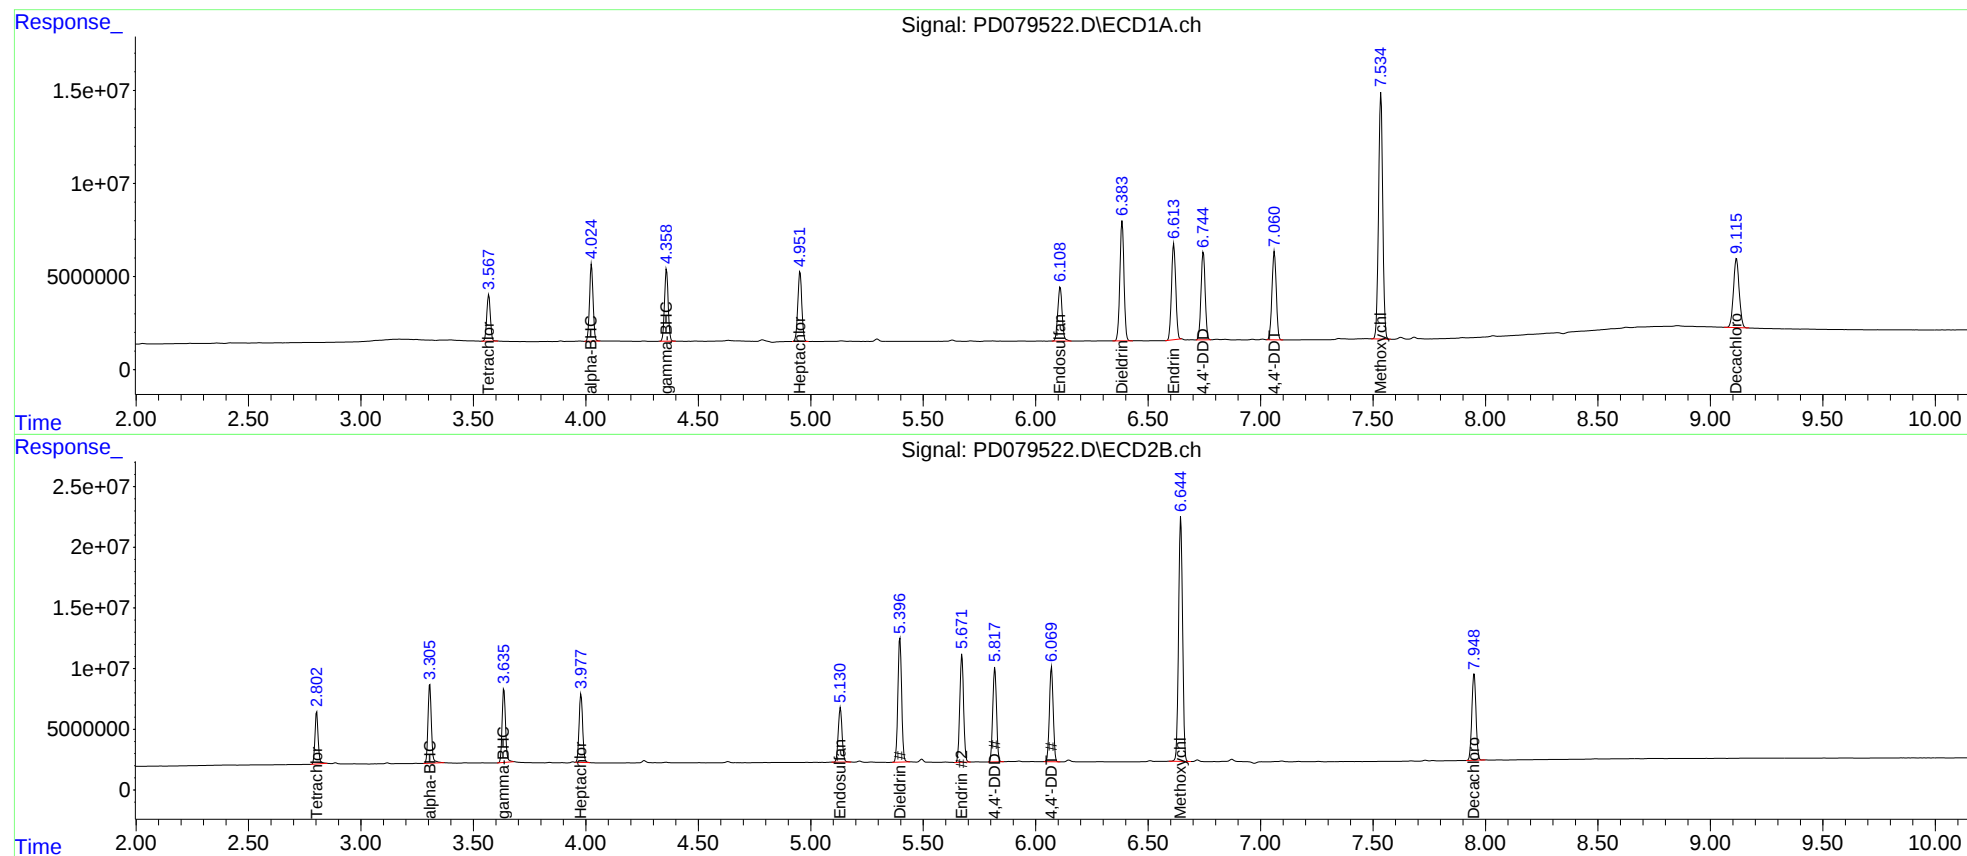

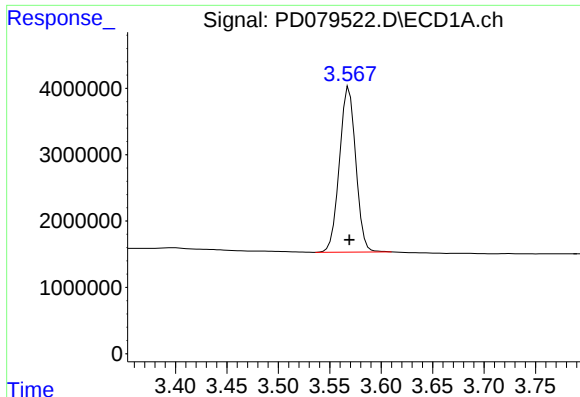


#1 Tetrachloro-m-xylene

R.T.: 3.569 min
Delta R.T.: 0.000 min
Response: 27481570
Conc: 20.00 ng/ml

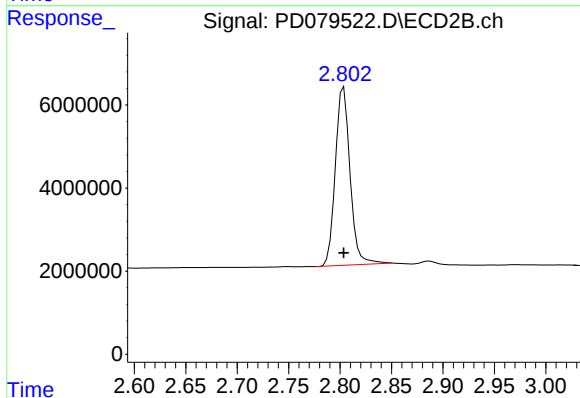


#1 Tetrachloro-m-xylene

R.T.: 2.804 min
Delta R.T.: 0.000 min
Response: 42734245
Conc: 20.00 ng/ml

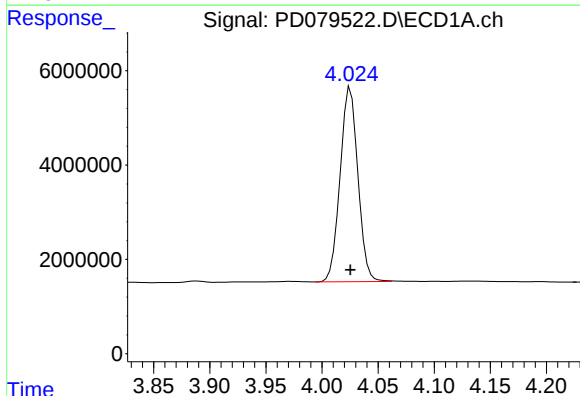


#2 alpha-BHC

R.T.: 4.025 min
Delta R.T.: 0.000 min
Response: 45462857
Conc: 20.00 ng/ml

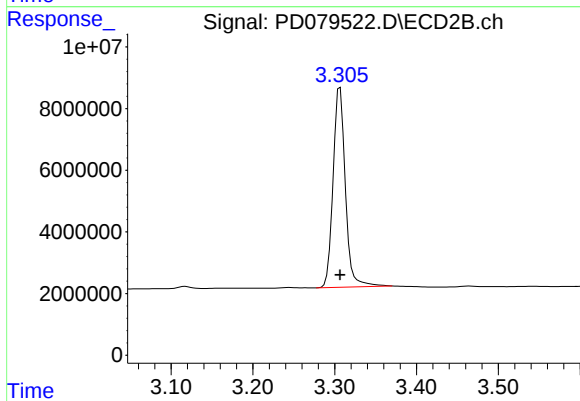


#2 alpha-BHC

R.T.: 3.307 min
Delta R.T.: 0.000 min
Response: 67894730
Conc: 20.00 ng/ml

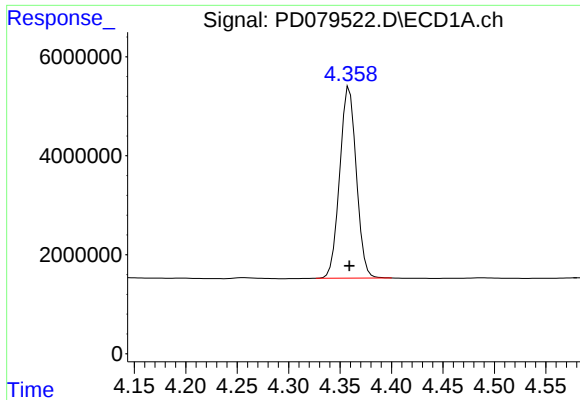


#3 gamma-BHC (Lindane)

R.T.: 4.359 min
Delta R.T.: 0.000 min
Response: 43466157
Conc: 20.00 ng/ml

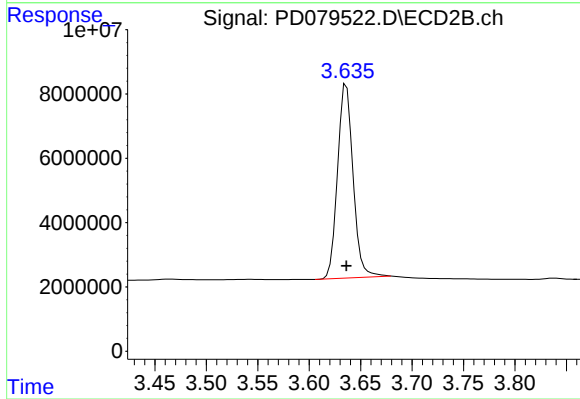


#3 gamma-BHC (Lindane)

R.T.: 3.636 min
Delta R.T.: 0.000 min
Response: 63451141
Conc: 20.00 ng/ml

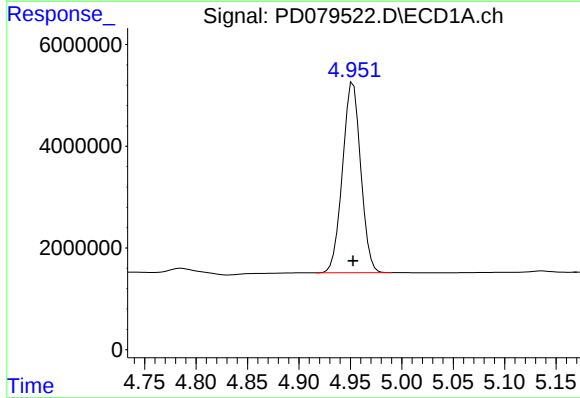


#4 Heptachlor

R.T.: 4.953 min
Delta R.T.: 0.000 min
Response: 46199817
Conc: 20.00 ng/ml

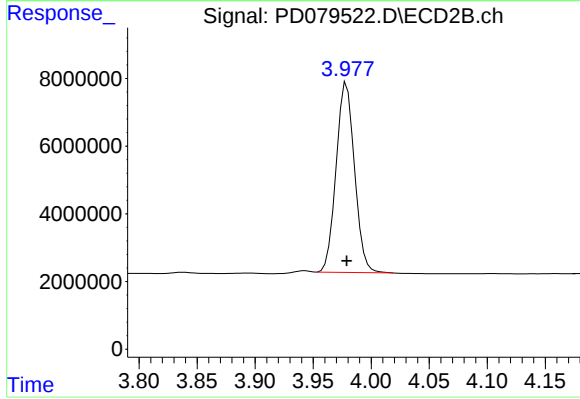


#4 Heptachlor

R.T.: 3.979 min
Delta R.T.: 0.000 min
Response: 62012376
Conc: 20.00 ng/ml

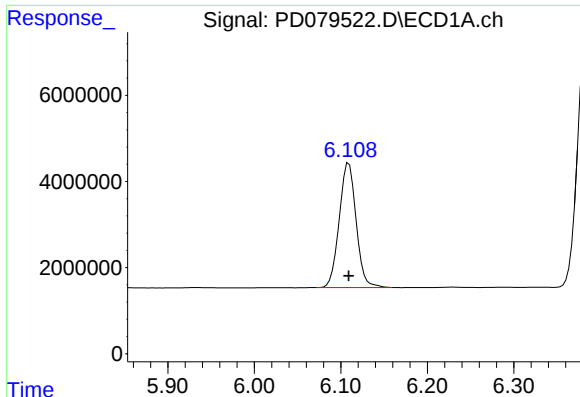


#9 Endosulfan I

R.T.: 6.109 min
Delta R.T.: 0.000 min
Response: 39054713
Conc: 20.00 ng/ml

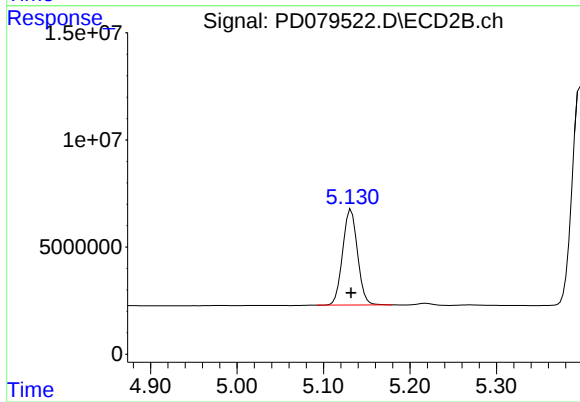


#9 Endosulfan I

R.T.: 5.132 min
Delta R.T.: 0.000 min
Response: 53053263
Conc: 20.00 ng/ml

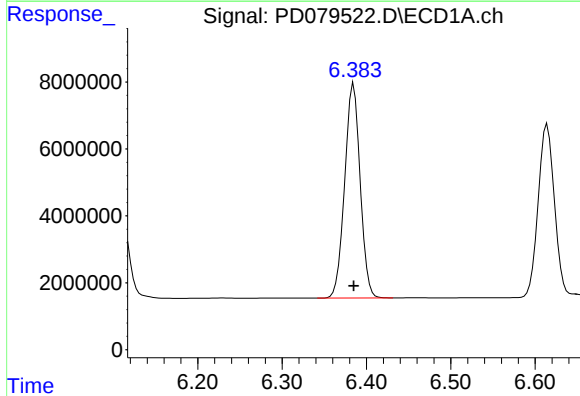


#13 Dieldrin

R.T.: 6.385 min
Delta R.T.: 0.000 min
Response: 81707513
Conc: 40.00 ng/ml

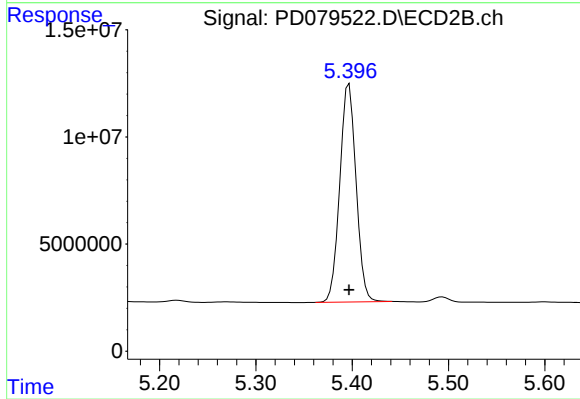


#13 Dieldrin

R.T.: 5.397 min
Delta R.T.: 0.000 min
Response: 119335453
Conc: 40.00 ng/ml

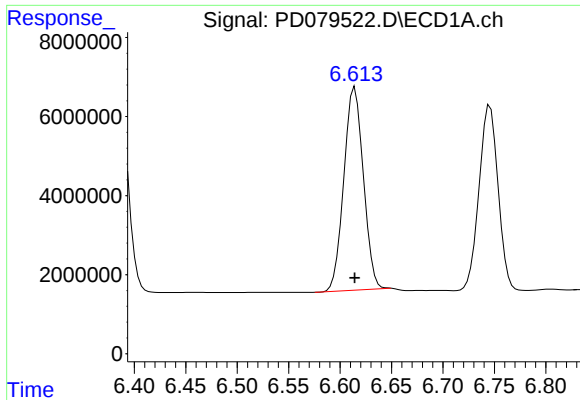


#14 Endrin

R.T.: 6.614 min
Delta R.T.: 0.000 min
Response: 67853324
Conc: 40.00 ng/ml

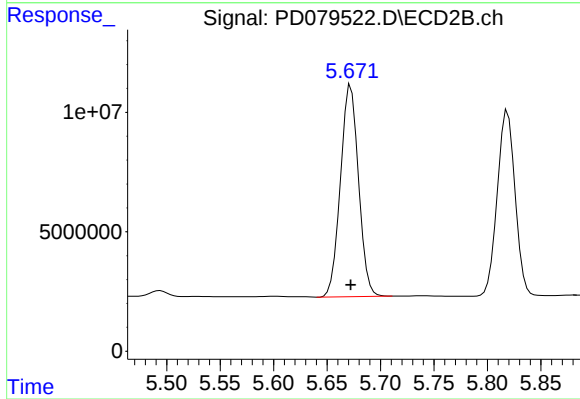


#14 Endrin

R.T.: 5.672 min
Delta R.T.: 0.000 min
Response: 104409274
Conc: 40.00 ng/ml

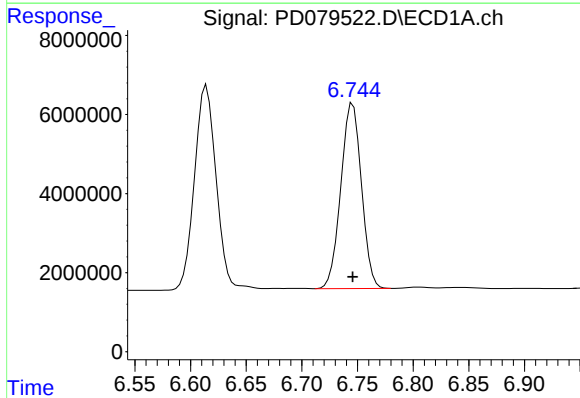


#16 4,4'-DDD

R.T.: 6.746 min
Delta R.T.: 0.000 min
Response: 60476280
Conc: 40.00 ng/ml

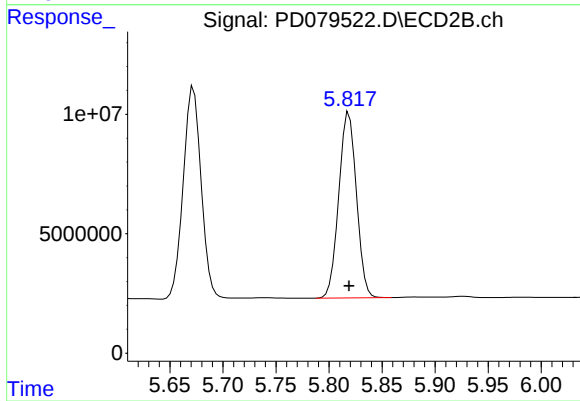


#16 4,4'-DDD

R.T.: 5.819 min
Delta R.T.: 0.000 min
Response: 89914075
Conc: 40.00 ng/ml

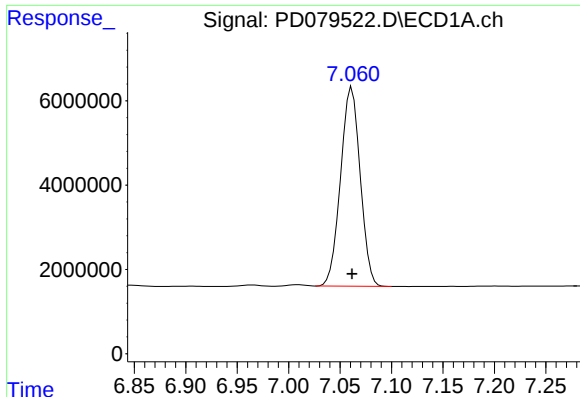


#17 4,4'-DDT

R.T.: 7.062 min
Delta R.T.: 0.000 min
Response: 62764383
Conc: 40.00 ng/ml

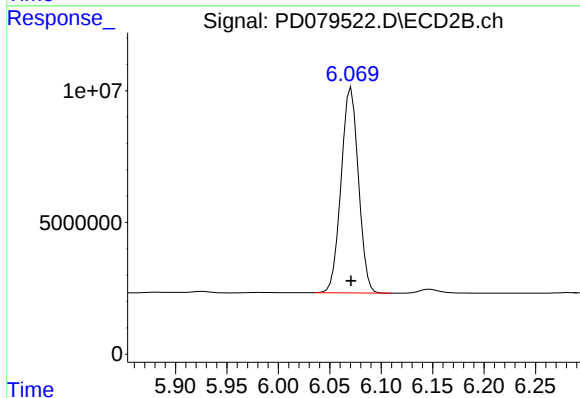


#17 4,4'-DDT

R.T.: 6.071 min
Delta R.T.: 0.000 min
Response: 91198915
Conc: 40.00 ng/ml

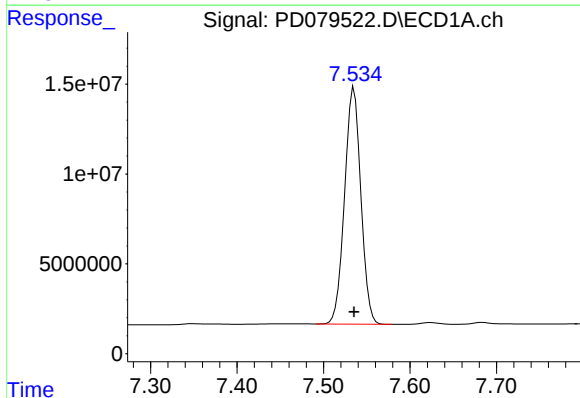


#20 Methoxychlor

R.T.: 7.535 min
Delta R.T.: 0.000 min
Response: 171340823
Conc: 200.00 ng/ml

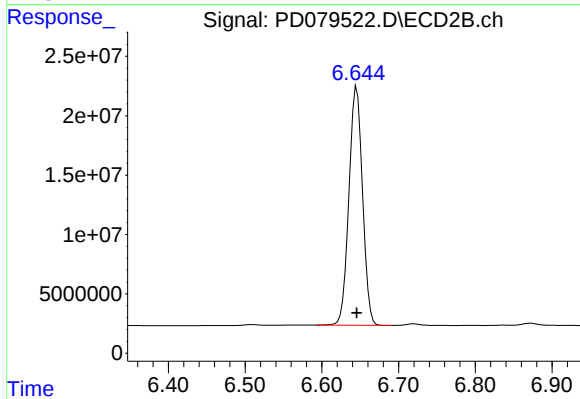


#20 Methoxychlor

R.T.: 6.645 min
Delta R.T.: 0.000 min
Response: 249321197
Conc: 200.00 ng/ml

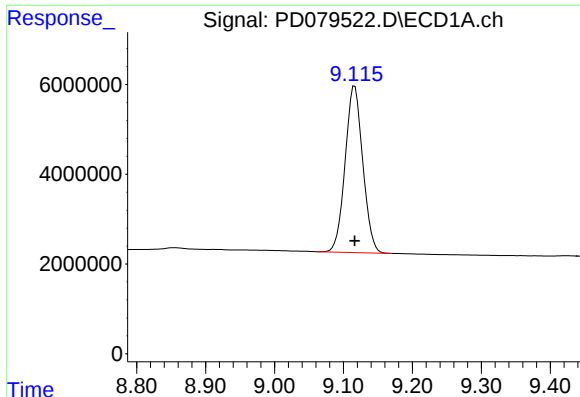

#27 Decachlorobiphenyl

R.T.: 9.116 min
Delta R.T.: 0.000 min
Response: 65894726
Conc: 40.00 ng/ml

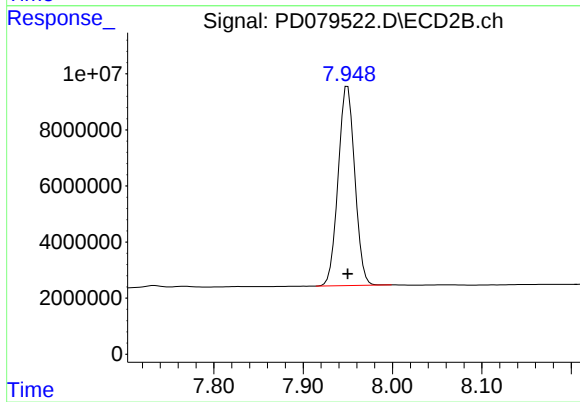

#27 Decachlorobiphenyl

R.T.: 7.950 min
Delta R.T.: 0.000 min
Response: 91957837
Conc: 40.00 ng/ml