

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111023\
 Data File : PD079524.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2023 20:34
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 01:05:19 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111023CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 08 01:02:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	2.804	54239135	85160939	39.473	39.856
27)	SA Decachlor...	9.118	7.950	130.5E6	183.8E6	79.227	79.928
Target Compounds							
2)	A alpha-BHC	4.026	3.307	94952067	141.2E6	41.771	41.581
3)	MA gamma-BHC...	4.360	3.636	90296237	131.0E6	41.548	41.276
4)	MA Heptachlor	4.953	3.979	93898728	128.1E6	40.649	41.325
9)	A Endosulfan I	6.109	5.132	76629537	107.8E6	39.242	40.657
13)	MA Dieldrin	6.385	5.397	169.2E6	249.1E6	82.853	83.479
14)	MA Endrin	6.615	5.672	139.4E6	216.8E6	82.170	83.055
16)	A 4,4'-DDD	6.746	5.819	125.7E6	189.2E6	83.149	84.176
17)	MA 4,4'-DDT	7.061	6.071	130.5E6	192.5E6	83.191	84.424
20)	A Methoxychlor	7.536	6.645	343.6E6	487.8E6	401.124	391.314


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111023\
Data File : PD079524.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2023 20:34
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 01:05:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111023CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 08 01:02:54 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

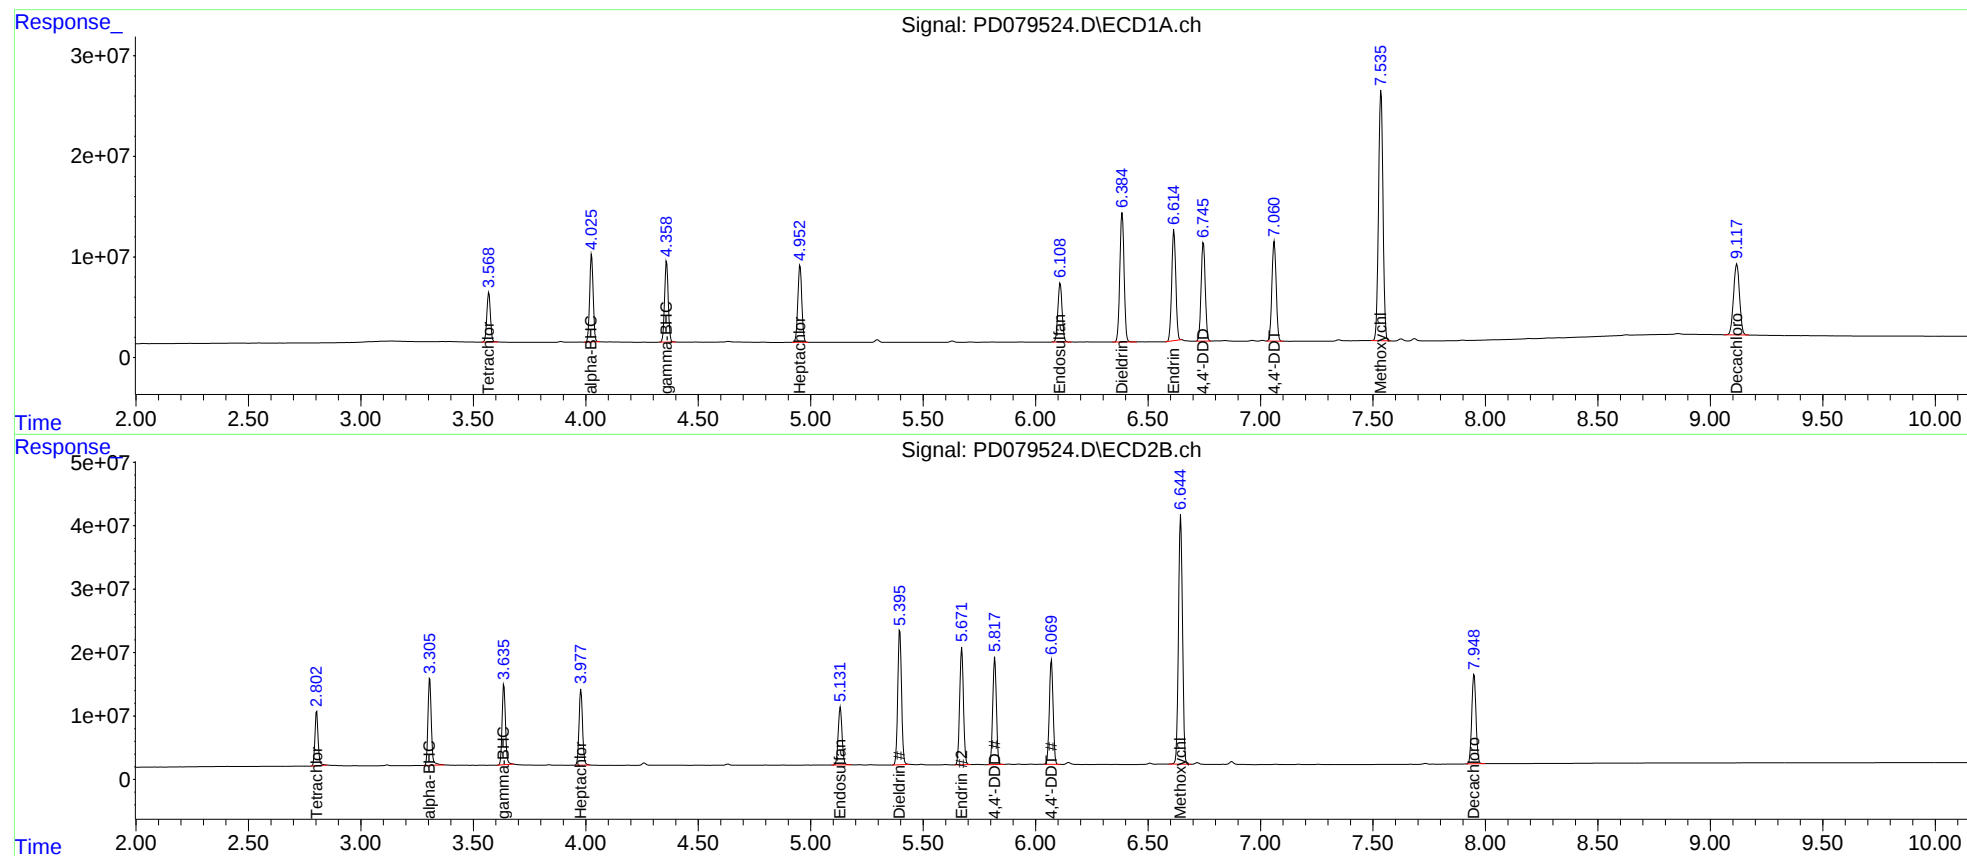

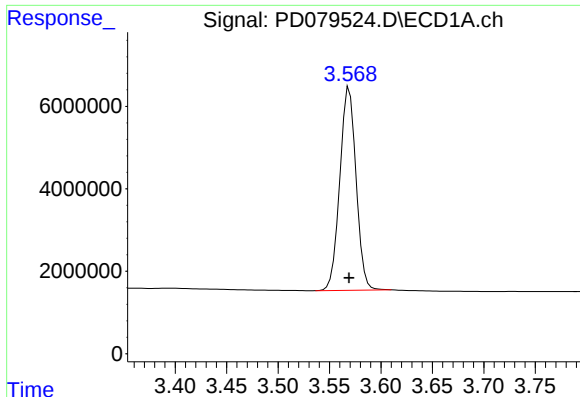


#1 Tetrachloro-m-xylene

R.T.: 3.569 min
Delta R.T.: 0.000 min
Response: 54239135
Conc: 39.47 ng/ml

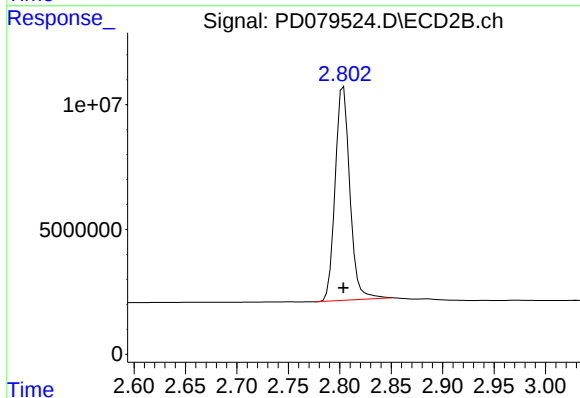


#1 Tetrachloro-m-xylene

R.T.: 2.804 min
Delta R.T.: 0.000 min
Response: 85160939
Conc: 39.86 ng/ml

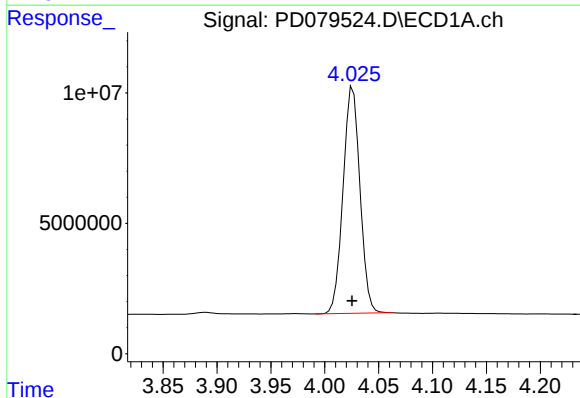


#2 alpha-BHC

R.T.: 4.026 min
Delta R.T.: 0.000 min
Response: 94952067
Conc: 41.77 ng/ml

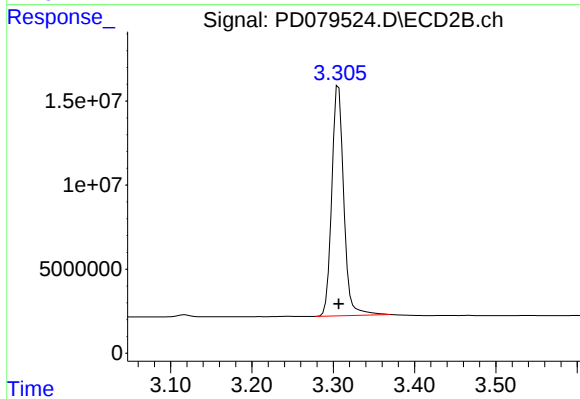


#2 alpha-BHC

R.T.: 3.307 min
Delta R.T.: 0.000 min
Response: 141157357
Conc: 41.58 ng/ml

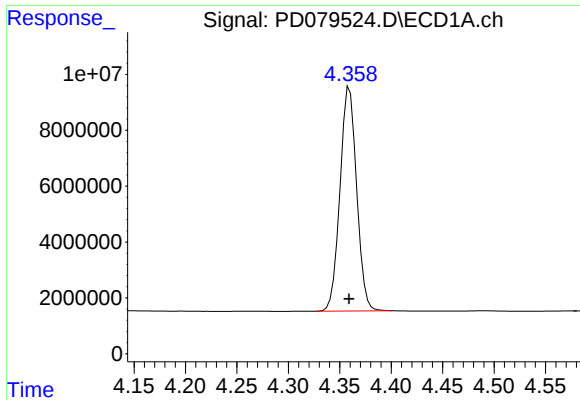


#3 gamma-BHC (Lindane)

R.T.: 4.360 min
Delta R.T.: 0.000 min
Response: 90296237
Conc: 41.55 ng/ml

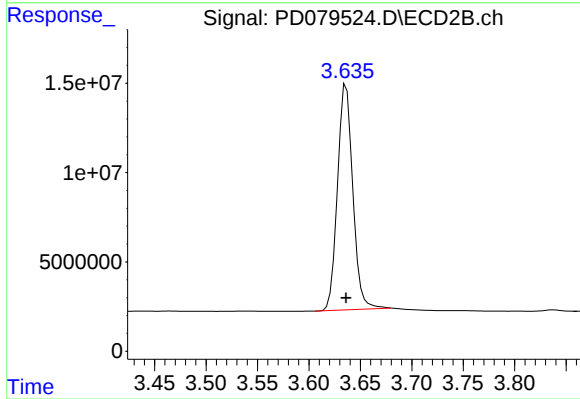


#3 gamma-BHC (Lindane)

R.T.: 3.636 min
Delta R.T.: 0.000 min
Response: 130951125
Conc: 41.28 ng/ml

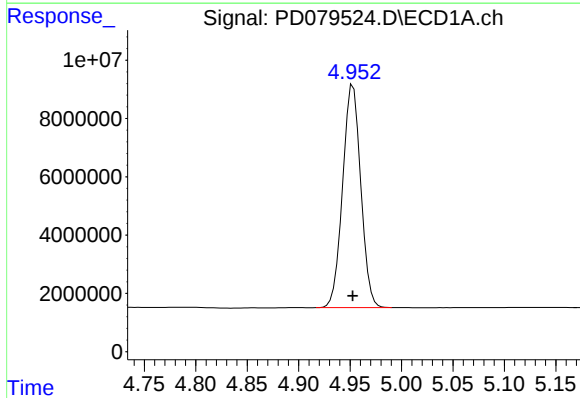


#4 Heptachlor

R.T.: 4.953 min
Delta R.T.: 0.000 min
Response: 93898728
Conc: 40.65 ng/ml

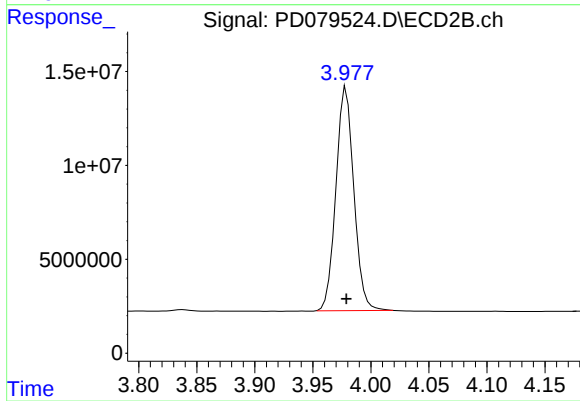


#4 Heptachlor

R.T.: 3.979 min
Delta R.T.: 0.000 min
Response: 128134437
Conc: 41.33 ng/ml

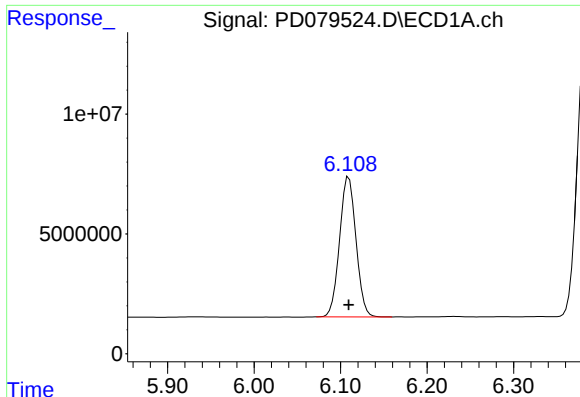


#9 Endosulfan I

R.T.: 6.109 min
Delta R.T.: 0.000 min
Response: 76629537
Conc: 39.24 ng/ml

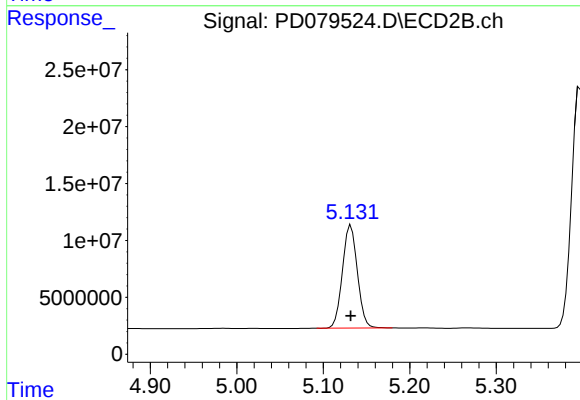


#9 Endosulfan I

R.T.: 5.132 min
Delta R.T.: 0.000 min
Response: 107849111
Conc: 40.66 ng/ml

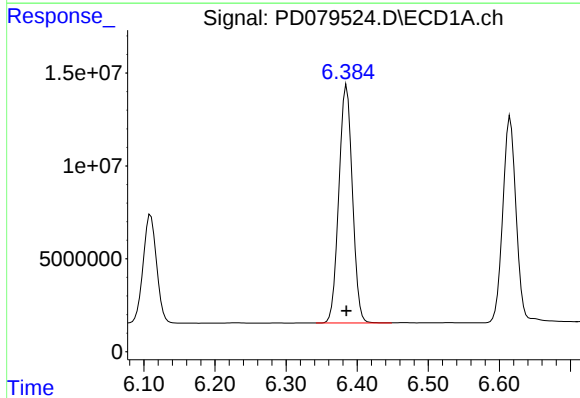


#13 Dieldrin

R.T.: 6.385 min
Delta R.T.: 0.000 min
Response: 169243262
Conc: 82.85 ng/ml

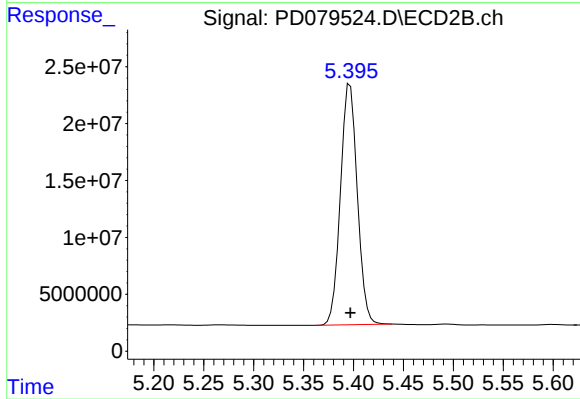


#13 Dieldrin

R.T.: 5.397 min
Delta R.T.: 0.000 min
Response: 249050731
Conc: 83.48 ng/ml

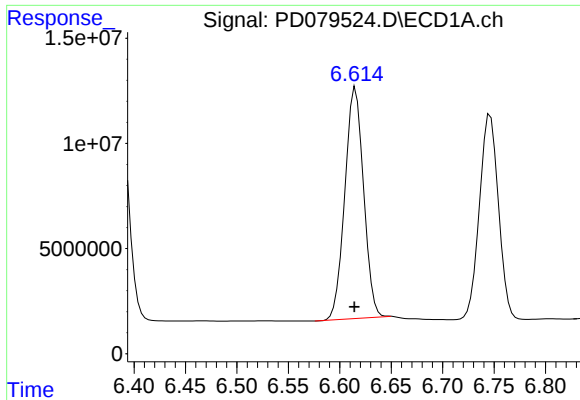


#14 Endrin

R.T.: 6.615 min
Delta R.T.: 0.000 min
Response: 139387716
Conc: 82.17 ng/ml

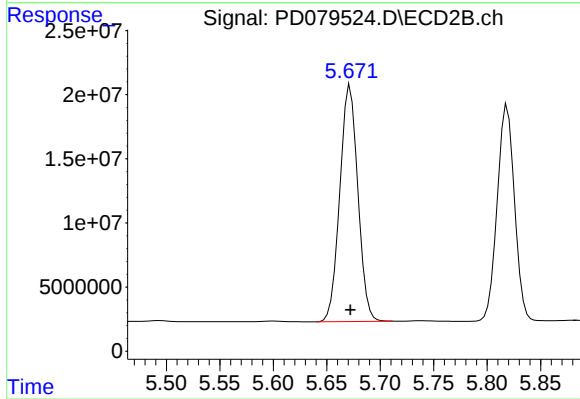


#14 Endrin

R.T.: 5.672 min
Delta R.T.: 0.000 min
Response: 216793666
Conc: 83.06 ng/ml

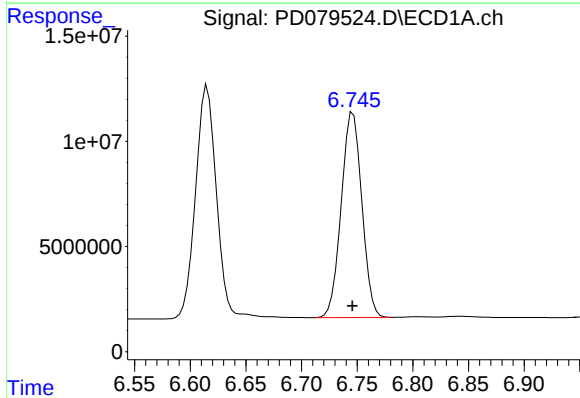


#16 4,4'-DDD

R.T.: 6.746 min
Delta R.T.: 0.000 min
Response: 125713678
Conc: 83.15 ng/ml

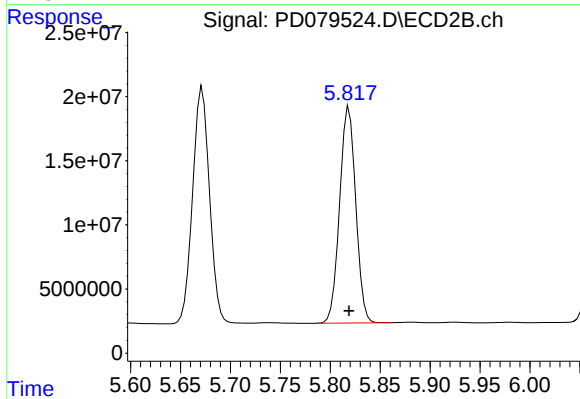


#16 4,4'-DDD

R.T.: 5.819 min
Delta R.T.: 0.000 min
Response: 189214202
Conc: 84.18 ng/ml

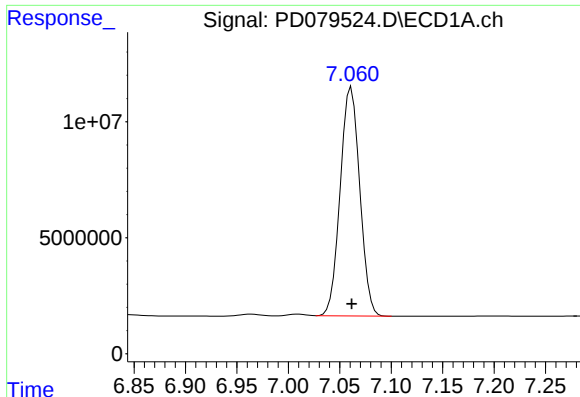


#17 4,4'-DDT

R.T.: 7.061 min
Delta R.T.: 0.000 min
Response: 130536160
Conc: 83.19 ng/ml

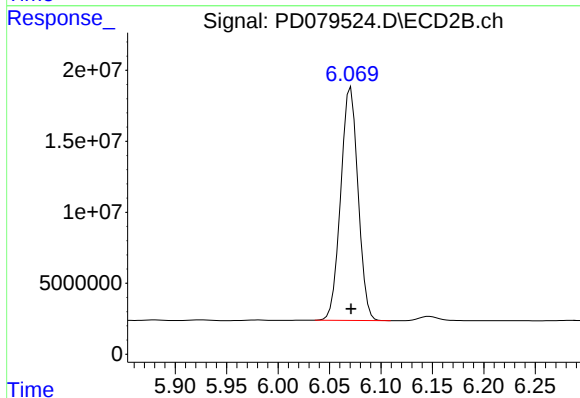


#17 4,4'-DDT

R.T.: 6.071 min
Delta R.T.: 0.000 min
Response: 192484286
Conc: 84.42 ng/ml

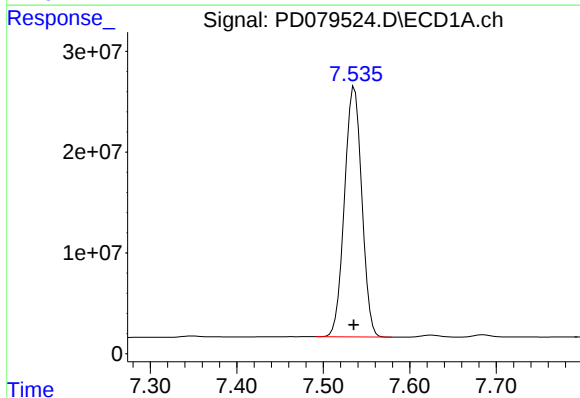


#20 Methoxychlor

R.T.: 7.536 min
Delta R.T.: 0.000 min
Response: 343644719
Conc: 401.12 ng/ml

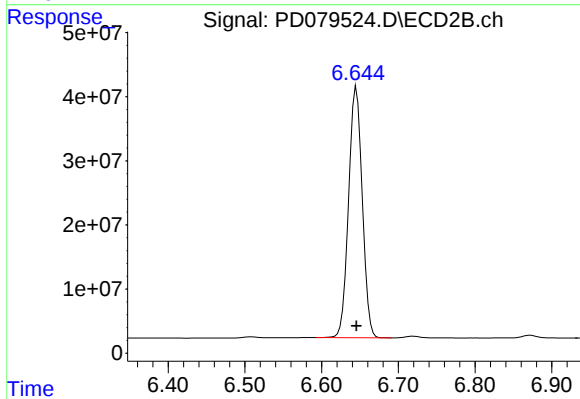


#20 Methoxychlor

R.T.: 6.645 min
Delta R.T.: 0.000 min
Response: 487814030
Conc: 391.31 ng/ml

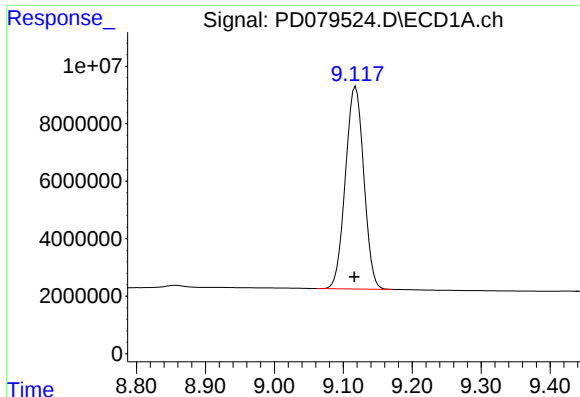

#27 Decachlorobiphenyl

R.T.: 9.118 min
Delta R.T.: 0.002 min
Response: 130516343
Conc: 79.23 ng/ml

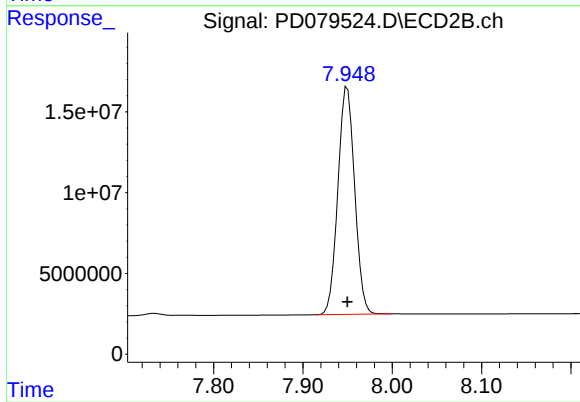

#27 Decachlorobiphenyl

R.T.: 7.950 min
Delta R.T.: 0.000 min
Response: 183750671
Conc: 79.93 ng/ml