

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111023\
 Data File : PD079525.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2023 20:47
 Operator : AR\AJ
 Sample : INDB401
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 21:44:33 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111023CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 07 21:42:20 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	0.000	55824207	0	39.770	N.D. #
27)	SA Decachlor...	9.116	7.949	134.2E6	187.1E6	78.616	78.511
Target Compounds							
5)	MB Aldrin	5.296	4.259	90293384	130.3E6	40.942	41.604
6)	B beta-BHC	4.552	3.931	39661166	38511476	38.728	23.943 #
7)	B delta-BHC	4.802	4.162	96747273	142.7E6	40.036	41.480
8)	B Heptachlo...	5.722	4.761	83755234	114.9E6	39.942	38.090
10)	B trans-Chl...	5.977	5.012	81744648	115.2E6	40.470	39.864
11)	B cis-Chlor...	6.058	5.076	82979980	119.7E6	40.233	39.806
12)	B 4,4'-DDE	6.228	5.265	158.3E6	193.9E6	83.491	70.531
15)	B Endosulfa...	6.832	5.964	144.4E6	173.4E6	80.064	68.587
18)	B Endrin al...	6.962	6.143	113.2E6	159.8E6	79.074	80.544
19)	B Endosulfa...	7.196	6.366	141.0E6	171.0E6	80.050	70.927
21)	B Endrin ke...	7.684	6.872	153.5E6	225.8E6	80.197	81.208


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111023\
Data File : PD079525.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2023 20:47
Operator : AR\AJ
Sample : INDB401
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 21:44:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111023CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Tue Nov 07 21:42:20 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

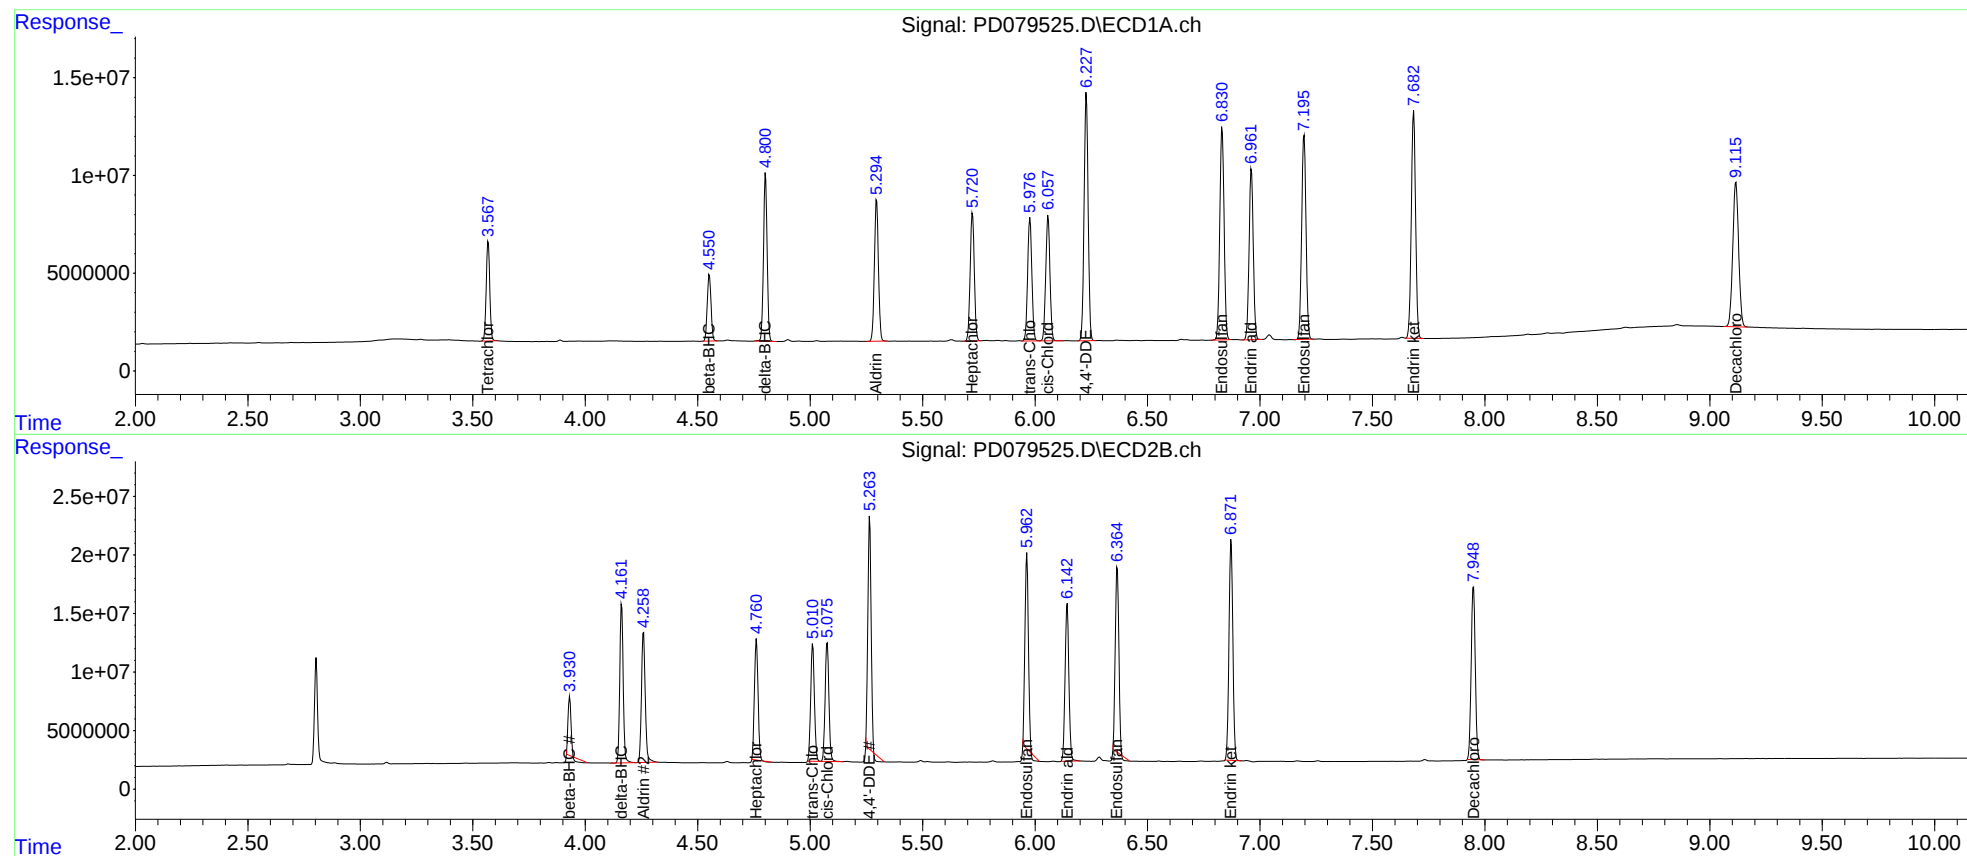

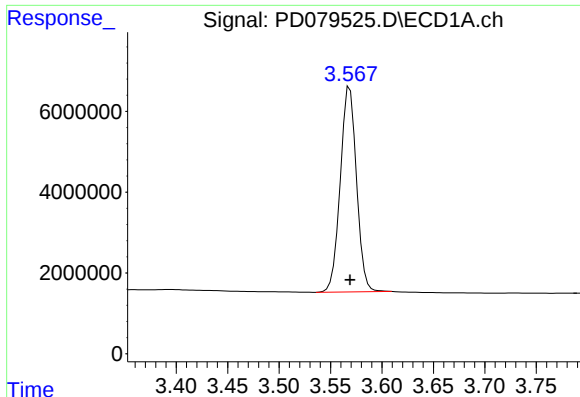


#1 Tetrachloro-m-xylene

R.T.: 3.569 min
Delta R.T.: 0.000 min
Response: 55824207
Conc: 39.77 ng/ml

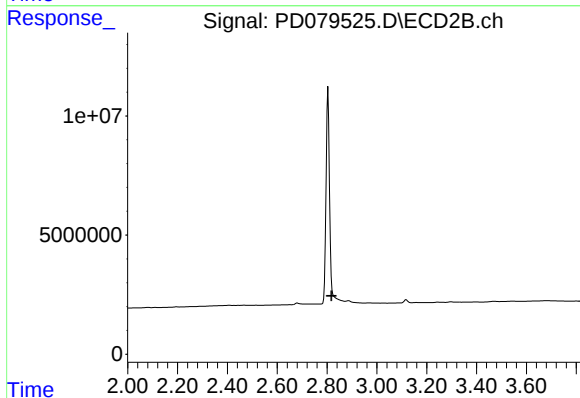


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 2.817 min
Response: 0
Conc: N.D.

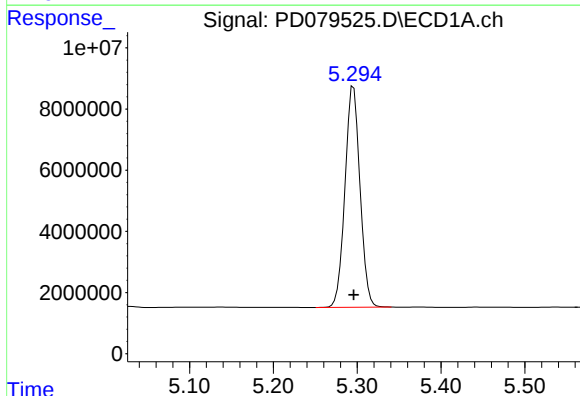


#5 Aldrin

R.T.: 5.296 min
Delta R.T.: 0.000 min
Response: 90293384
Conc: 40.94 ng/ml

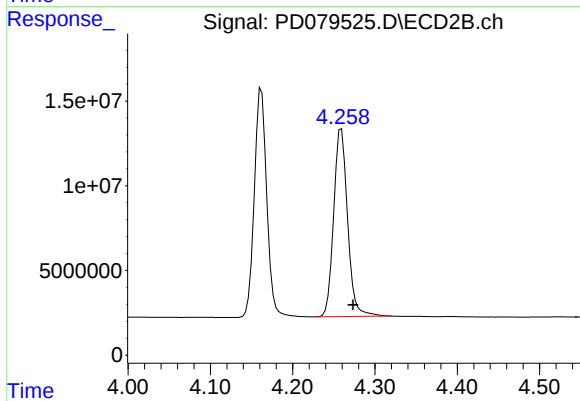


#5 Aldrin

R.T.: 4.259 min
Delta R.T.: -0.014 min
Response: 130292571
Conc: 41.60 ng/ml

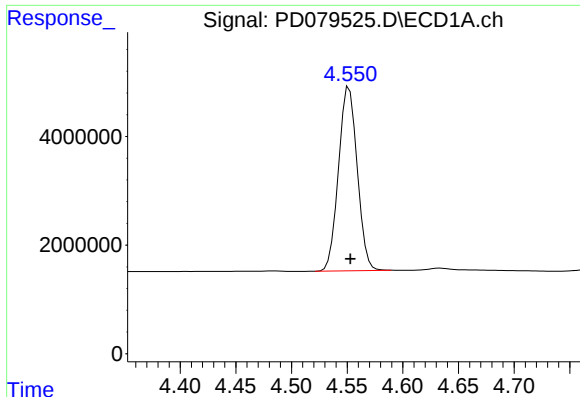


#6 beta-BHC

R.T.: 4.552 min
Delta R.T.: -0.001 min
Response: 39661166
Conc: 38.73 ng/ml

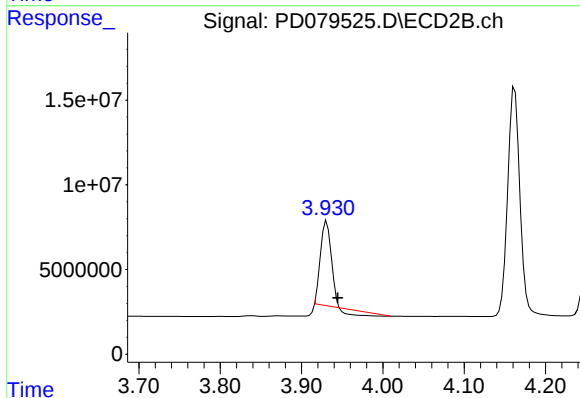


#6 beta-BHC

R.T.: 3.931 min
Delta R.T.: -0.014 min
Response: 38511476
Conc: 23.94 ng/ml

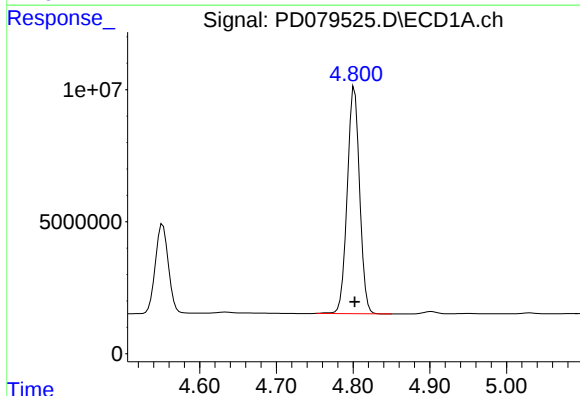


#7 delta-BHC

R.T.: 4.802 min
Delta R.T.: 0.000 min
Response: 96747273
Conc: 40.04 ng/ml

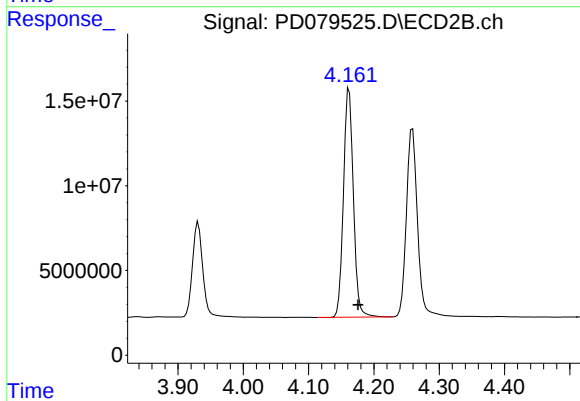


#7 delta-BHC

R.T.: 4.162 min
Delta R.T.: -0.014 min
Response: 142650648
Conc: 41.48 ng/ml

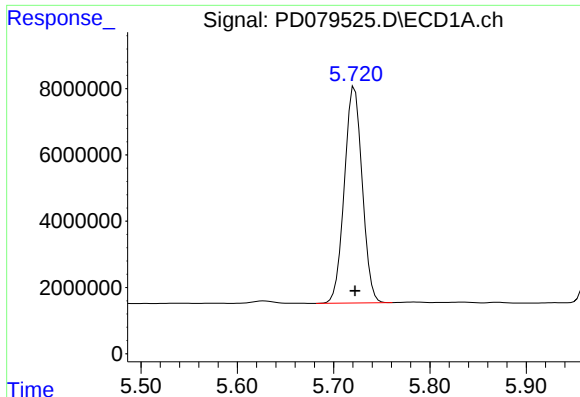


#8 Heptachlor epoxide

R.T.: 5.722 min
Delta R.T.: 0.000 min
Response: 83755234
Conc: 39.94 ng/ml

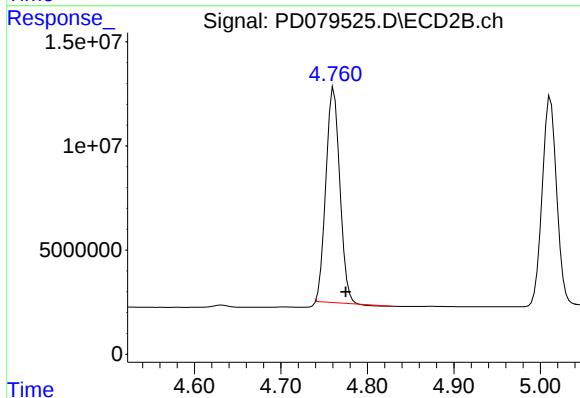


#8 Heptachlor epoxide

R.T.: 4.761 min
Delta R.T.: -0.014 min
Response: 114923646
Conc: 38.09 ng/ml

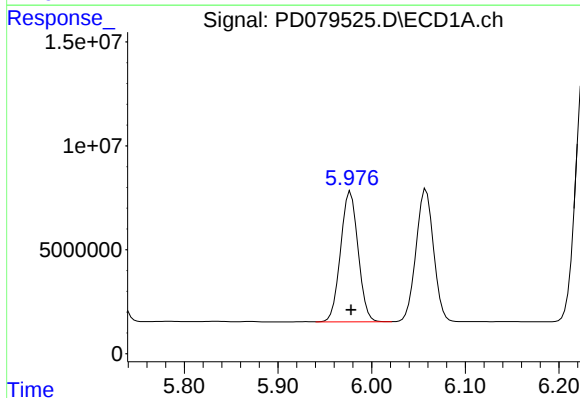


#10 trans-Chlordane

R.T.: 5.977 min
Delta R.T.: 0.000 min
Response: 81744648
Conc: 40.47 ng/ml

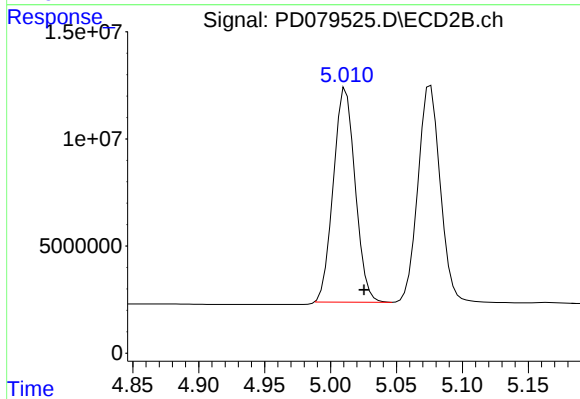


#10 trans-Chlordane

R.T.: 5.012 min
Delta R.T.: -0.014 min
Response: 115175201
Conc: 39.86 ng/ml

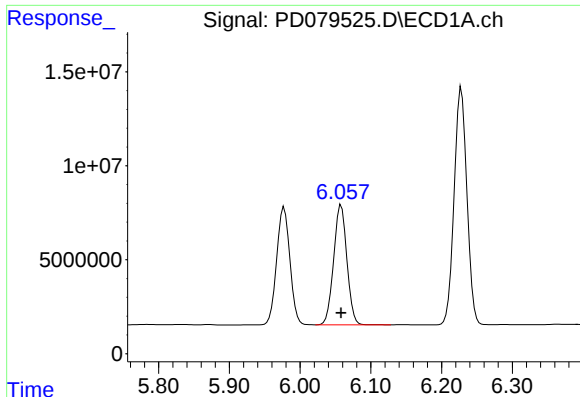


#11 cis-Chlordane

R.T.: 6.058 min
Delta R.T.: 0.000 min
Response: 82979980
Conc: 40.23 ng/ml

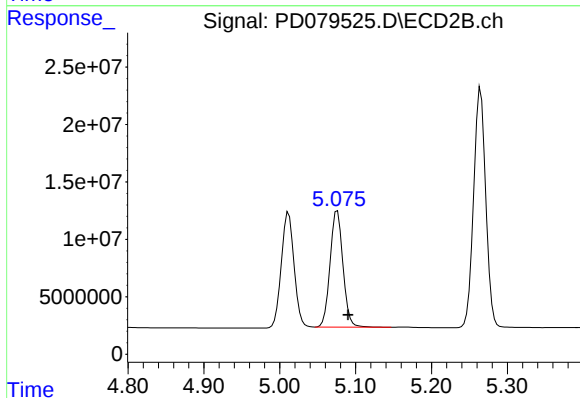


#11 cis-Chlordane

R.T.: 5.076 min
Delta R.T.: -0.014 min
Response: 119675666
Conc: 39.81 ng/ml

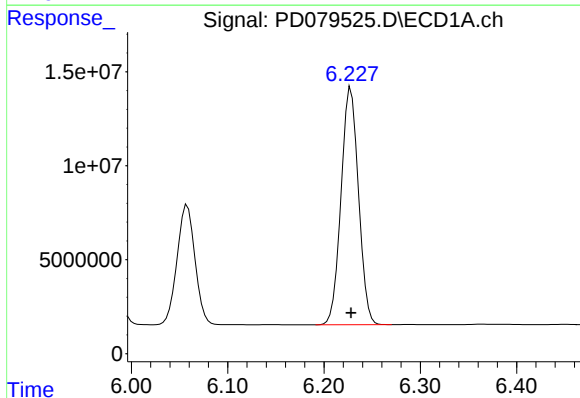


#12 4,4'-DDE

R.T.: 6.228 min
Delta R.T.: 0.000 min
Response: 158266896
Conc: 83.49 ng/ml

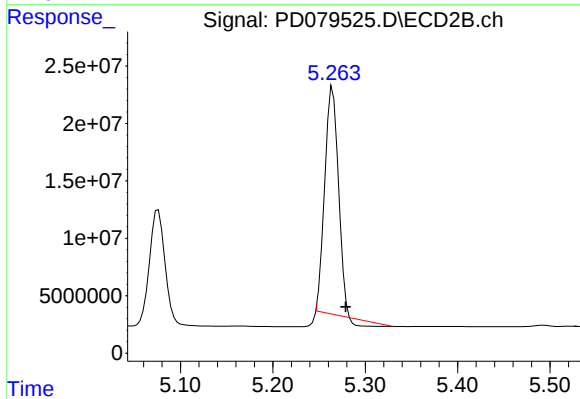


#12 4,4'-DDE

R.T.: 5.265 min
Delta R.T.: -0.014 min
Response: 193866719
Conc: 70.53 ng/ml

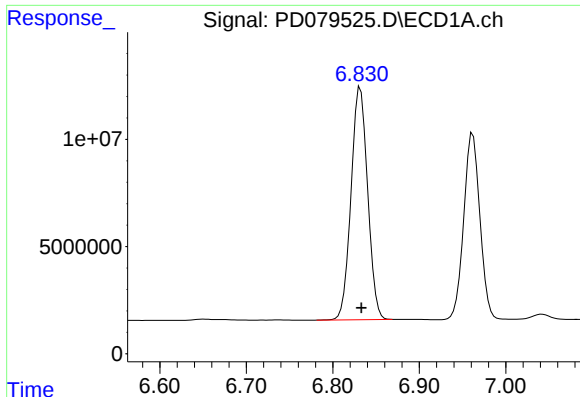


#15 Endosulfan II

R.T.: 6.832 min
Delta R.T.: 0.000 min
Response: 144437507
Conc: 80.06 ng/ml

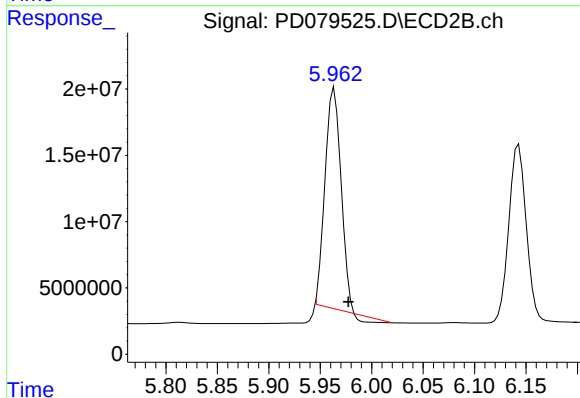


#15 Endosulfan II

R.T.: 5.964 min
Delta R.T.: -0.014 min
Response: 173417768
Conc: 68.59 ng/ml

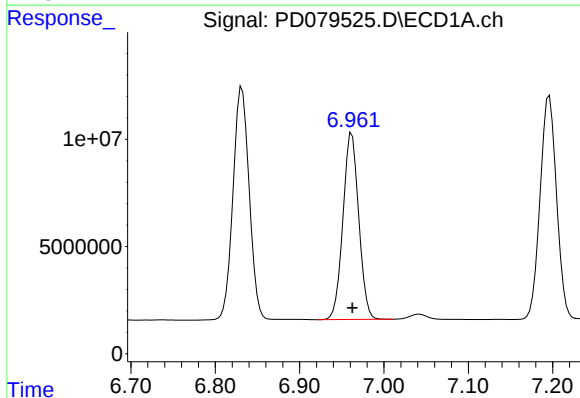


#18 Endrin aldehyde

R.T.: 6.962 min
Delta R.T.: 0.000 min
Response: 113152876
Conc: 79.07 ng/ml

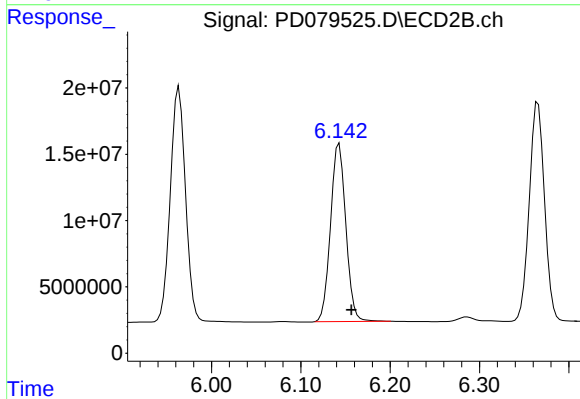


#18 Endrin aldehyde

R.T.: 6.143 min
Delta R.T.: -0.014 min
Response: 159786750
Conc: 80.54 ng/ml

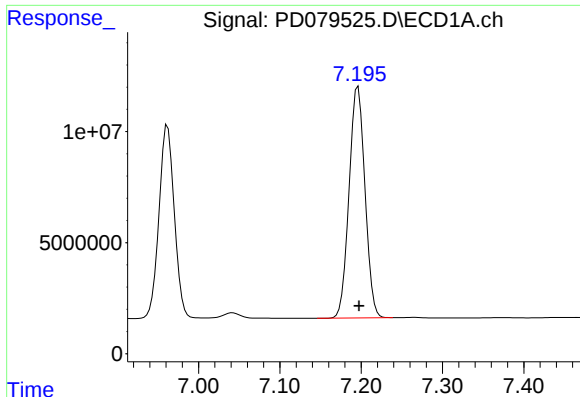


#19 Endosulfan Sulfate

R.T.: 7.196 min
Delta R.T.: -0.001 min
Response: 140983902
Conc: 80.05 ng/ml

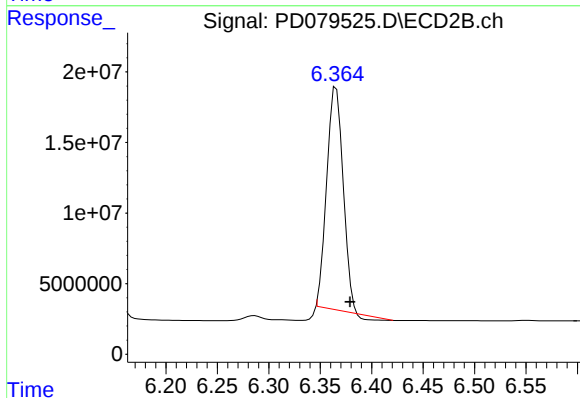


#19 Endosulfan Sulfate

R.T.: 6.366 min
Delta R.T.: -0.014 min
Response: 170988355
Conc: 70.93 ng/ml

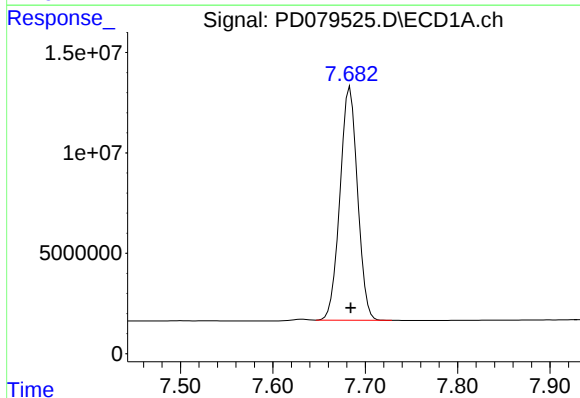


#21 Endrin ketone

R.T.: 7.684 min
Delta R.T.: 0.000 min
Response: 153510191
Conc: 80.20 ng/ml

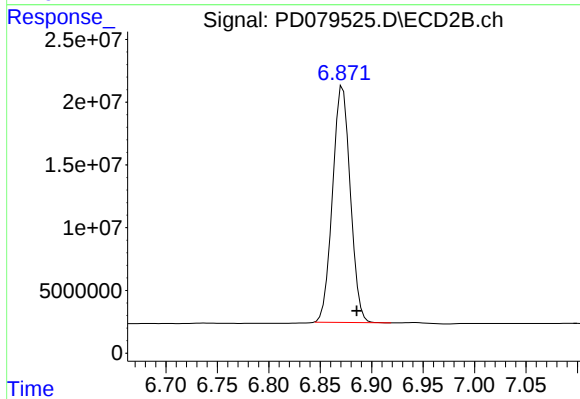


#21 Endrin ketone

R.T.: 6.872 min
Delta R.T.: -0.013 min
Response: 225836753
Conc: 81.21 ng/ml

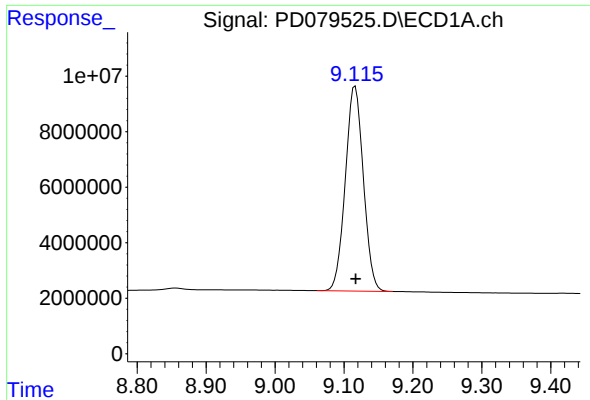

#27 Decachlorobiphenyl

R.T.: 9.116 min
Delta R.T.: 0.000 min
Response: 134209775
Conc: 78.62 ng/ml

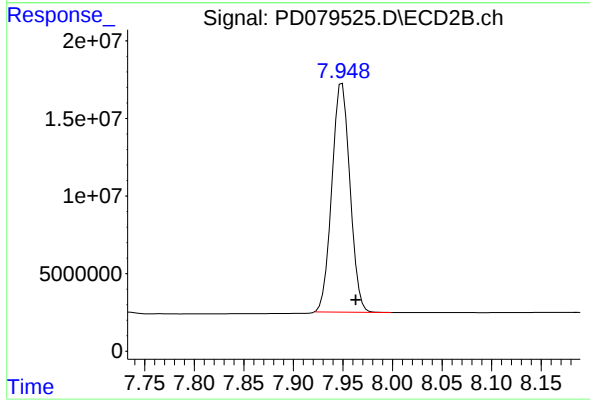

#27 Decachlorobiphenyl

R.T.: 7.949 min
Delta R.T.: -0.014 min
Response: 187071198
Conc: 78.51 ng/ml