

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111023\
 Data File : PD079526.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2023 21:00
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 01:05:32 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111023CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 08 01:02:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	2.804	106.7E6	168.4E6	77.627	78.830
27)	SA Decachlor...	9.116	7.949	252.9E6	358.8E6	153.546	156.084
Target Compounds							
2)	A alpha-BHC	4.025	3.307	198.8E6	289.7E6	87.474	85.331
3)	MA gamma-BHC...	4.359	3.636	185.1E6	266.7E6	85.166	84.070
4)	MA Heptachlor	4.952	3.979	188.2E6	257.5E6	81.474	83.055
9)	A Endosulfan I	6.109	5.132	150.2E6	214.8E6	76.896	80.977
13)	MA Dieldrin	6.384	5.396	342.3E6	501.0E6	167.570	167.936
14)	MA Endrin	6.615	5.672	281.6E6	433.8E6	166.003	166.186
16)	A 4,4'-DDD	6.745	5.818	253.8E6	380.2E6	167.877	169.134
17)	MA 4,4'-DDT	7.061	6.070	265.6E6	391.7E6	169.282	171.813
20)	A Methoxychlor	7.535	6.645	671.1E6	908.6E6	783.298	728.848


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111023\
Data File : PD079526.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2023 21:00
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 01:05:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111023CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 08 01:02:54 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

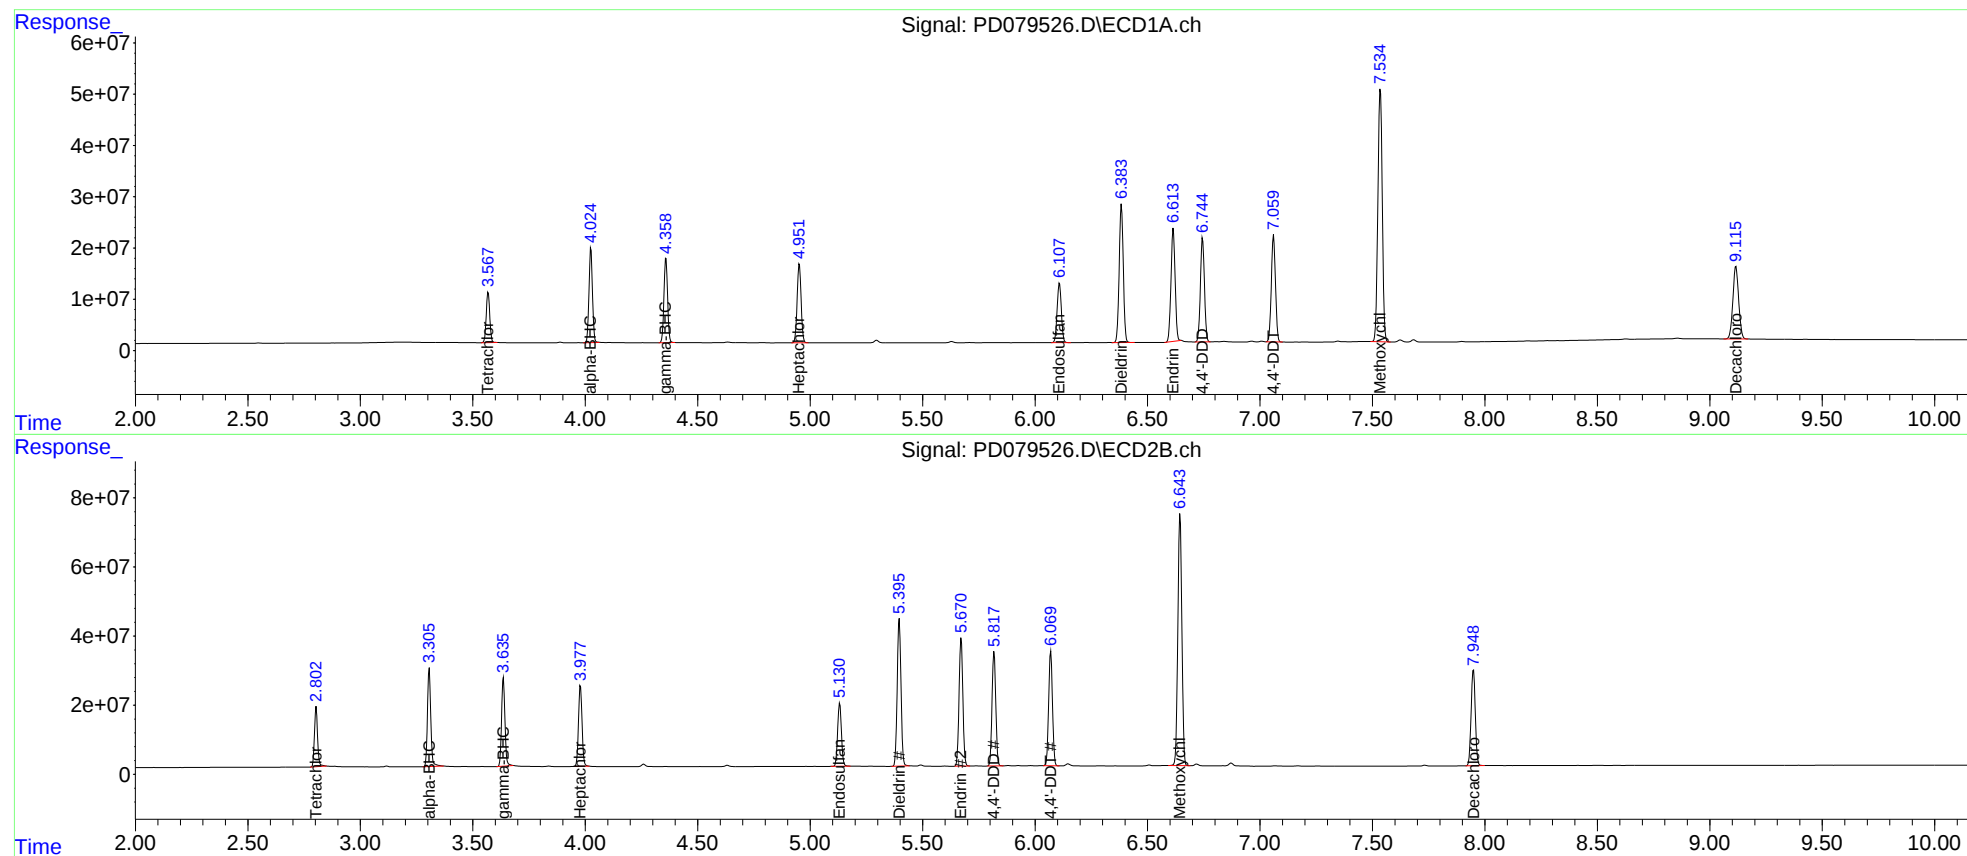

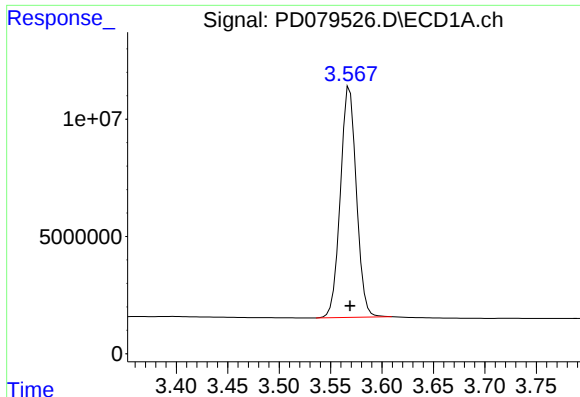


#1 Tetrachloro-m-xylene

R.T.: 3.569 min
Delta R.T.: 0.000 min
Response: 106665384
Conc: 77.63 ng/ml

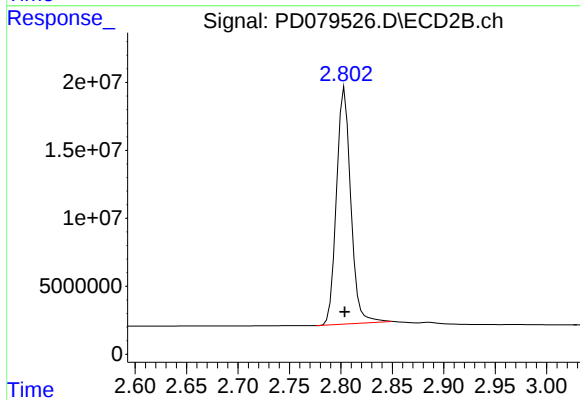


#1 Tetrachloro-m-xylene

R.T.: 2.804 min
Delta R.T.: 0.000 min
Response: 168437385
Conc: 78.83 ng/ml

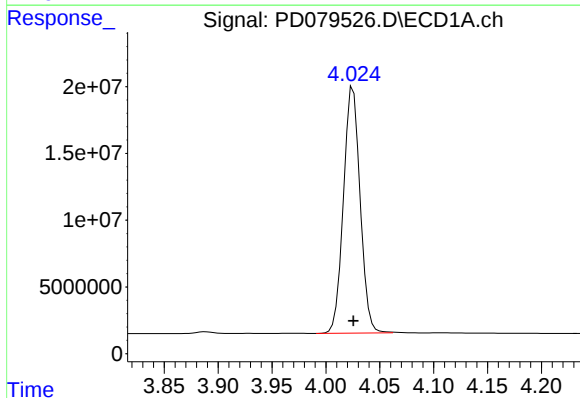


#2 alpha-BHC

R.T.: 4.025 min
Delta R.T.: 0.000 min
Response: 198841051
Conc: 87.47 ng/ml

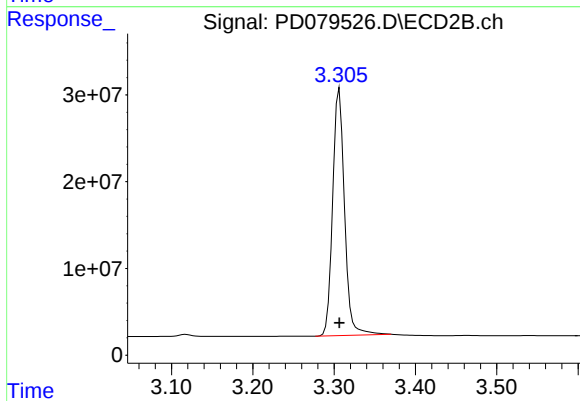


#2 alpha-BHC

R.T.: 3.307 min
Delta R.T.: 0.000 min
Response: 289676376
Conc: 85.33 ng/ml

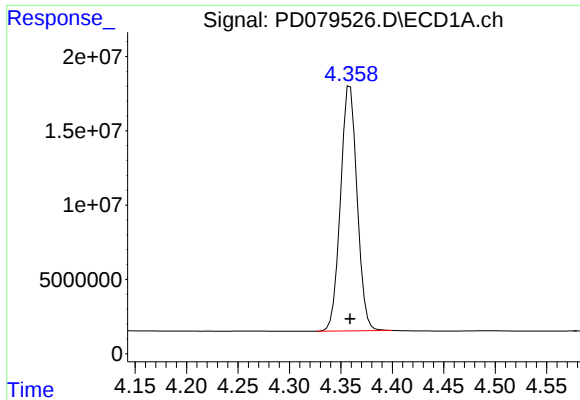


#3 gamma-BHC (Lindane)

R.T.: 4.359 min
Delta R.T.: 0.000 min
Response: 185092931
Conc: 85.17 ng/ml

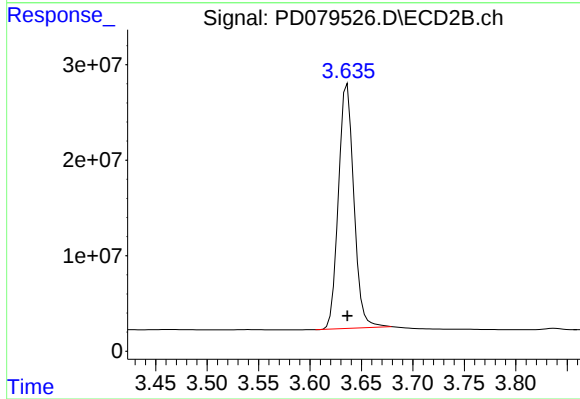


#3 gamma-BHC (Lindane)

R.T.: 3.636 min
Delta R.T.: 0.000 min
Response: 266717190
Conc: 84.07 ng/ml

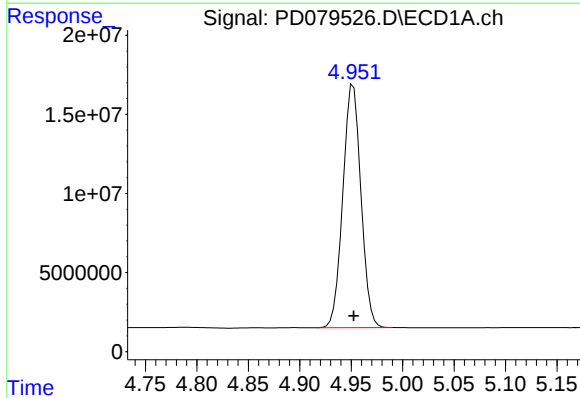


#4 Heptachlor

R.T.: 4.952 min
Delta R.T.: 0.000 min
Response: 188205139
Conc: 81.47 ng/ml

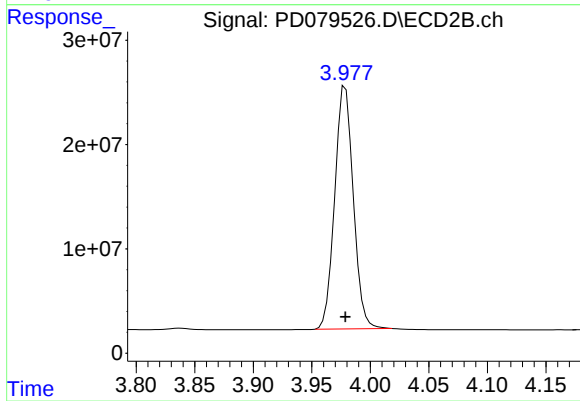


#4 Heptachlor

R.T.: 3.979 min
Delta R.T.: 0.000 min
Response: 257522553
Conc: 83.06 ng/ml

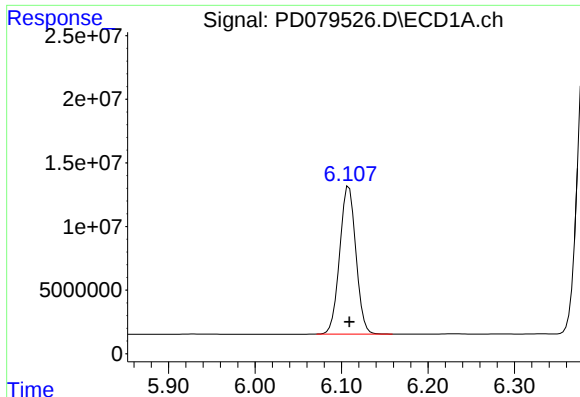


#9 Endosulfan I

R.T.: 6.109 min
Delta R.T.: 0.000 min
Response: 150157333
Conc: 76.90 ng/ml

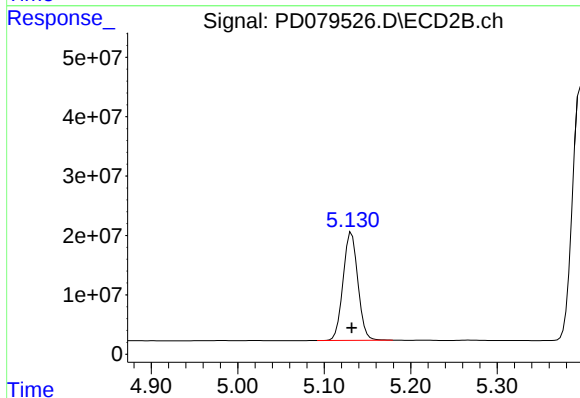


#9 Endosulfan I

R.T.: 5.132 min
Delta R.T.: 0.000 min
Response: 214805153
Conc: 80.98 ng/ml

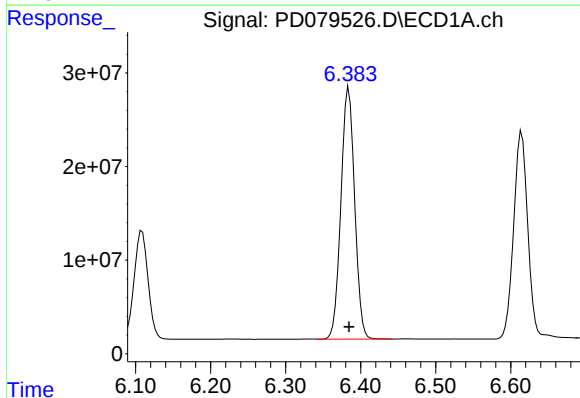


#13 Dieldrin

R.T.: 6.384 min
Delta R.T.: 0.000 min
Response: 342293782
Conc: 167.57 ng/ml

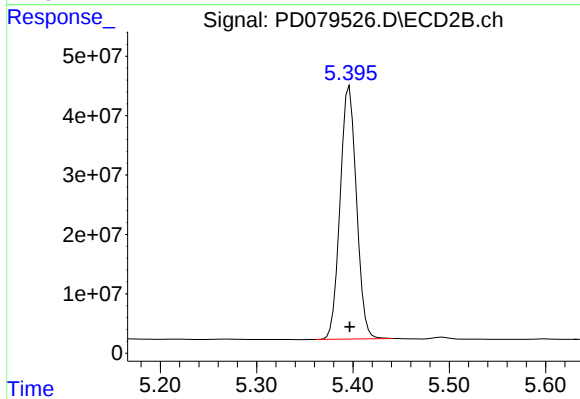


#13 Dieldrin

R.T.: 5.396 min
Delta R.T.: 0.000 min
Response: 501018383
Conc: 167.94 ng/ml

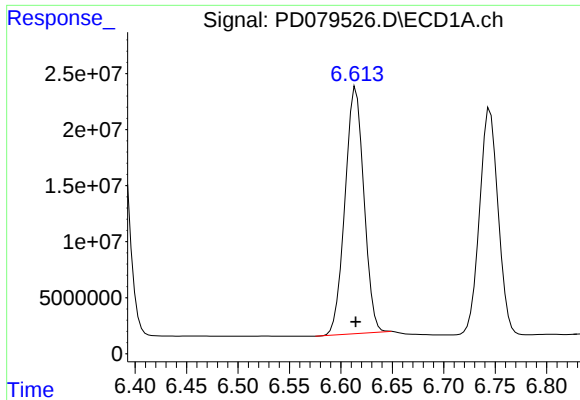


#14 Endrin

R.T.: 6.615 min
Delta R.T.: 0.000 min
Response: 281595817
Conc: 166.00 ng/ml

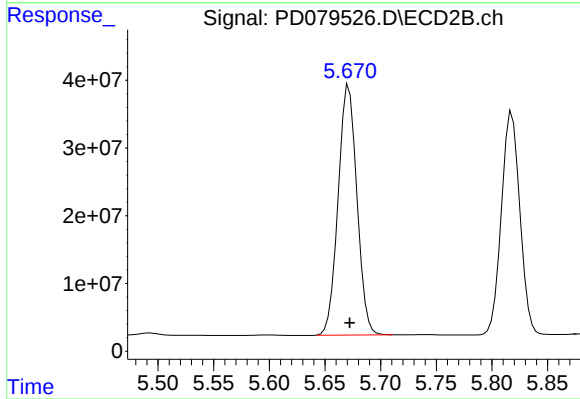


#14 Endrin

R.T.: 5.672 min
Delta R.T.: 0.000 min
Response: 433784538
Conc: 166.19 ng/ml

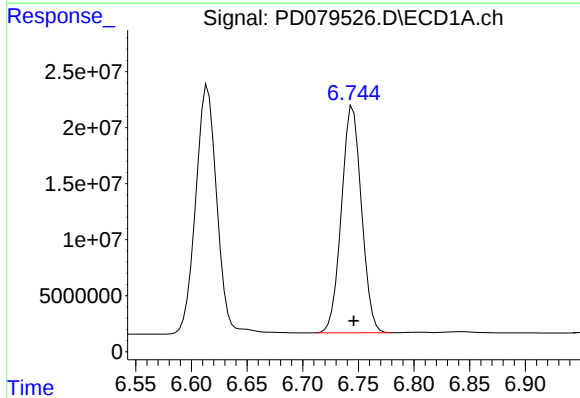


#16 4,4'-DDD

R.T.: 6.745 min
Delta R.T.: 0.000 min
Response: 253813696
Conc: 167.88 ng/ml

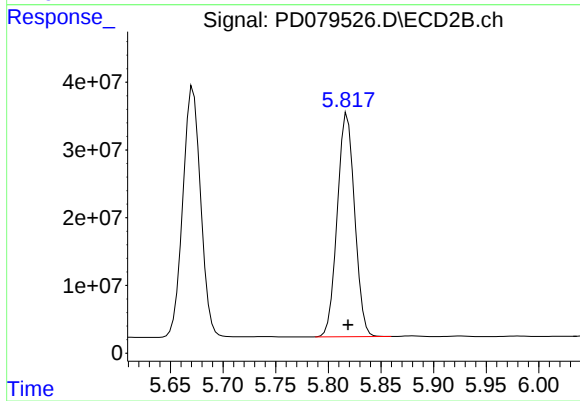


#16 4,4'-DDD

R.T.: 5.818 min
Delta R.T.: 0.000 min
Response: 380188289
Conc: 169.13 ng/ml

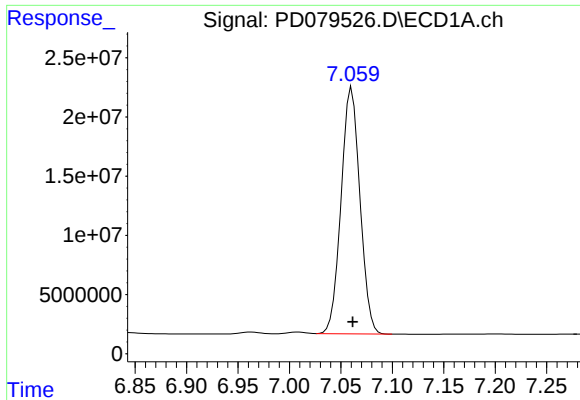


#17 4,4'-DDT

R.T.: 7.061 min
Delta R.T.: 0.000 min
Response: 265621228
Conc: 169.28 ng/ml

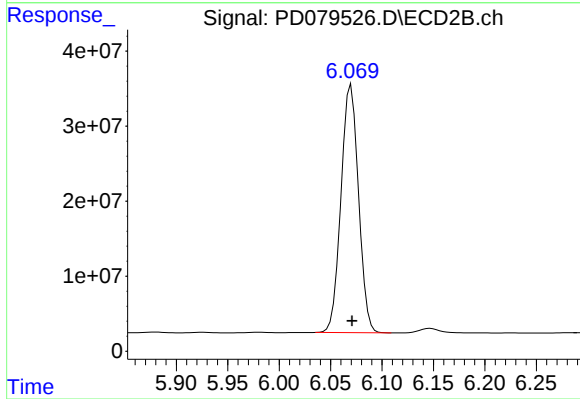


#17 4,4'-DDT

R.T.: 6.070 min
Delta R.T.: 0.000 min
Response: 391728875
Conc: 171.81 ng/ml

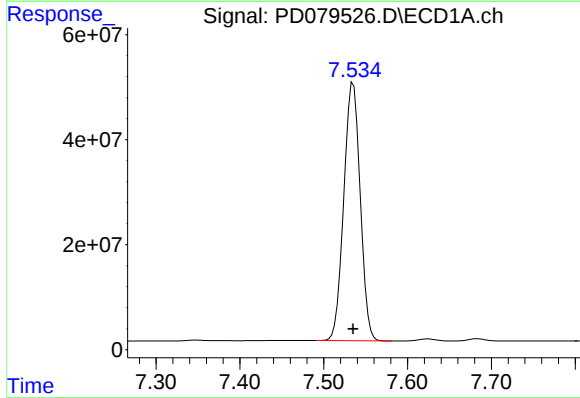


#20 Methoxychlor

R.T.: 7.535 min
Delta R.T.: 0.000 min
Response: 671054544
Conc: 783.30 ng/ml

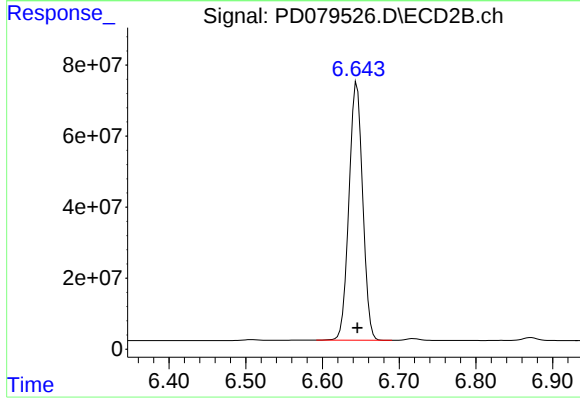

#20 Methoxychlor

R.T.: 6.645 min
Delta R.T.: 0.000 min
Response: 908586092
Conc: 728.85 ng/ml

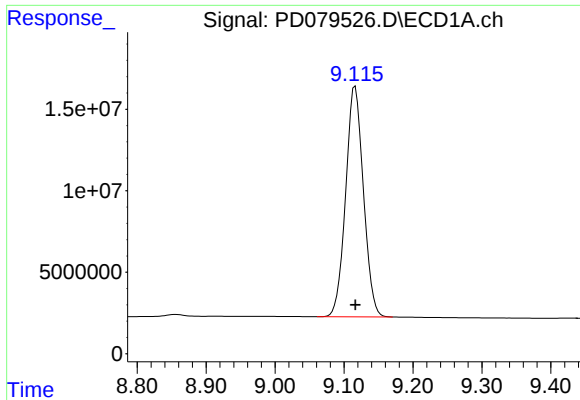


#27 Decachlorobiphenyl

R.T.: 9.116 min

Delta R.T.: 0.000 min

Response: 252946986

Conc: 153.55 ng/ml

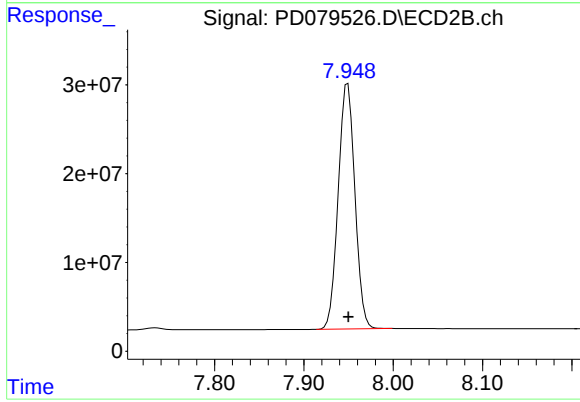

#27 Decachlorobiphenyl

R.T.: 7.949 min

Delta R.T.: 0.000 min

Response: 358828944

Conc: 156.08 ng/ml