

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111023\
 Data File : PD079528.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2023 21:27
 Operator : AR\AJ
 Sample : INDA601
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 01:05:46 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111023CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 08 01:02:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	2.804	216.4E6	339.8E6	157.521	159.052
27)	SA Decachlor...	9.117	7.950	510.3E6	721.7E6	309.769	313.931
Target Compounds							
2)	A alpha-BHC	4.026	3.307	421.8E6	597.8E6	185.563	176.105
3)	MA gamma-BHC...	4.359	3.636	390.6E6	549.9E6	179.728	173.316
4)	MA Heptachlor	4.952	3.979	388.8E6	521.6E6	168.293	168.222
9)	A Endosulfan I	6.109	5.132	303.9E6	435.1E6	155.632	164.022
13)	MA Dieldrin	6.385	5.397	703.4E6	1006.6E6	344.335	337.396
14)	MA Endrin	6.616	5.672	578.8E6	867.5E6	341.209	332.364
16)	A 4,4'-DDD	6.746	5.819	524.3E6	766.3E6	346.766	340.908
17)	MA 4,4'-DDT	7.061	6.070	553.4E6	802.4E6	352.712	351.946
20)	A Methoxychlor	7.536	6.645	1339.2E6	1688.0E6	1563.176	1354.083


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111023\
Data File : PD079528.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2023 21:27
Operator : AR\AJ
Sample : INDA601
Misc :
ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 01:05:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111023CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 08 01:02:54 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

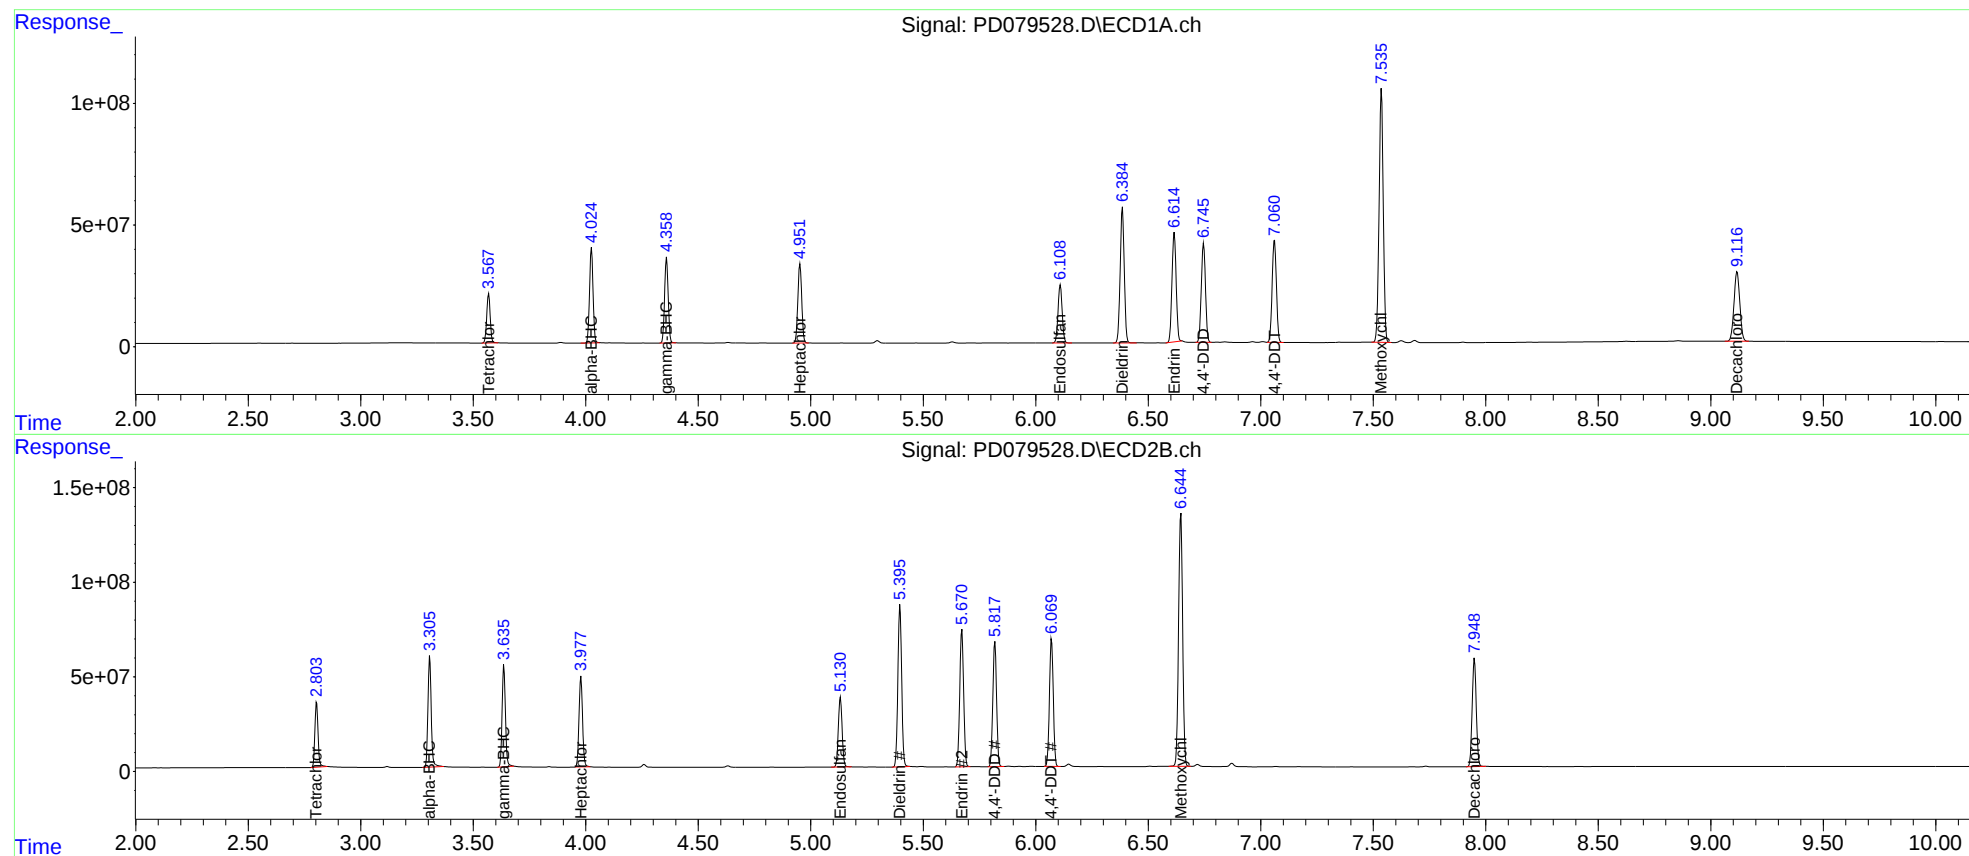

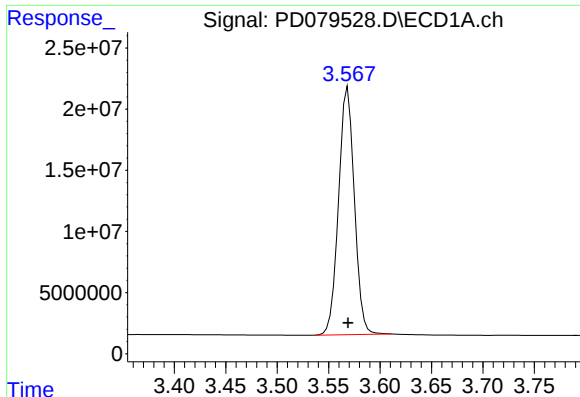


#1 Tetrachloro-m-xylene

R.T.: 3.569 min
Delta R.T.: 0.000 min
Response: 216446712
Conc: 157.52 ng/ml

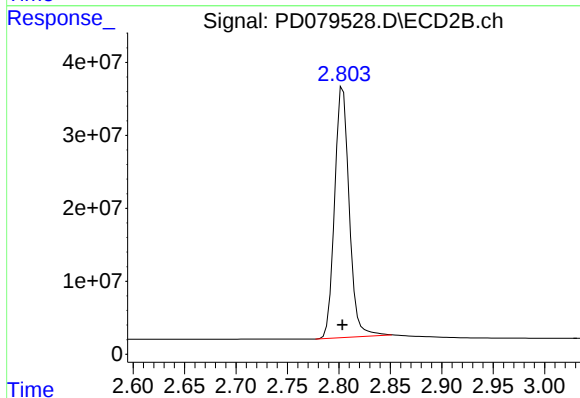


#1 Tetrachloro-m-xylene

R.T.: 2.804 min
Delta R.T.: 0.000 min
Response: 339849343
Conc: 159.05 ng/ml

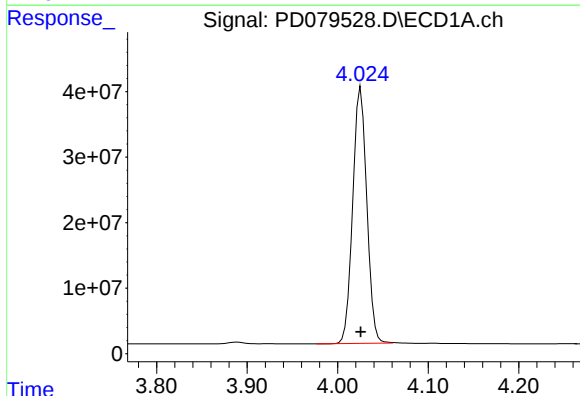


#2 alpha-BHC

R.T.: 4.026 min
Delta R.T.: 0.000 min
Response: 421811054
Conc: 185.56 ng/ml

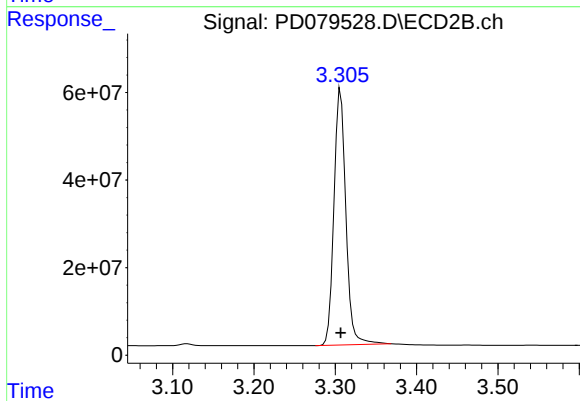


#2 alpha-BHC

R.T.: 3.307 min
Delta R.T.: 0.000 min
Response: 597830360
Conc: 176.11 ng/ml

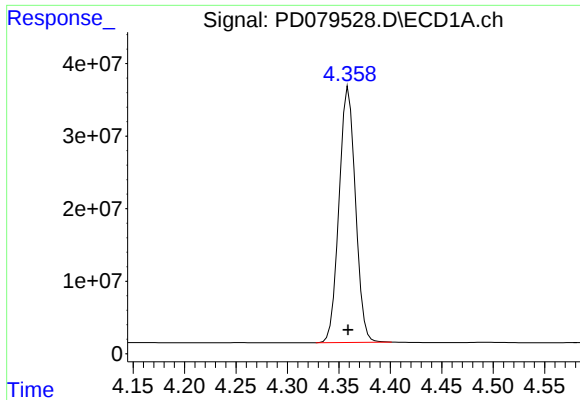


#3 gamma-BHC (Lindane)

R.T.: 4.359 min
Delta R.T.: 0.000 min
Response: 390603570
Conc: 179.73 ng/ml

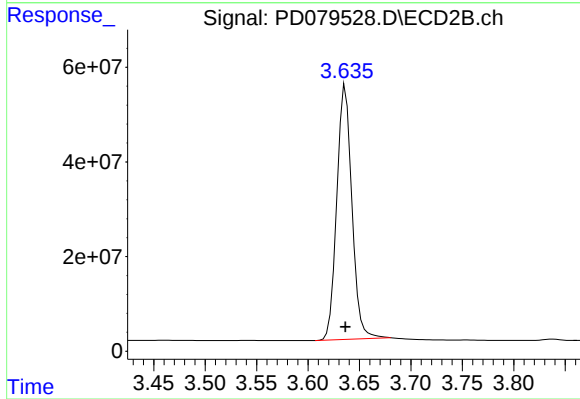


#3 gamma-BHC (Lindane)

R.T.: 3.636 min
Delta R.T.: 0.000 min
Response: 549855439
Conc: 173.32 ng/ml

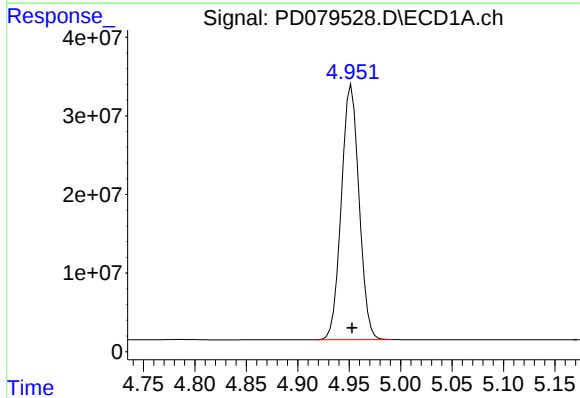


#4 Heptachlor

R.T.: 4.952 min
Delta R.T.: 0.000 min
Response: 388755514
Conc: 168.29 ng/ml

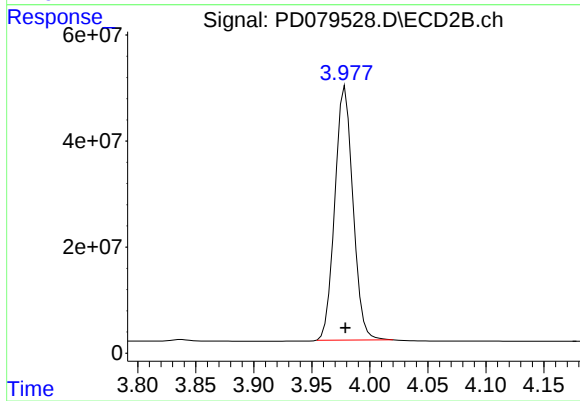


#4 Heptachlor

R.T.: 3.979 min
Delta R.T.: 0.000 min
Response: 521592714
Conc: 168.22 ng/ml

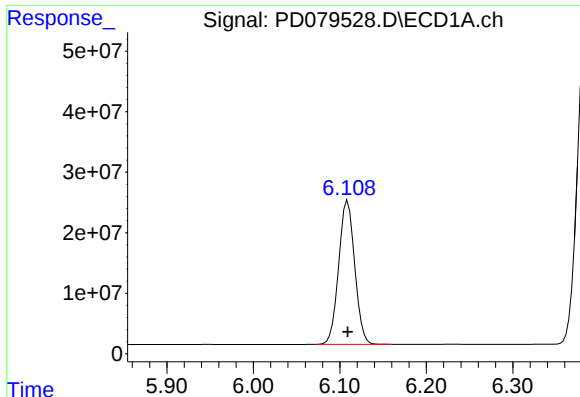


#9 Endosulfan I

R.T.: 6.109 min
Delta R.T.: 0.000 min
Response: 303907295
Conc: 155.63 ng/ml

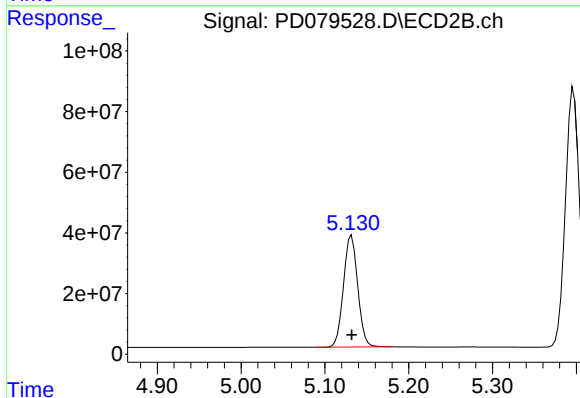


#9 Endosulfan I

R.T.: 5.132 min
Delta R.T.: 0.000 min
Response: 435096412
Conc: 164.02 ng/ml

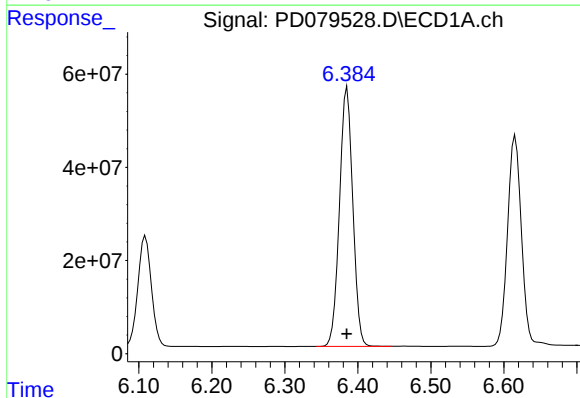


#13 Dieldrin

R.T.: 6.385 min
Delta R.T.: 0.000 min
Response: 703368633
Conc: 344.33 ng/ml

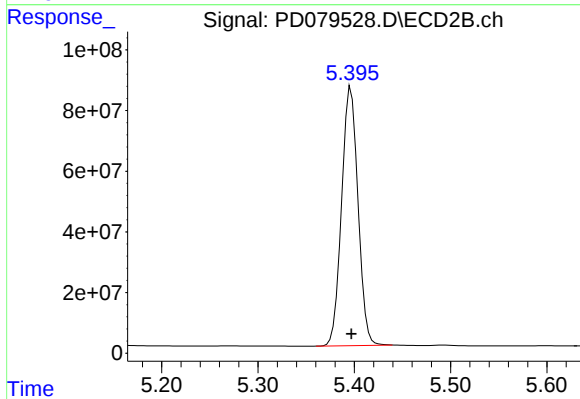


#13 Dieldrin

R.T.: 5.397 min
Delta R.T.: 0.000 min
Response: 1006582920
Conc: 337.40 ng/ml

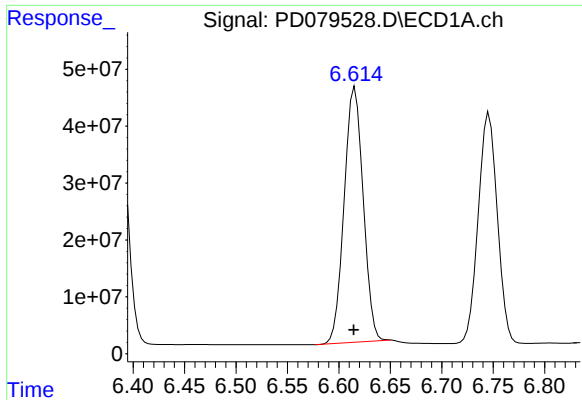


#14 Endrin

R.T.: 6.616 min
Delta R.T.: 0.001 min
Response: 578803927
Conc: 341.21 ng/ml

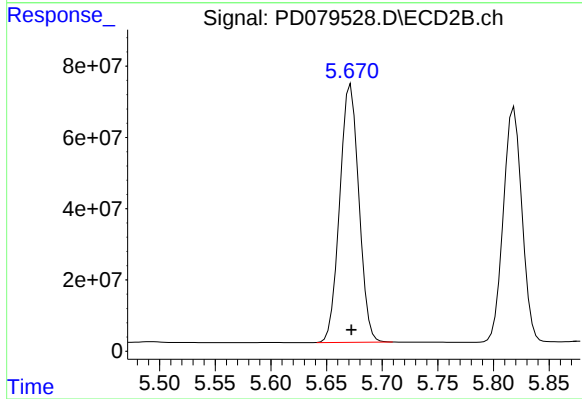


#14 Endrin

R.T.: 5.672 min
Delta R.T.: 0.000 min
Response: 867547457
Conc: 332.36 ng/ml

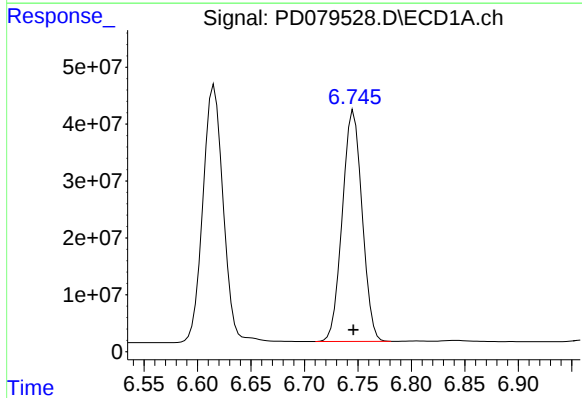


#16 4,4'-DDD

R.T.: 6.746 min
Delta R.T.: 0.000 min
Response: 524278627
Conc: 346.77 ng/ml

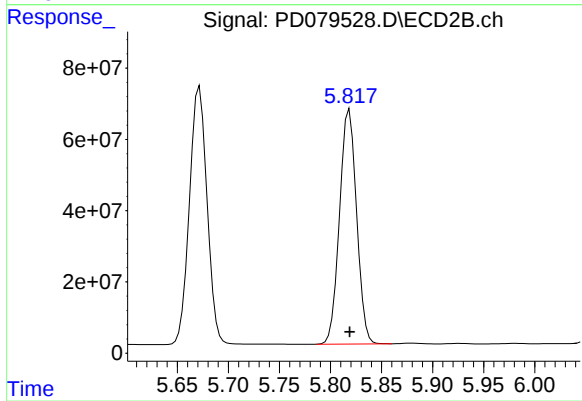


#16 4,4'-DDD

R.T.: 5.819 min
Delta R.T.: 0.000 min
Response: 766310890
Conc: 340.91 ng/ml

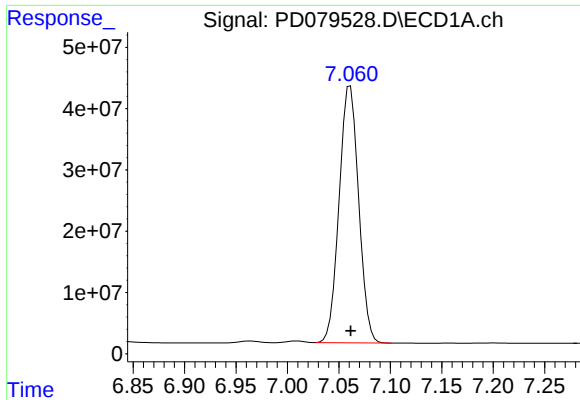


#17 4,4'-DDT

R.T.: 7.061 min
Delta R.T.: 0.000 min
Response: 553444411
Conc: 352.71 ng/ml

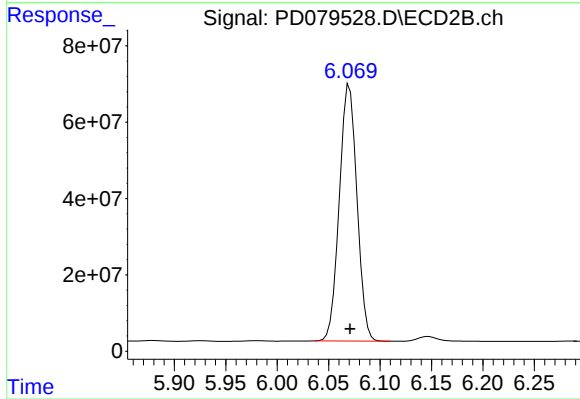


#17 4,4'-DDT

R.T.: 6.070 min
Delta R.T.: 0.000 min
Response: 802427809
Conc: 351.95 ng/ml

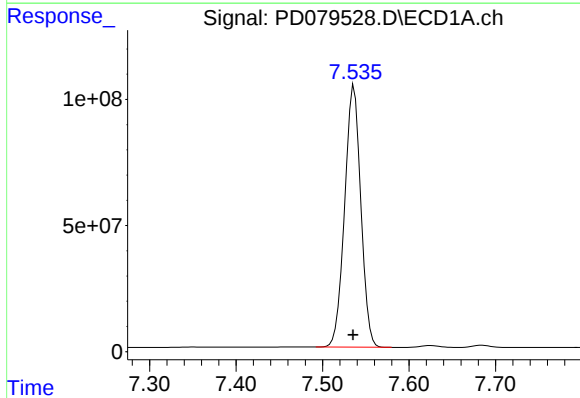


#20 Methoxychlor

R.T.: 7.536 min
Delta R.T.: 0.001 min
Response: 1339179482
Conc: 1563.18 ng/ml

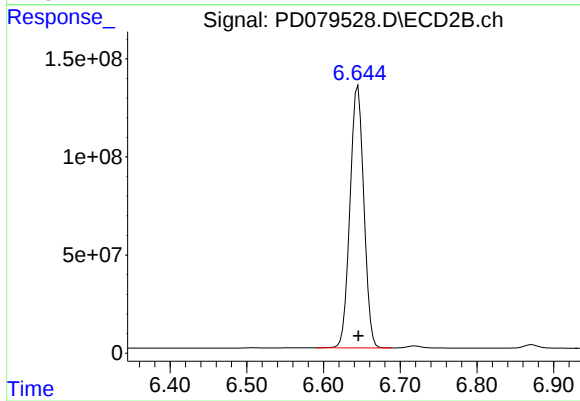


#20 Methoxychlor

R.T.: 6.645 min
Delta R.T.: 0.000 min
Response: 1688007975
Conc: 1354.08 ng/ml

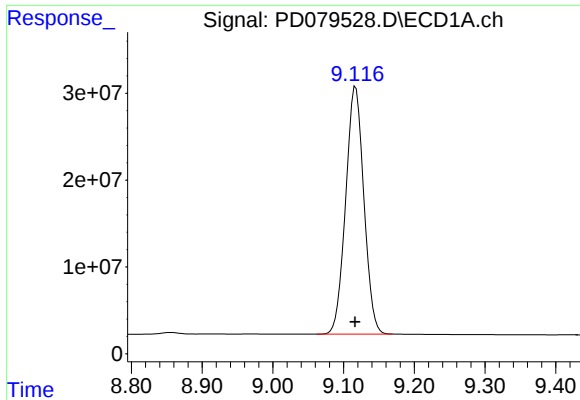

#27 Decachlorobiphenyl

R.T.: 9.117 min
Delta R.T.: 0.000 min
Response: 510303590
Conc: 309.77 ng/ml

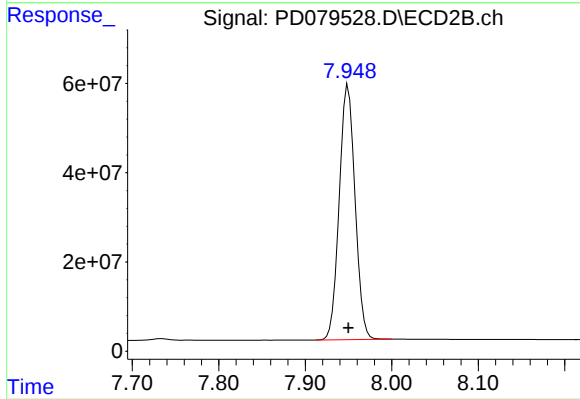

#27 Decachlorobiphenyl

R.T.: 7.950 min
Delta R.T.: 0.000 min
Response: 721710994
Conc: 313.93 ng/ml