

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111023\
 Data File : PD079525.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2023 20:47
 Operator : AR\AJ
 Sample : INDB401
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDB4008

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/08/2023
 Supervised By : Ankita Jodhani 11/08/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 22:13:34 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111023CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 07 22:13:27 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	2.802	55824207	88000792	38.135	39.391m
27)	SA Decachlor...	9.116	7.948	134.2E6	189.3E6	76.621	76.568m
Target Compounds							
5)	MB Aldrin	5.296	4.259	90293384	130.3E6	39.476	40.292
6)	B beta-BHC	4.552	3.930	39661166	59444376	37.156	37.700m
7)	B delta-BHC	4.802	4.162	96747273	142.7E6	40.647	40.949
8)	B Heptachlo...	5.722	4.760	83755234	122.1E6	38.440	39.537m
10)	B trans-Chl...	5.977	5.010	81744648	118.9E6	38.766	40.111m
11)	B cis-Chlor...	6.058	5.076	82979980	119.7E6	38.513	39.040
12)	B 4,4'-DDE	6.228	5.263	158.3E6	231.5E6	81.900	83.114m
15)	B Endosulfa...	6.832	5.962	144.4E6	209.2E6	77.146	80.826m
18)	B Endrin al...	6.962	6.143	113.2E6	159.8E6	76.089	78.699
19)	B Endosulfa...	7.196	6.364	141.0E6	196.0E6	76.930	79.456m
21)	B Endrin ke...	7.684	6.871	153.5E6	227.1E6	77.752	80.289m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111023\
Data File : PD079525.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2023 20:47
Operator : AR\AJ
Sample : INDB401
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 22:13:34 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111023CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Tue Nov 07 22:13:27 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

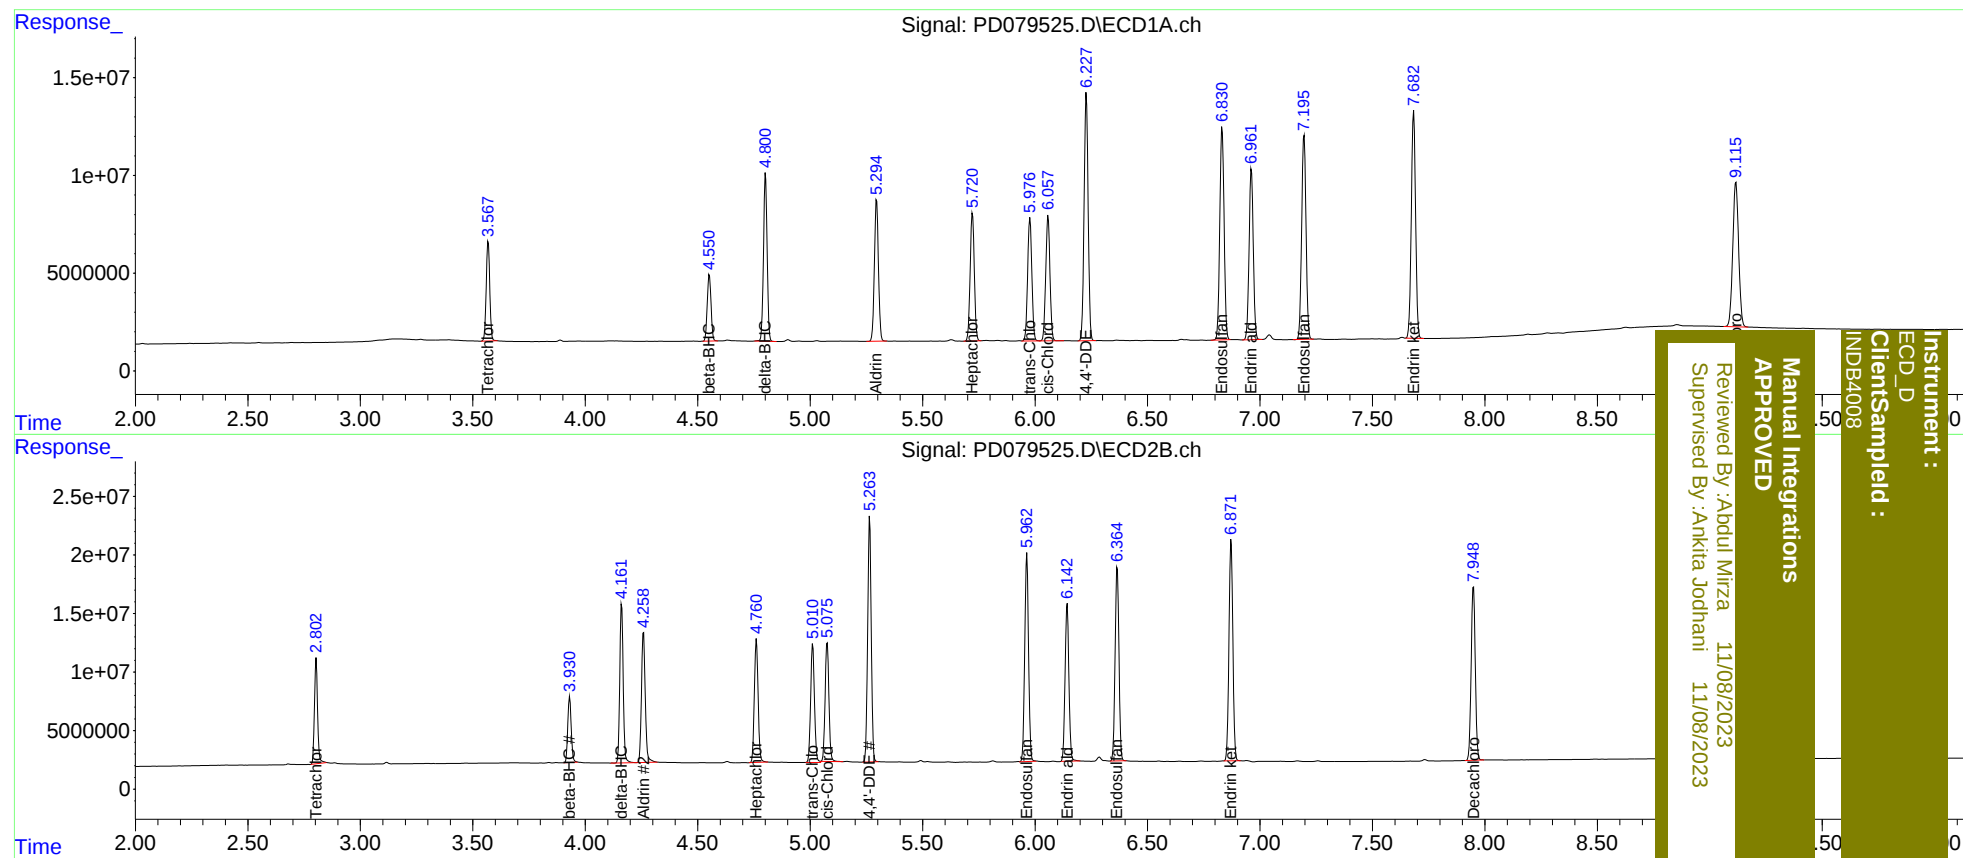

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 11/08/2023
Supervised By: Ankita Jodhani 11/08/2023

Instrument :
ECD_D
ClientSampled :
INDB4008