

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111023\
 Data File : PD079510.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2023 17:27
 Operator : AR\AJ
 Sample : RESC014
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC015

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 04:23:32 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111023CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 08 02:29:03 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	2.804	28512189	44409366	20.430	20.476
2)	SA Decachlor...	9.119	7.951	68172882	93076536	41.047	39.679
Target Compounds							
2)	A alpha-BHC	4.026	3.307	18625181	27926145	7.798	7.941
3)	MA gamma-BHC...	4.359	3.637	18106417	26296330	7.967	8.041
4)	MA Heptachlor	4.953	3.979	20064150	26800281	8.386	8.330
5)	MB Aldrin	5.296	4.260	27761615	38915017	12.083	11.916
6)	B beta-BHC	4.552	3.932	12913792	19953513	12.497	12.907
7)	B delta-BHC	4.802	4.163	29788785	40501860	12.041	11.340
8)	B Heptachlo...	5.723	4.762	26208062	36695624	12.146	11.920
9)	A Endosulfan I	6.110	5.132	17913558	23066108	9.106	8.484
10)	B trans-Chl...	5.979	5.012	25236008	34413375	12.034	11.482
11)	B cis-Chlor...	6.059	5.077	25861695	35714757	12.147	11.713
12)	B 4,4'-DDE	6.230	5.266	45636472	64549793	23.138	22.777
13)	MA Dieldrin	6.386	5.397	35095642	49232182	16.562	16.092
14)	MA Endrin	6.615	5.672	29084555	43223887	16.564	16.179
15)	B Endosulfa...	6.833	5.965	45034566	59603465	24.368	23.031
16)	A 4,4'-DDD	6.746	5.819	25782514	37284877	16.396	16.035
17)	MA 4,4'-DDT	7.062	6.071	27008480	37038094	16.585	15.733
18)	B Endrin al...	6.963	6.144	35349431	48105833	24.264	23.988
19)	B Endosulfa...	7.198	6.366	43661118	57825478	24.193	23.633
20)	A Methoxychlor	7.536	6.646	76209811	108.1E6	87.673	88.921
21)	B Endrin ke...	7.685	6.873	47222986	66637703	24.156	23.754

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111023\
Data File : PD079510.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2023 17:27
Operator : AR\AJ
Sample : RESC014
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 04:23:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111023CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 08 02:29:03 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

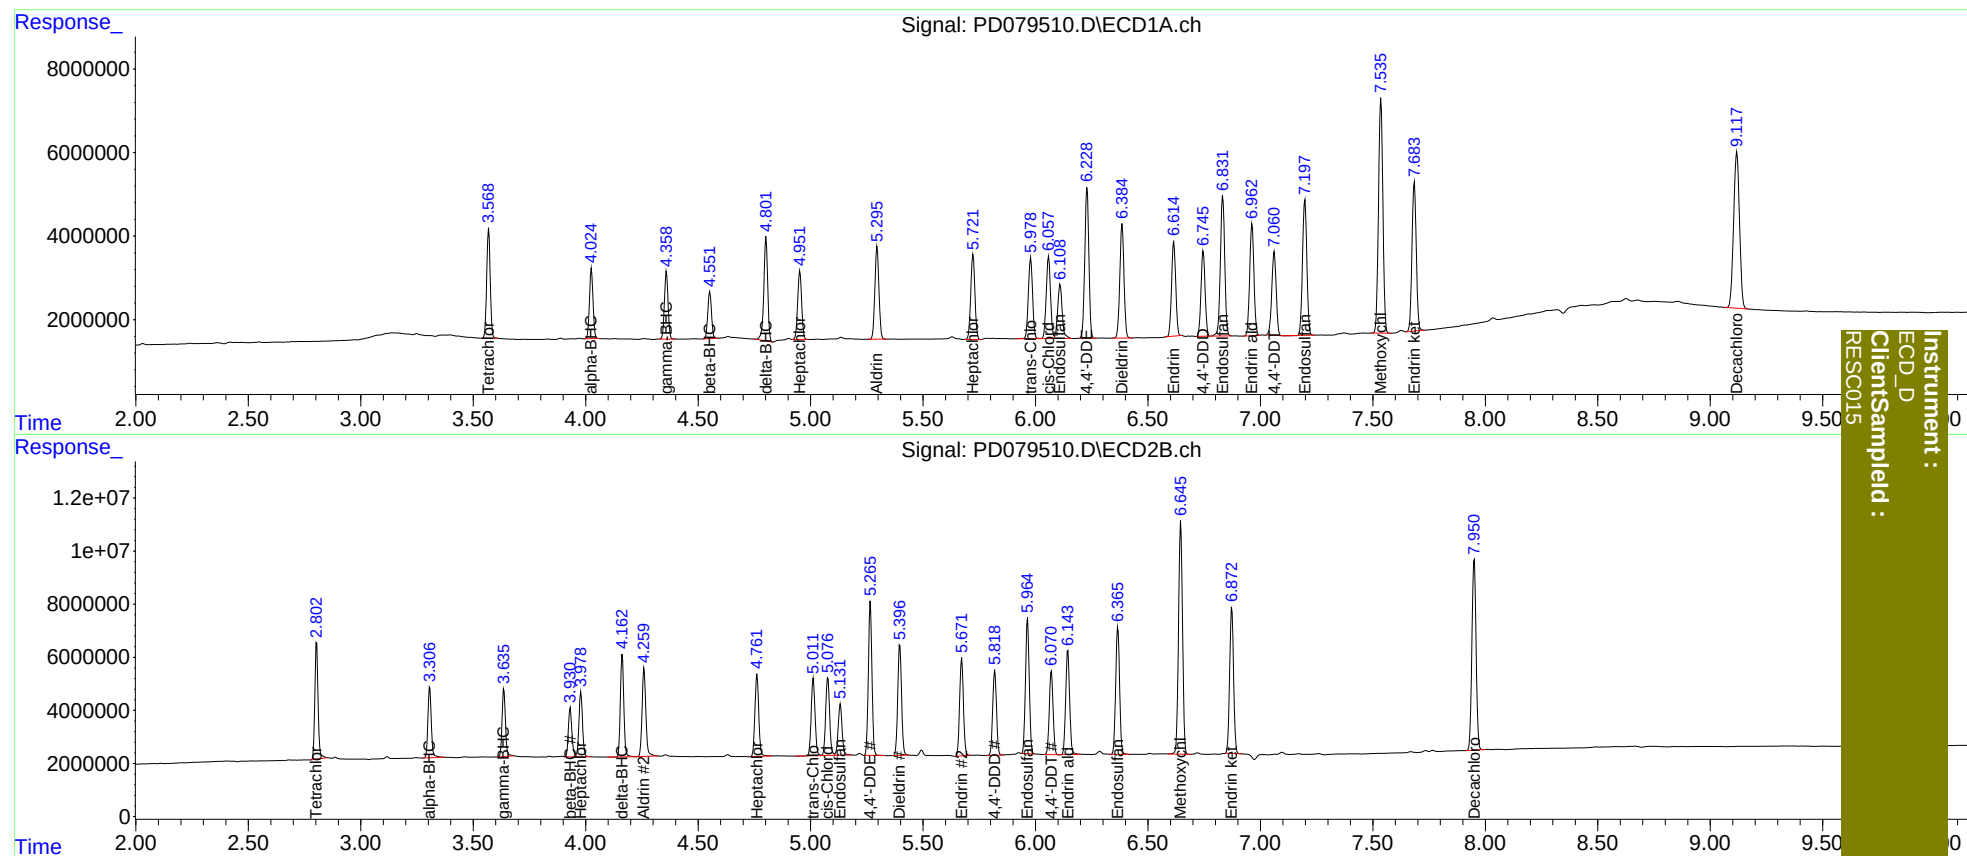

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111023\
Data File : PD079510.D
Acq On : 07 Nov 2023 17:27
Operator : AR\AJ
Sample : RESC014
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC015

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111023CLP-TCLP.M
Title : GC Extractables
Last Update : Wed Nov 08 02:29:03 2023
Integrator: ChemStation

RT#1	RT#2	Resolution
3.569	4.026	100.00%
4.026	4.359	100.00%
4.359	4.552	100.00%
4.552	4.802	100.00%
4.802	4.953	100.00%
4.953	5.296	100.00%
5.296	5.723	100.00%
5.723	5.979	100.00%
5.979	6.059	100.00%
6.059	6.110	97.01%
6.110	6.230	100.00%
6.230	6.386	100.00%
6.386	6.615	100.00%
6.615	6.746	100.00%
6.746	6.833	100.00%
6.833	6.963	100.00%
6.963	7.062	100.00%
7.062	7.198	100.00%
7.198	7.536	100.00%
7.536	7.685	100.00%
7.685	9.119	100.00%

Signal #2


2.804	3.307	100.00%
3.307	3.637	100.00%
3.637	3.932	100.00%
3.932	3.979	96.85%
3.979	4.163	100.00%
4.163	4.260	100.00%
4.260	4.762	100.00%
4.762	5.012	100.00%
5.012	5.077	100.00%
5.077	5.132	98.97%
5.132	5.266	100.00%
5.266	5.397	100.00%
5.397	5.672	100.00%
5.672	5.819	100.00%
5.819	5.965	100.00%
5.965	6.071	100.00%
6.071	6.144	100.00%
6.144	6.366	100.00%
6.366	6.646	100.00%
6.646	6.873	100.00%
6.873	7.951	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111023\
Data File : PD079510.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2023 17:27
Operator : AR\AJ
Sample : RESC014
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC015

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 04:23:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111023CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 08 02:29:03 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

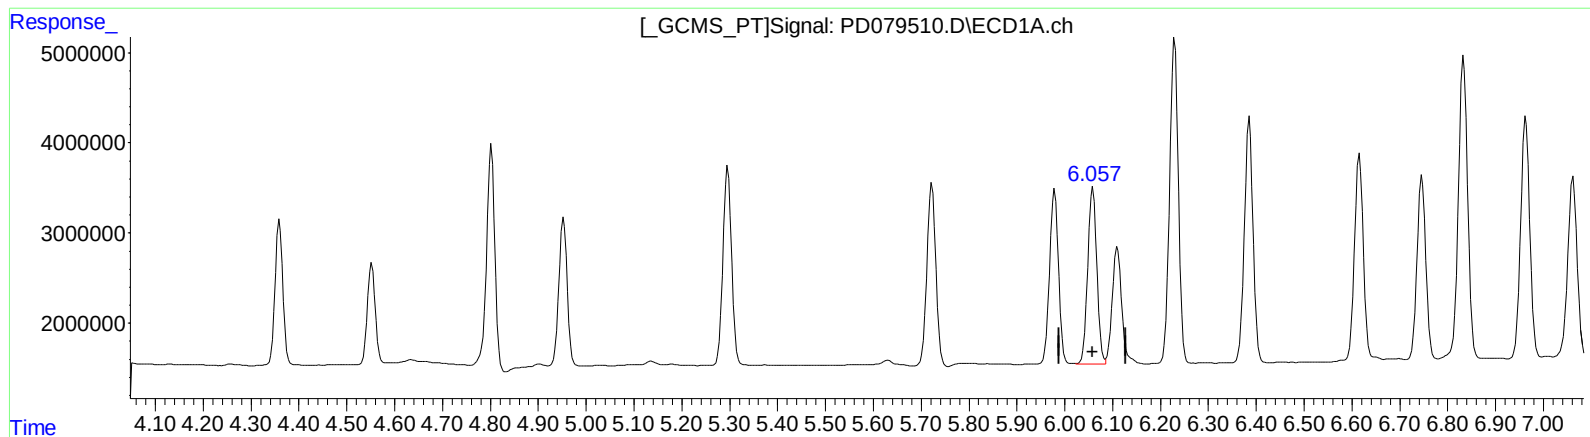

QEdit

(11) cis-Chlordane (B)

6.059min 12.147 ng/ml

response 25861695

(11) cis-Chlordane #2 (B)

5.077min 11.713 ng/ml


response 35714757

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111023\
Data File : PD079510.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2023 17:27
Operator : AR\AJ
Sample : RESC014
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC015

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 04:23:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111023CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 08 02:29:03 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

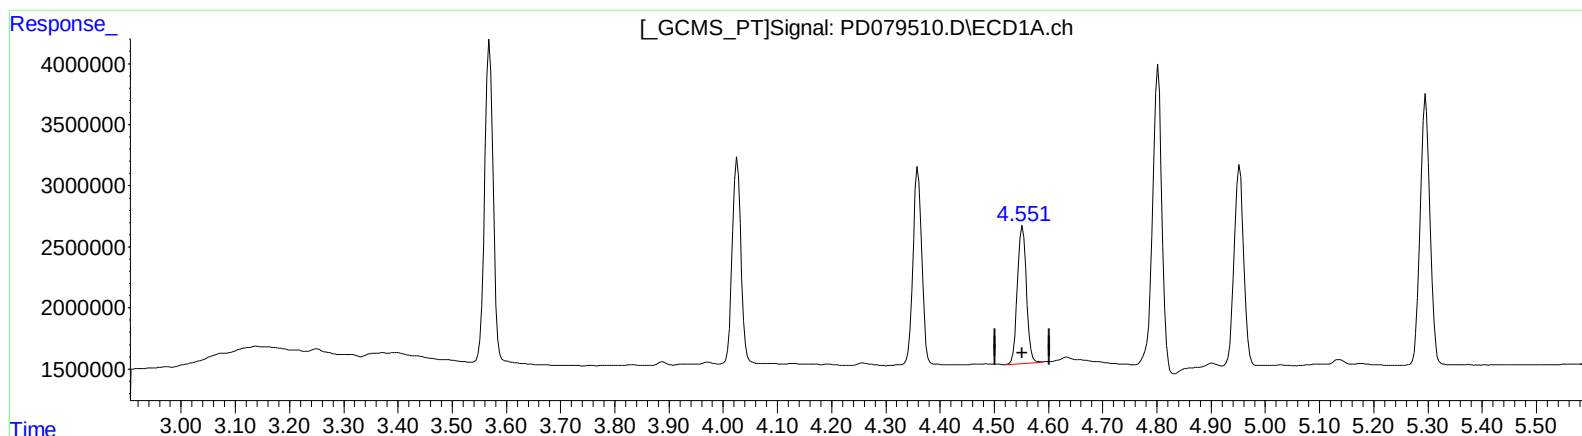

(6) beta-BHC (B)

4.552min 12.497 ng/ml

response 12913792

(6) beta-BHC #2 (B)

3.932min 12.907 ng/ml


response 19953513

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111023\
Data File : PD079510.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2023 17:27
Operator : AR\AJ
Sample : RESC014
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC015

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 04:23:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111023CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 08 02:29:03 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

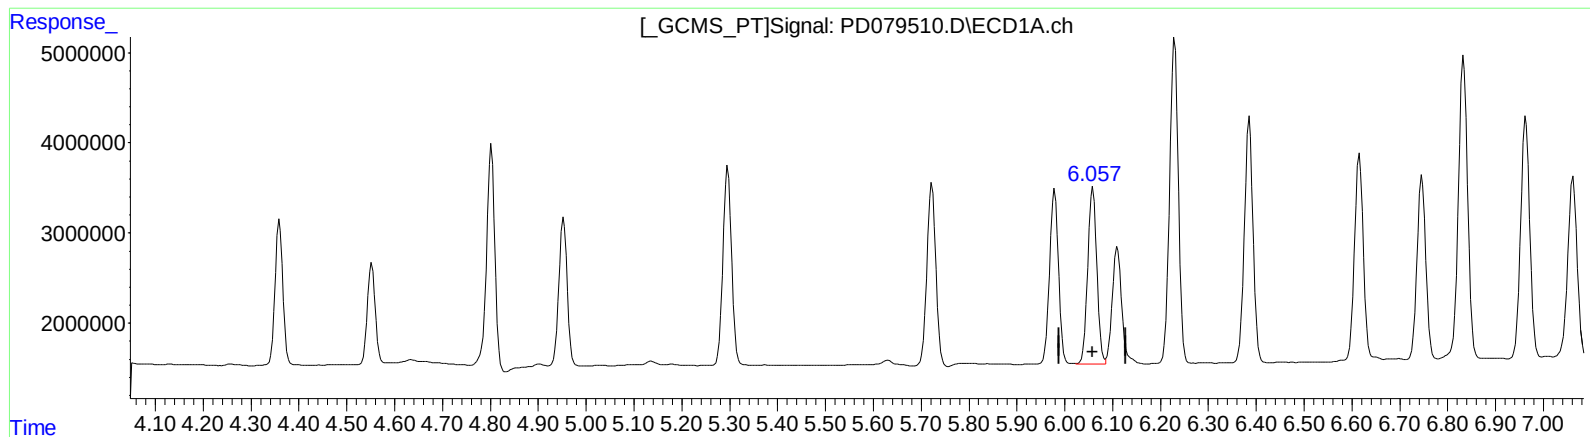

QEdit

(11) cis-Chlordane (B)

6.059min 12.147 ng/ml

response 25861695

(11) cis-Chlordane #2 (B)

5.077min 11.713 ng/ml

response 35714757