

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111023\
 Data File : PD079528.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2023 21:27
 Operator : AR\AJ
 Sample : INDA601
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA6011

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/08/2023
 Supervised By : Ankita Jodhani 11/08/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 01:32:15 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111023CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 08 01:32:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	2.804	216.4E6	339.8E6	155.088	156.693
27)	SA Decachlor...	9.117	7.950	510.3E6	721.7E6	307.254	307.669
Target Compounds							
2)	A alpha-BHC	4.026	3.307	421.8E6	597.8E6	176.595	169.988
3)	MA gamma-BHC...	4.359	3.636	390.6E6	549.9E6	171.867	168.146
4)	MA Heptachlor	4.952	3.977	388.8E6	529.8E6	162.491	164.631m
9)	A Endosulfan I	6.109	5.132	303.9E6	435.1E6	154.478	160.030
13)	MA Dieldrin	6.385	5.397	703.4E6	1006.6E6	331.918	329.004
14)	MA Endrin	6.616	5.672	578.8E6	867.5E6	329.634	324.734
16)	A 4,4'-DDD	6.746	5.819	524.3E6	766.3E6	333.411	329.559
17)	MA 4,4'-DDT	7.061	6.070	553.4E6	802.4E6	339.853	340.846
20)	A Methoxychlor	7.536	6.645	1339.2E6	1688.0E6	1540.619	1388.508

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111023\
Data File : PD079528.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2023 21:27
Operator : AR\AJ
Sample : INDA601
Misc :
ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 01:32:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111023CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 08 01:32:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

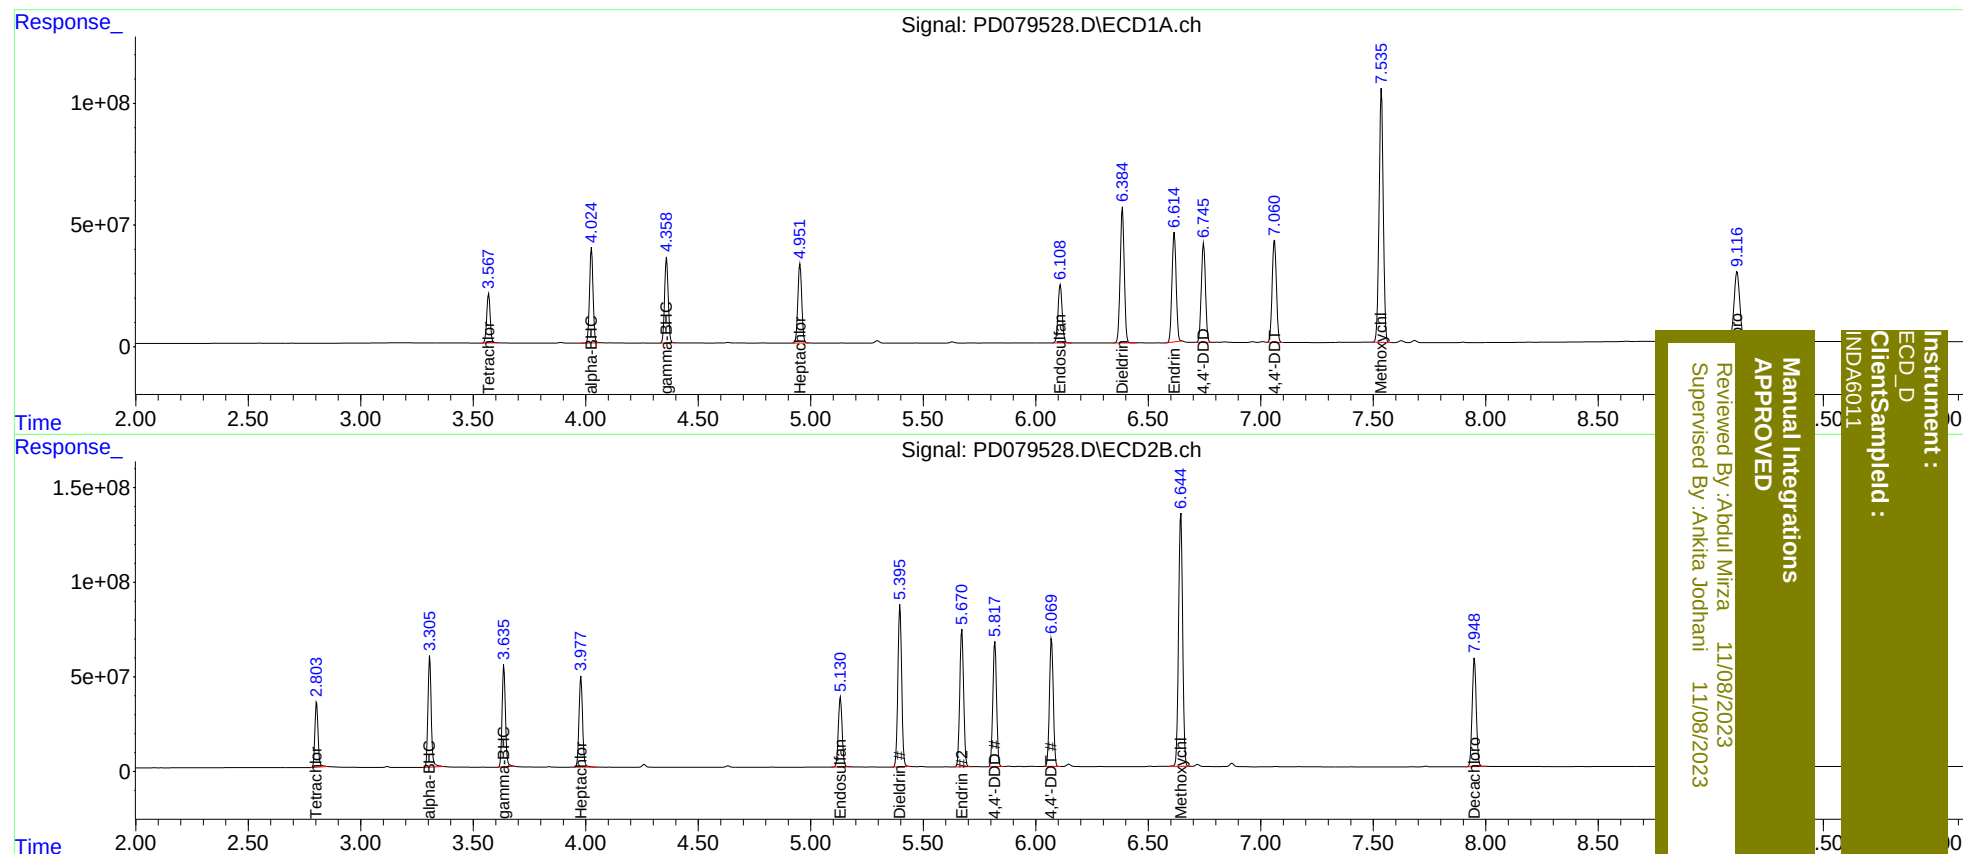

Reviewed By: Abdul Mirza 11/08/2023
Supervised By: Ankita Jodhani 11/08/2023

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
INDA6011