

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111119\
 Data File : PD055858.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Nov 2019 08:32
 Operator : SG\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 00:32:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 02 07:20:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	0.000	3.915f	0	272268	N.D.	0.260
Target Compounds						
8) B Heptachlo...	4.891f	0.000	4056602	0	4.543	N.D. #
9) A Endosulfan I	5.323f	0.000	2213024	0	2.641	N.D. #
20) A Methoxychlor	6.682	0.000	2178957	0	5.825	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111119\
Data File : PD055858.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Nov 2019 08:32
Operator : SG\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 00:32:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 02 07:20:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

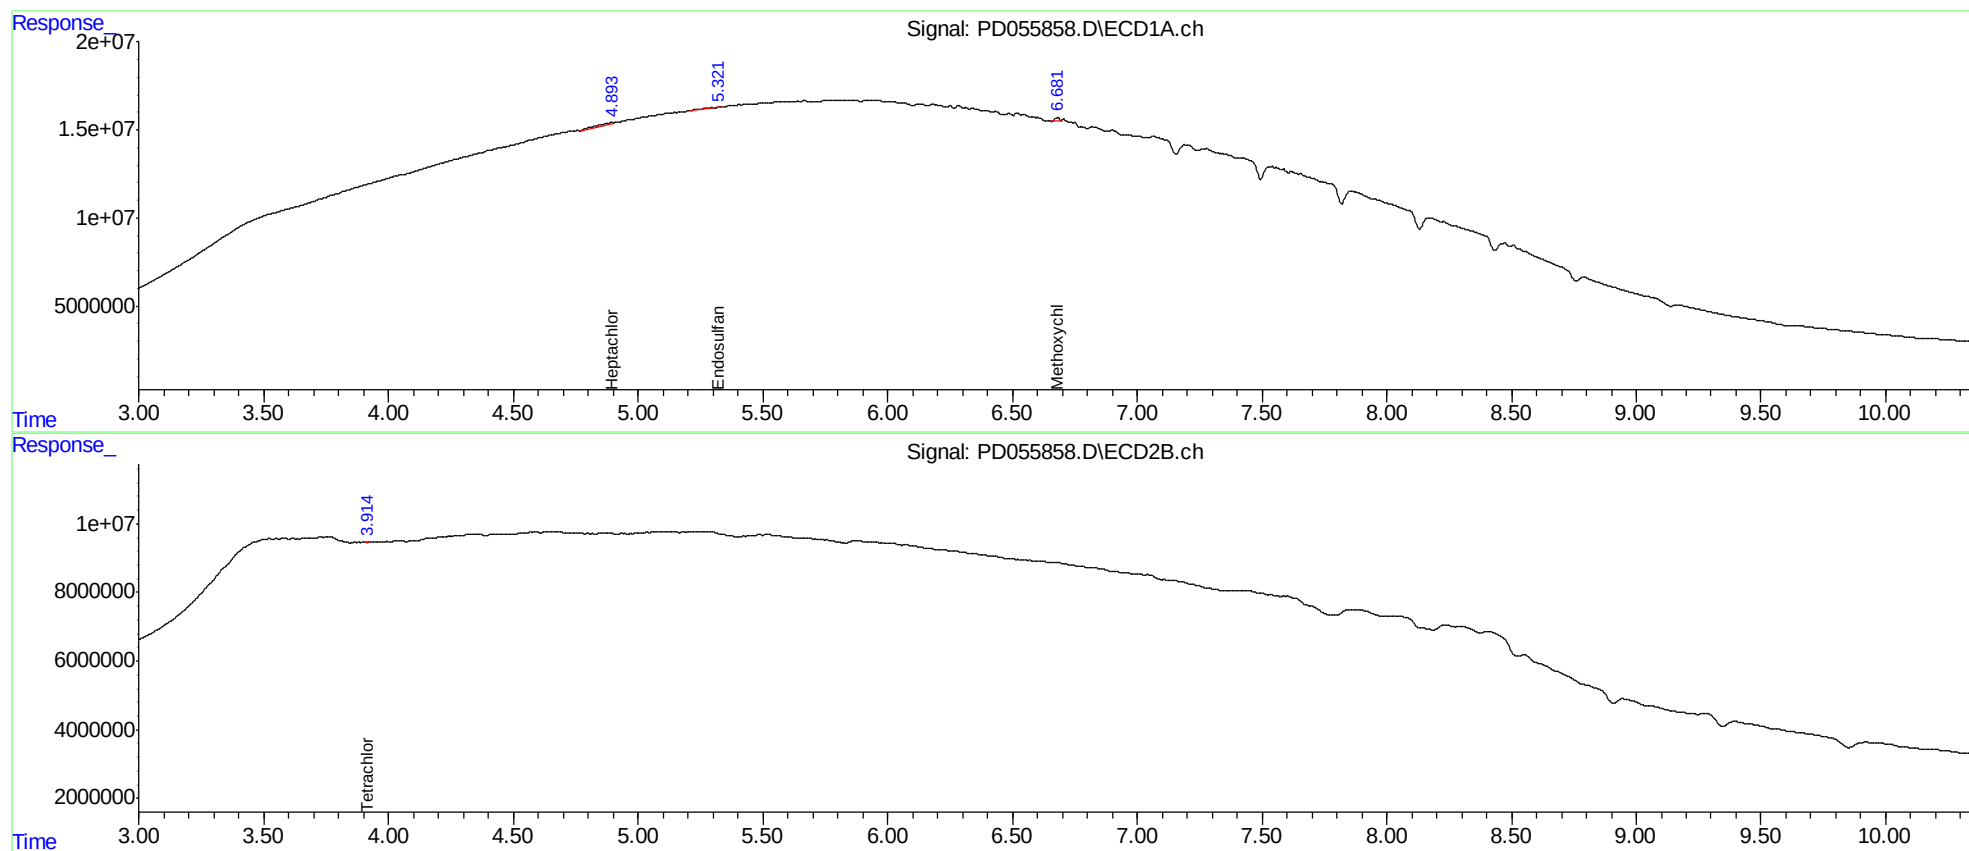


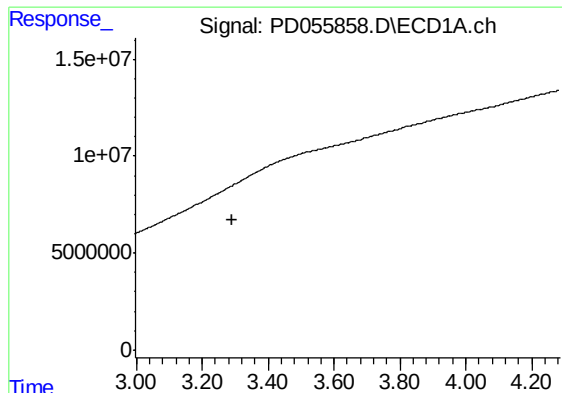

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.289 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

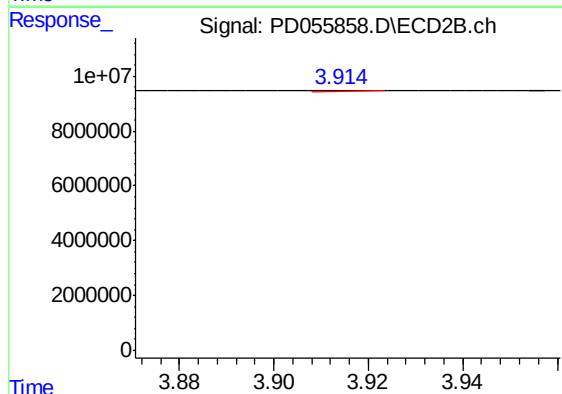


#1 Tetrachloro-m-xylene

R.T.: 3.915 min
Delta R.T.: -0.047 min
Response: 272268
Conc: 0.26 ng/ml

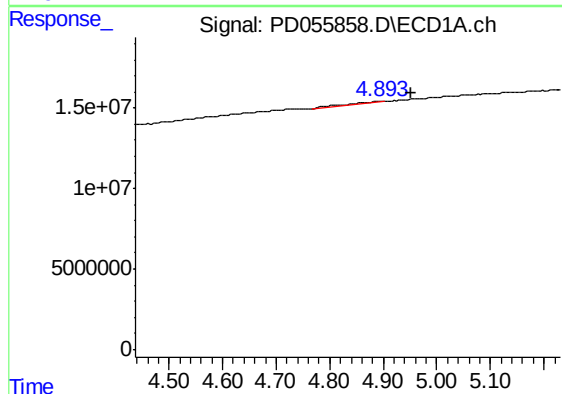


#8 Heptachlor epoxide

R.T.: 4.891 min
Delta R.T.: -0.061 min
Response: 4056602
Conc: 4.54 ng/ml

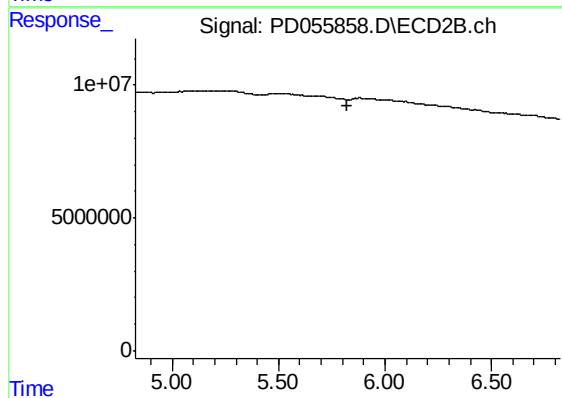

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.824 min
Response: 0
Conc: N.D.

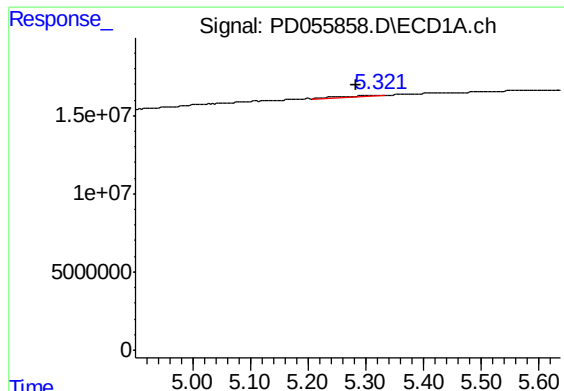

#9 Endosulfan I


R.T.: 5.323 min
Delta R.T.: 0.039 min
Response: 2213024
Conc: 2.64 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

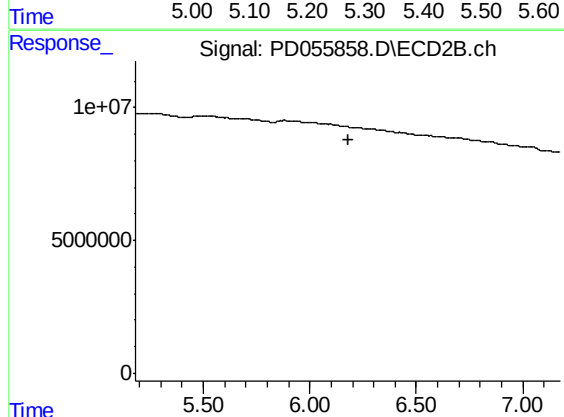


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.180 min
Response: 0
Conc: N.D.

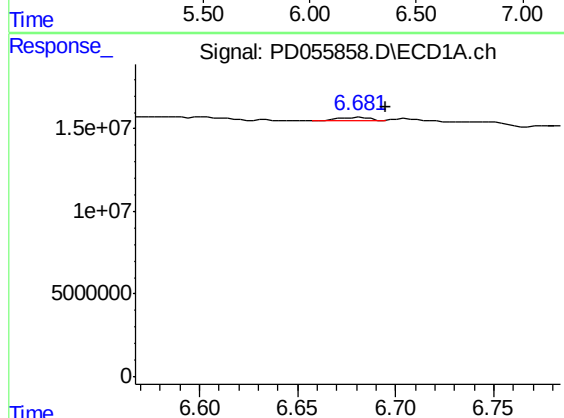


#20 Methoxychlor

R.T.: 6.682 min
Delta R.T.: -0.013 min
Response: 2178957
Conc: 5.83 ng/ml

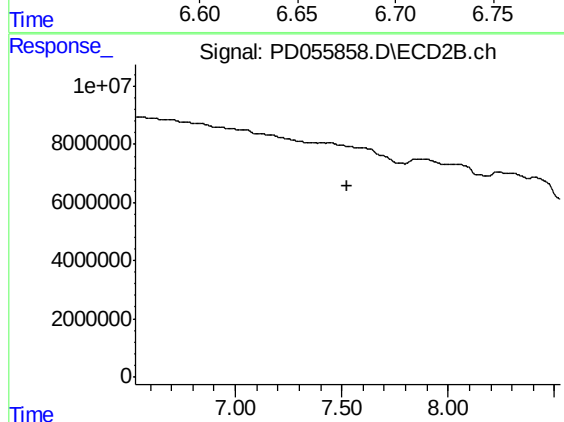

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.529 min
Response: 0
Conc: N.D.

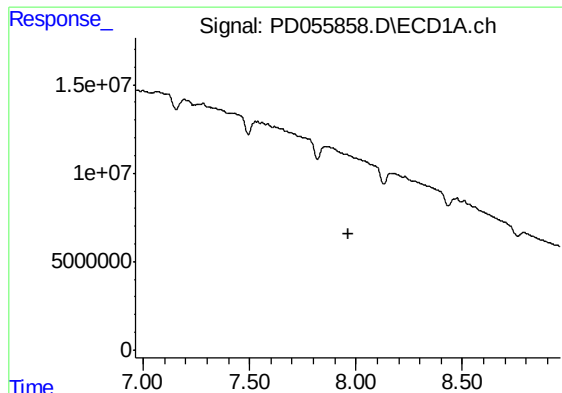

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.963 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

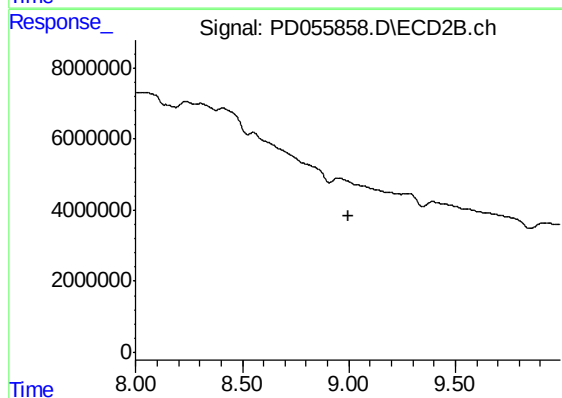

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.997 min
Response: 0
Conc: N.D.