

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111119\
 Data File : PD055861.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Nov 2019 09:48
 Operator : SG\AJ
 Sample : PB124663BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PBLK63

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 00:32:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 02 07:20:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.292	3.961	21887334	28053187	29.076	26.770
27)	SA Decachlor...	7.967	8.998	31036994	42092734	38.077	37.068
Target Compounds							
19)	B Endosulfa...	0.000	7.242f	0	2096389	N.D.	1.739


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111119\
Data File : PD055861.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Nov 2019 09:48
Operator : SG\AJ
Sample : PB124663BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PBLK63

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 00:32:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 02 07:20:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

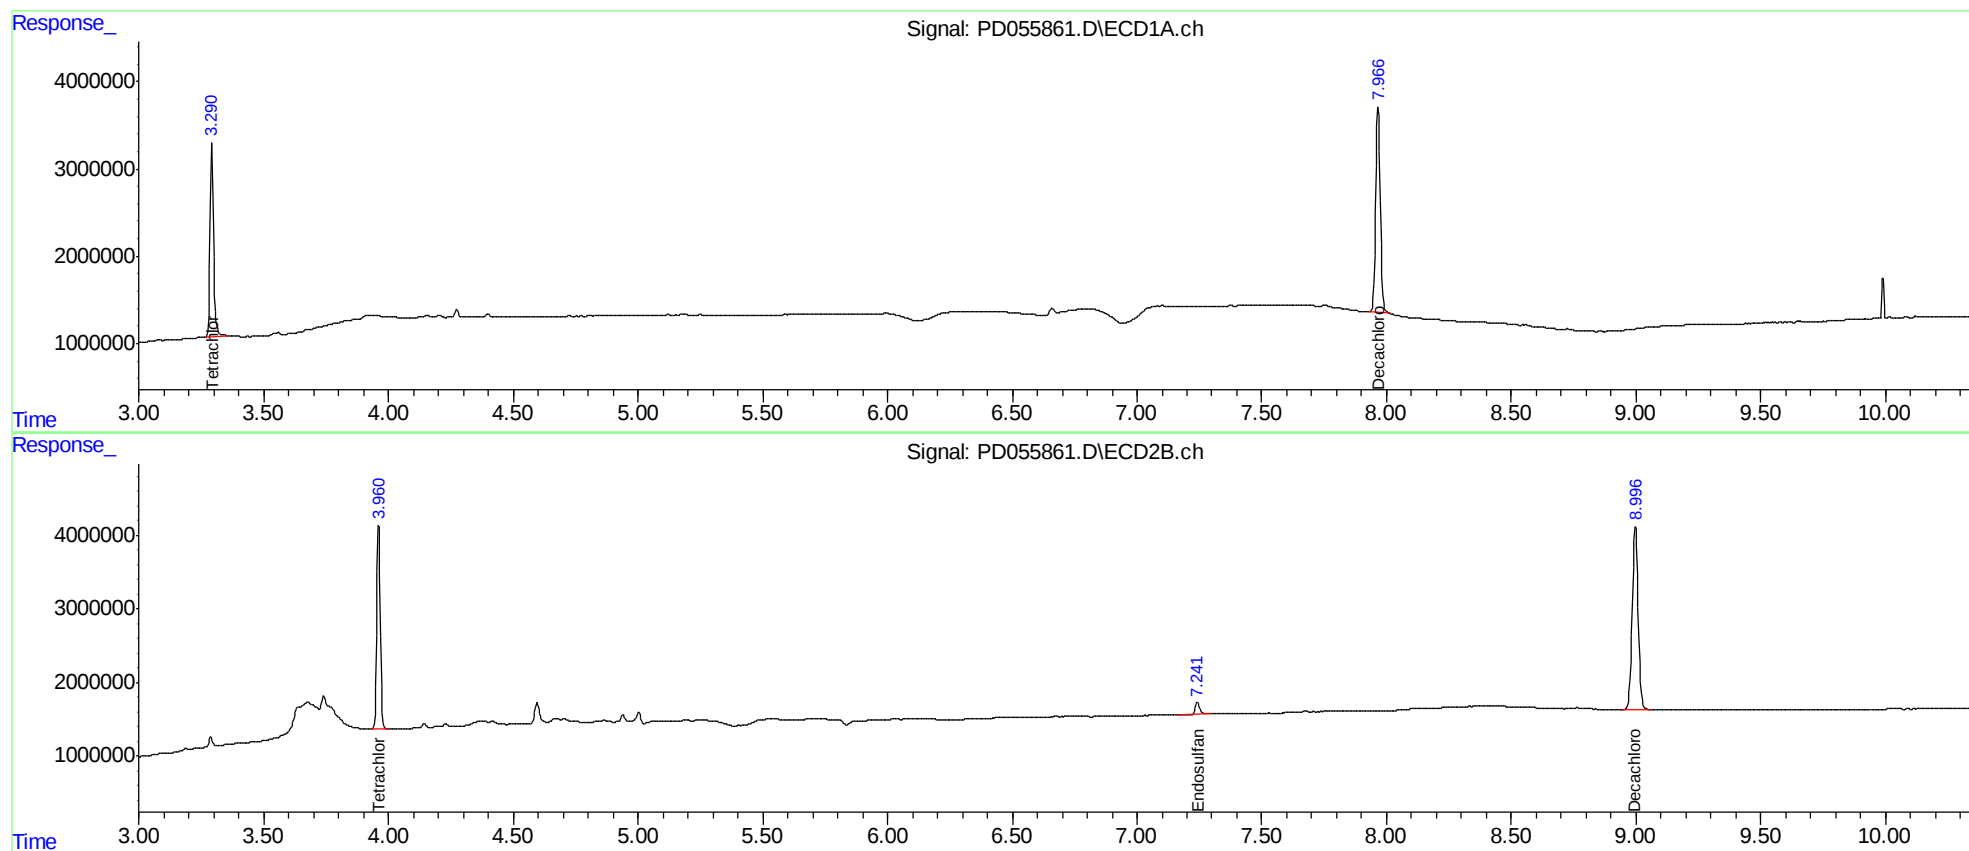


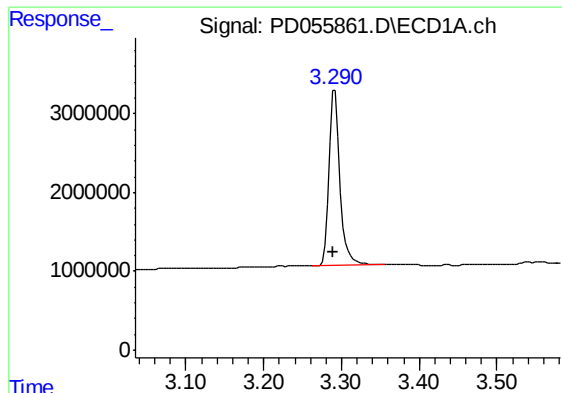

#1 Tetrachloro-m-xylene


R.T.: 3.292 min
Delta R.T.: 0.002 min
Response: 21887334
Conc: 29.08 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK63

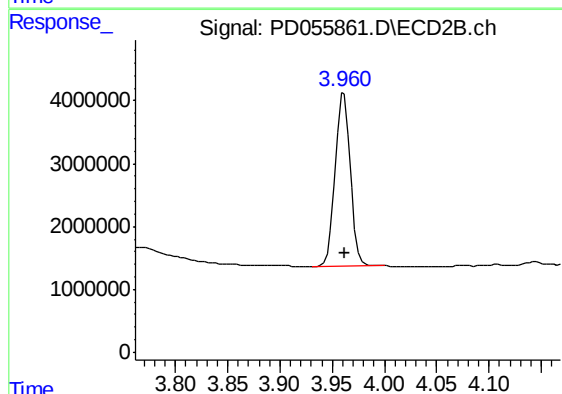


#1 Tetrachloro-m-xylene

R.T.: 3.961 min
Delta R.T.: 0.000 min
Response: 28053187
Conc: 26.77 ng/ml

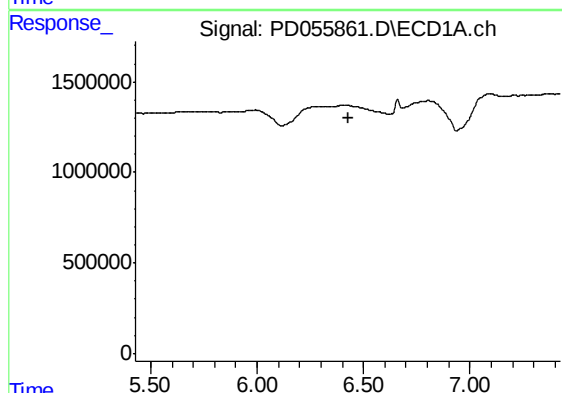


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 6.428 min
Response: 0
Conc: N.D.

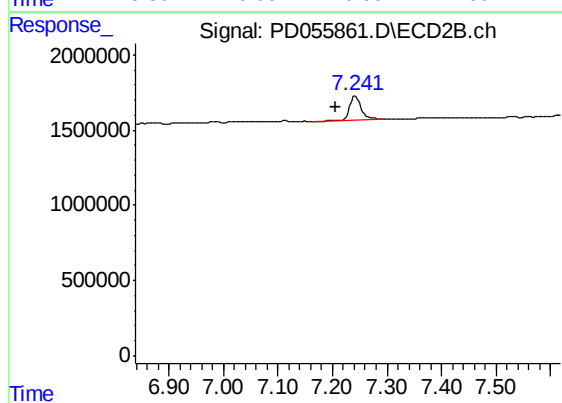

#19 Endosulfan Sulfate


R.T.: 7.242 min
Delta R.T.: 0.037 min
Response: 2096389
Conc: 1.74 ng/ml

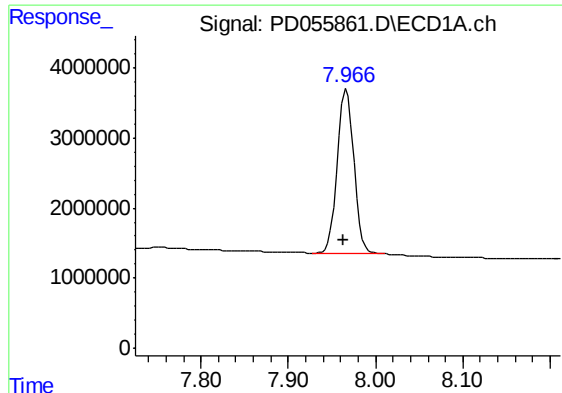

#27 Decachlorobiphenyl

R.T.: 7.967 min
Delta R.T.: 0.004 min
Response: 31036994
Conc: 38.08 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK63

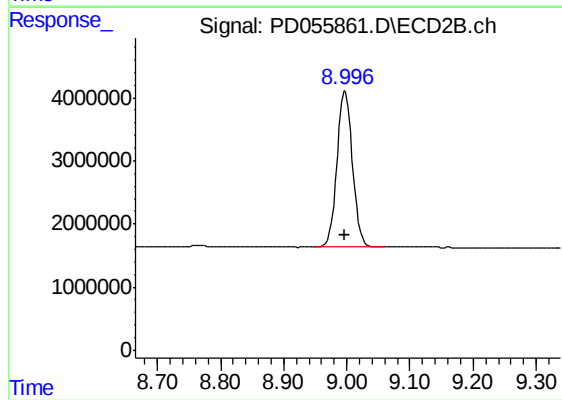

#27 Decachlorobiphenyl

R.T.: 8.998 min
Delta R.T.: 0.000 min
Response: 42092734
Conc: 37.07 ng/ml