

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111119\
 Data File : PD055893.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Nov 2019 17:31
 Operator : SG\AJ
 Sample : K5719-19
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 F2J16

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 00:40:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 02 07:20:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.290	3.963	14620390	18541452	19.422	17.693
27)	SA Decachlor...	7.966	8.999	21457659	27475023	26.325	24.195
Target Compounds							
4)	MA Heptachlor	0.000	5.119	0	2809724	N.D.	1.932
5)	MB Aldrin	4.529	0.000	4868940	0	5.255	N.D. #
6)	B beta-BHC	4.204f	0.000	32902905	0	72.745	N.D. #
10)	B trans-Chl...	0.000	6.042	0	1459360	N.D.	1.023


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111119\
Data File : PD055893.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Nov 2019 17:31
Operator : SG\AJ
Sample : K5719-19
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
F2J16

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 00:40:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 02 07:20:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

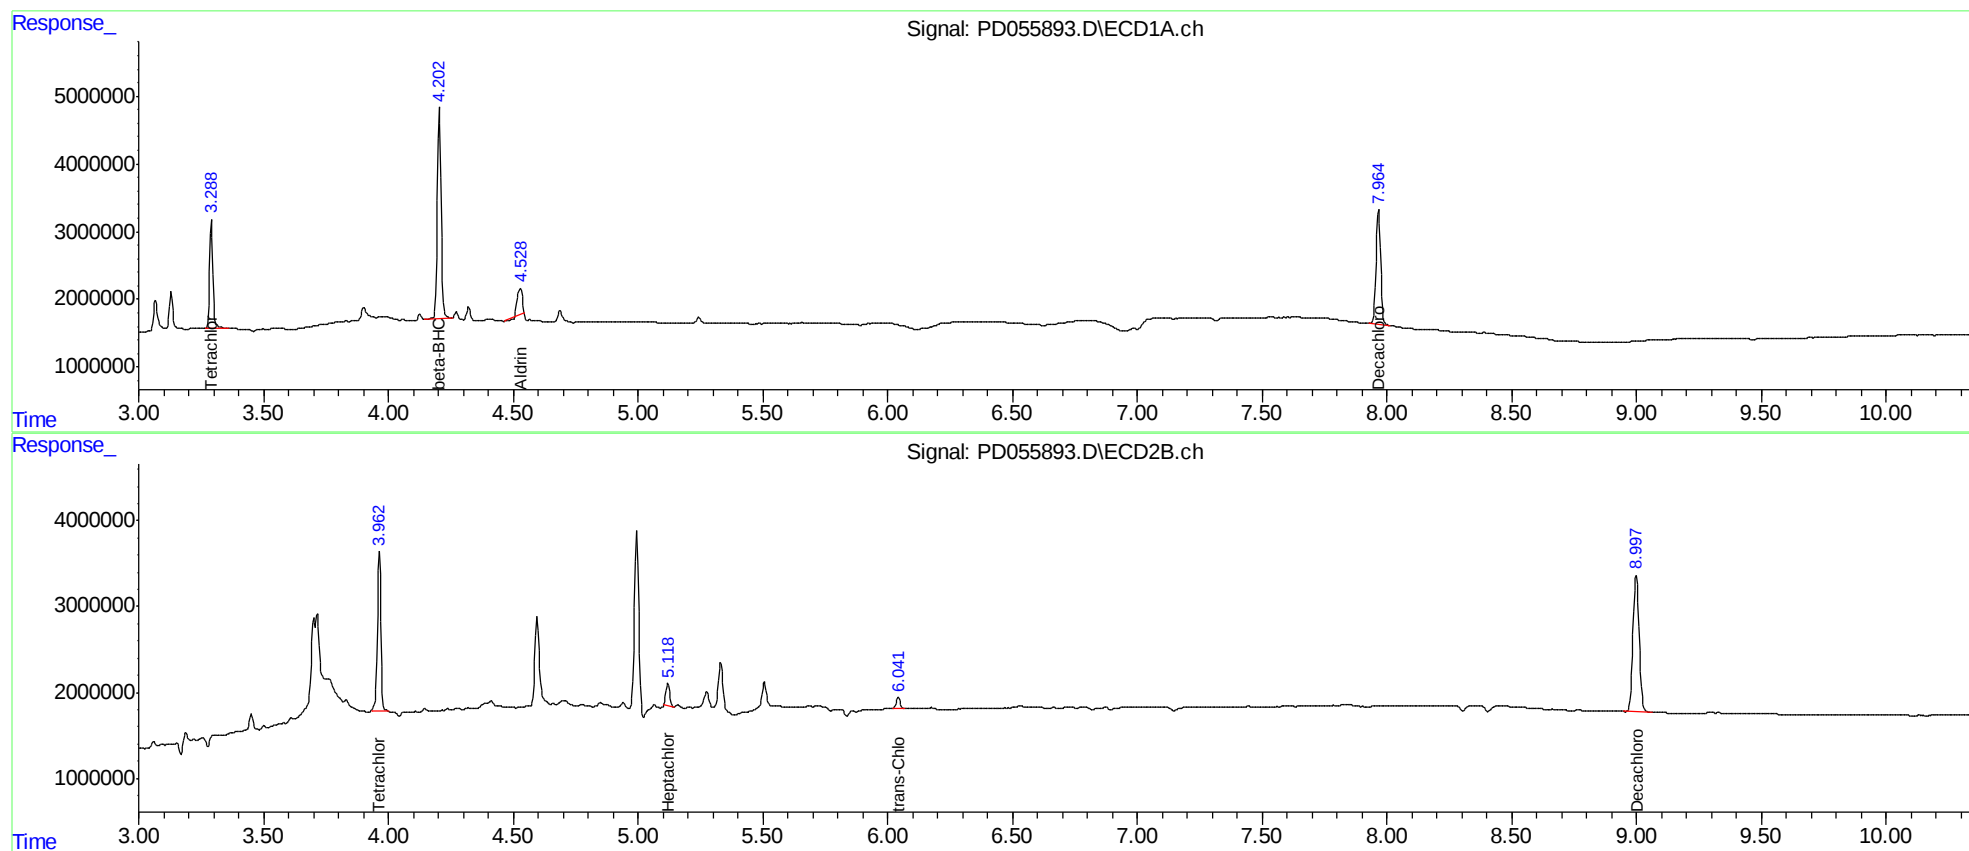


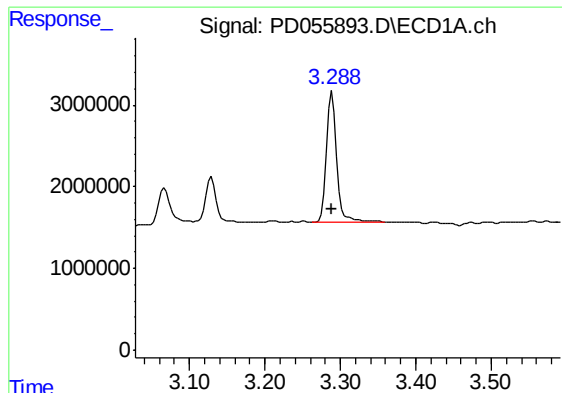

#1 Tetrachloro-m-xylene


R.T.: 3.290 min
Delta R.T.: 0.000 min
Response: 14620390
Conc: 19.42 ng/ml

Instrument :
ECD_D
ClientSampleId :
F2J16

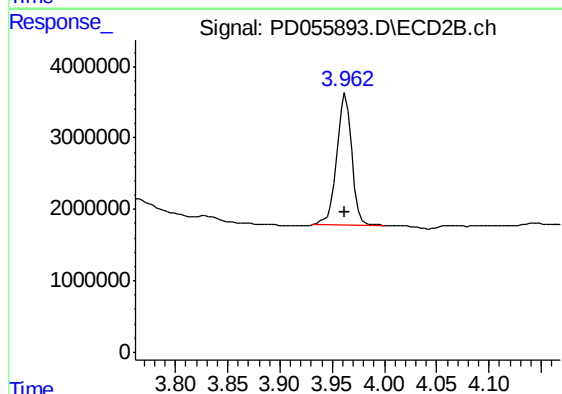


#1 Tetrachloro-m-xylene

R.T.: 3.963 min
Delta R.T.: 0.001 min
Response: 18541452
Conc: 17.69 ng/ml

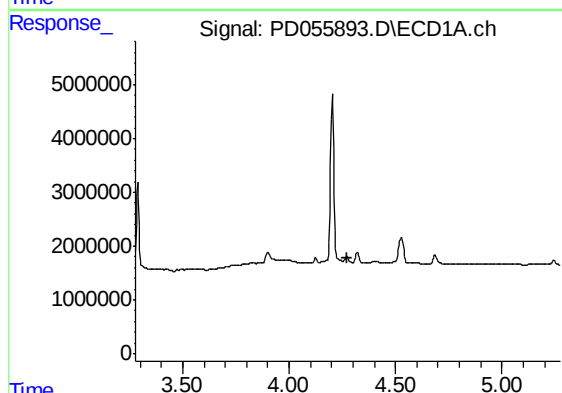


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.277 min
Response: 0
Conc: N.D.

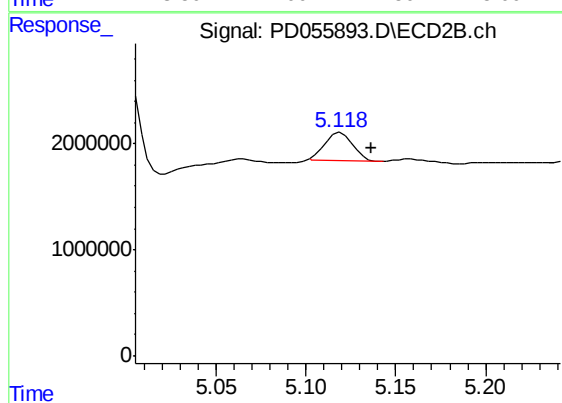

#4 Heptachlor


R.T.: 5.119 min
Delta R.T.: -0.017 min
Response: 2809724
Conc: 1.93 ng/ml

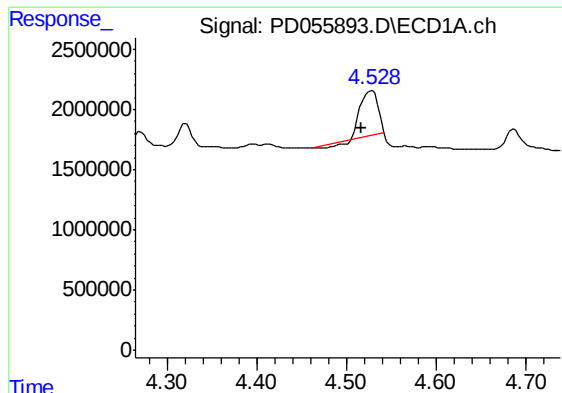

#5 Aldrin


R.T.: 4.529 min
Delta R.T.: 0.013 min
Response: 4868940
Conc: 5.26 ng/ml

Instrument :
ECD_D
ClientSampleId :
F2J16

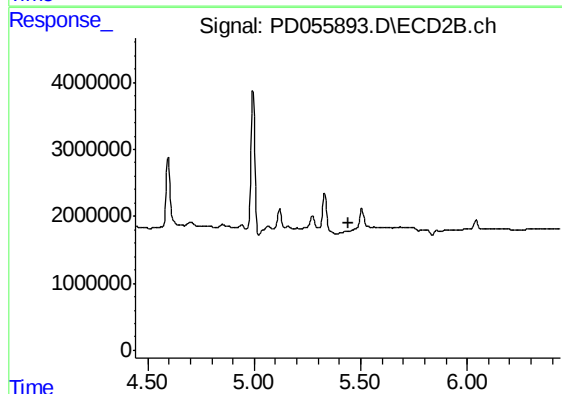


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.440 min
Response: 0
Conc: N.D.

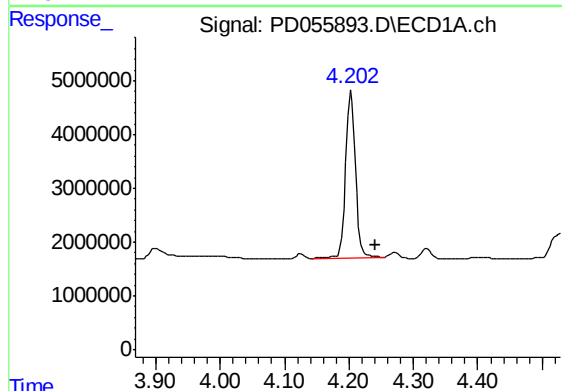


#6 beta-BHC

R.T.: 4.204 min
Delta R.T.: -0.037 min
Response: 32902905
Conc: 72.75 ng/ml

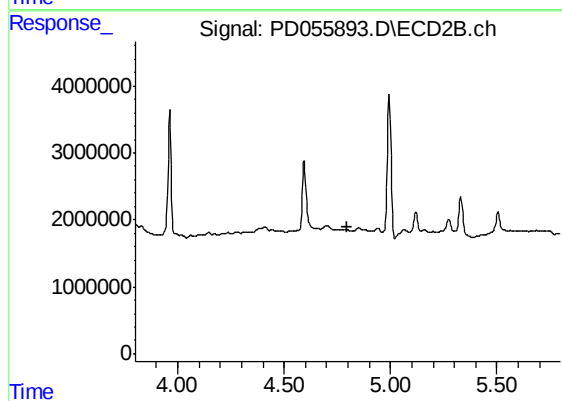

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.799 min
Response: 0
Conc: N.D.

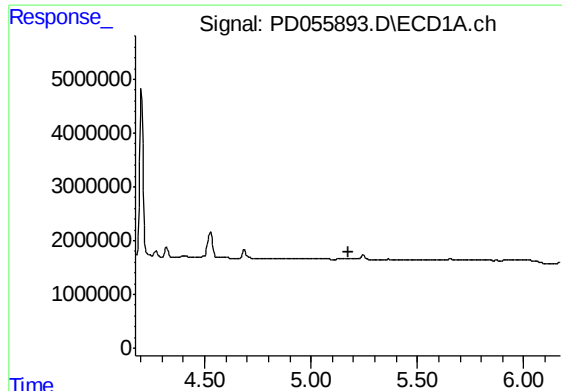

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.174 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
F2J16

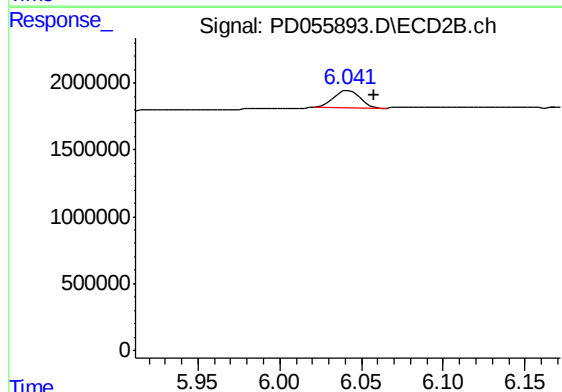


#10 trans-Chlordane

R.T.: 6.042 min
Delta R.T.: -0.016 min
Response: 1459360
Conc: 1.02 ng/ml

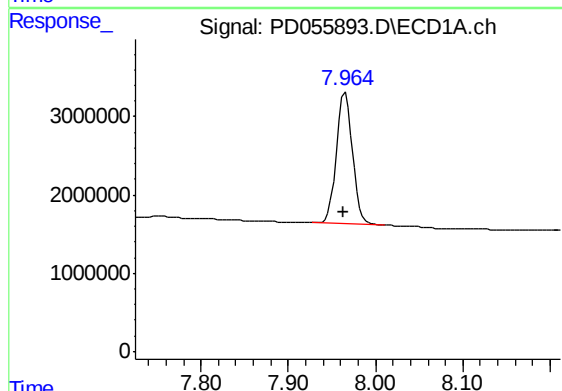

#27 Decachlorobiphenyl

R.T.: 7.966 min
Delta R.T.: 0.002 min
Response: 21457659
Conc: 26.32 ng/ml

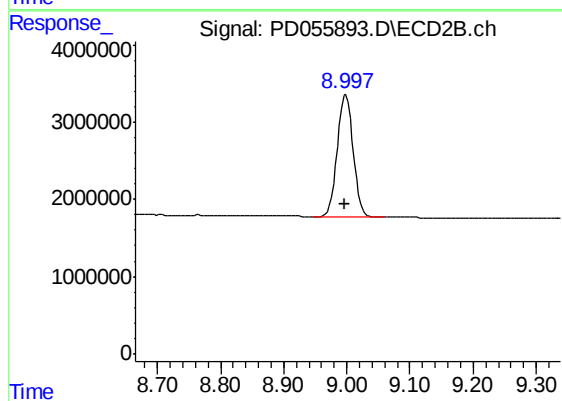

#27 Decachlorobiphenyl

R.T.: 8.999 min
Delta R.T.: 0.002 min
Response: 27475023
Conc: 24.20 ng/ml