

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111123\
Data File : PD079543.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Nov 2023 11:42
Operator : AR\AJ
Sample : INDA323
Misc :
ALS Vial : 10 Sample Multiplier: 1


Instrument :
ECD_D
LabSampleId :
INDA323

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 11/09/2023
Supervised By :Ankita Jodhani 11/09/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 03:34:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111023CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 09 03:10:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

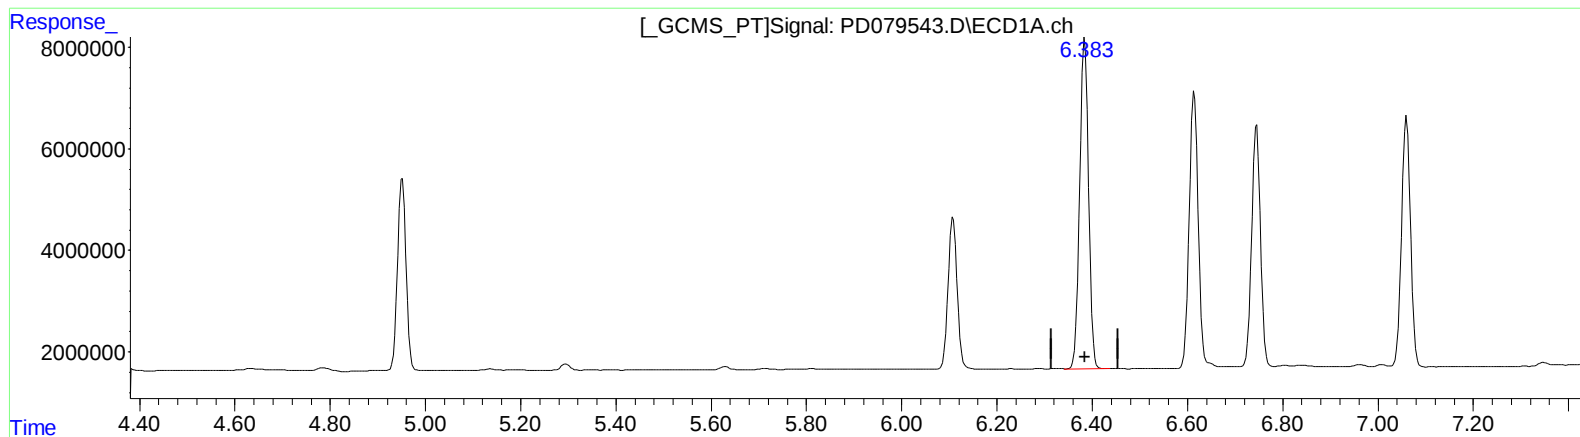

(13) Dieldrin (MA)
6.384min 39.547 ng/ml
response 83803260

(13) Dieldrin #2 (MA)
5.396min 29.978 ng/ml
response 91717094

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111123\
Data File : PD079543.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Nov 2023 11:42
Operator : AR\AJ
Sample : INDA323
Misc :
ALS Vial : 10 Sample Multiplier: 1


Instrument :
ECD_D
LabSampleId :
INDA323

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 11/09/2023
Supervised By :Ankita Jodhani 11/09/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 03:34:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111023CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 09 03:10:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

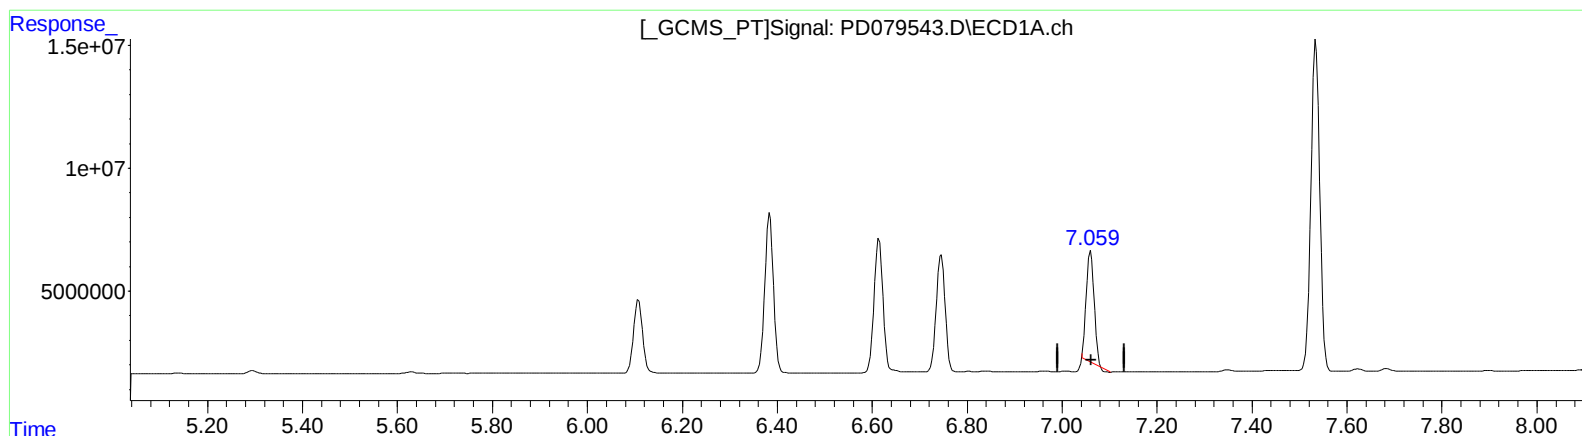

(17) 4,4'-DDT (MA)

7.060min 32.260 ng/ml

response 52534419

(17) 4,4'-DDT #2 (MA)

6.069min 39.720 ng/ml

response 93510279

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111123\
Data File : PD079543.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Nov 2023 11:42
Operator : AR\AJ
Sample : INDA323
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :

ECD_D

LabSampleId :

INDA323



Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 11/09/2023

Supervised By :Ankita Jodhani 11/09/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 03:34:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111023CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 09 03:10:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

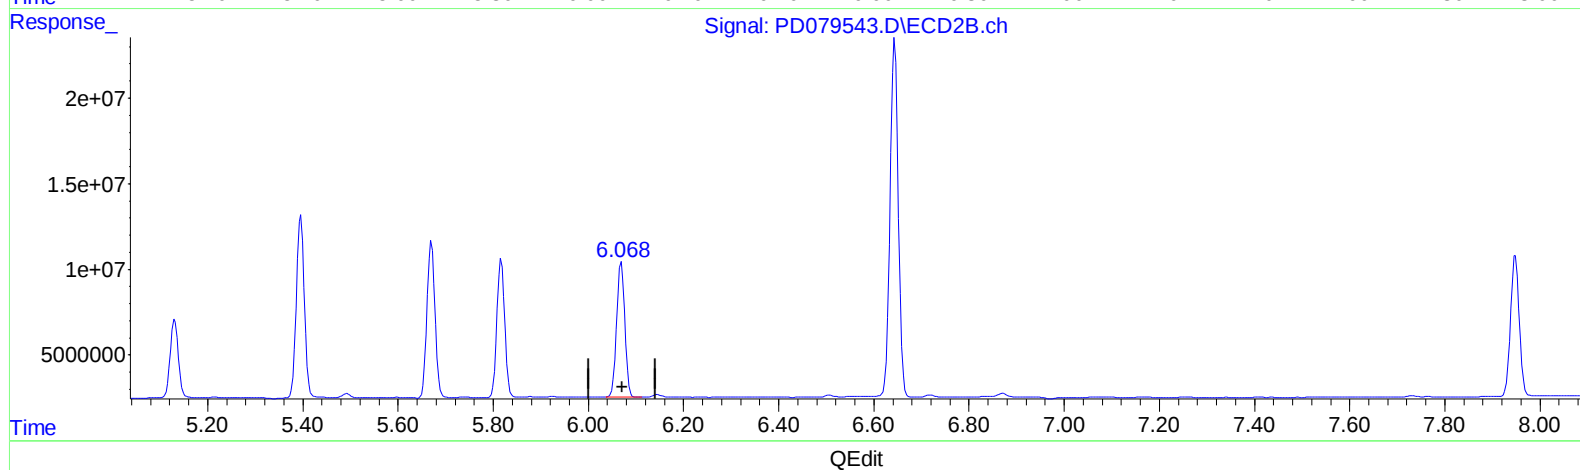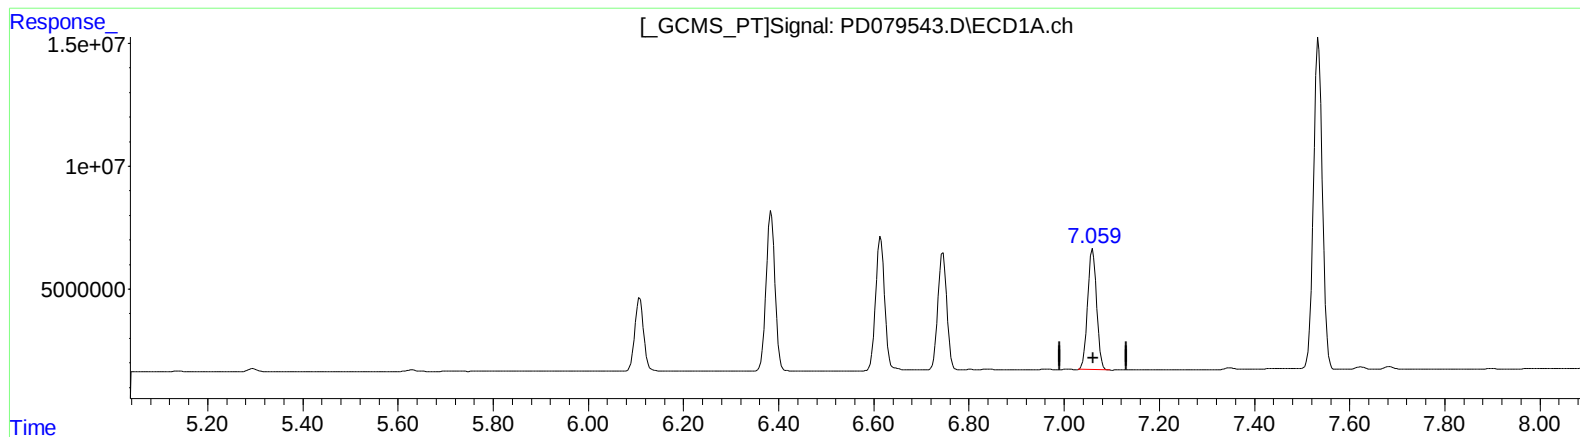

(17) 4,4'-DDT (MA)

7.059min 39.065 ng/ml m

response 63616251

(17) 4,4'-DDT #2 (MA)

6.069min 39.720 ng/ml

response 93510279