

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111124\
 Data File : PD086514.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Nov 2024 12:21
 Operator : AR\AJ
 Sample : PB164033BL
 Misc : BL/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB164033BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 01:36:04 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD103024.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 31 11:38:14 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.563	2.887	26192672	207.7E6	17.931	21.000
28) SA Decachlor...	9.100	8.095	38797399	229.3E6	20.237	21.406

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111124\
Data File : PD086514.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Nov 2024 12:21
Operator : AR\AJ
Sample : PB164033BL
Misc : BL/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PB164033BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 01:36:04 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD103024.M
Quant Title : GC Extractables
QLast Update : Thu Oct 31 11:38:14 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

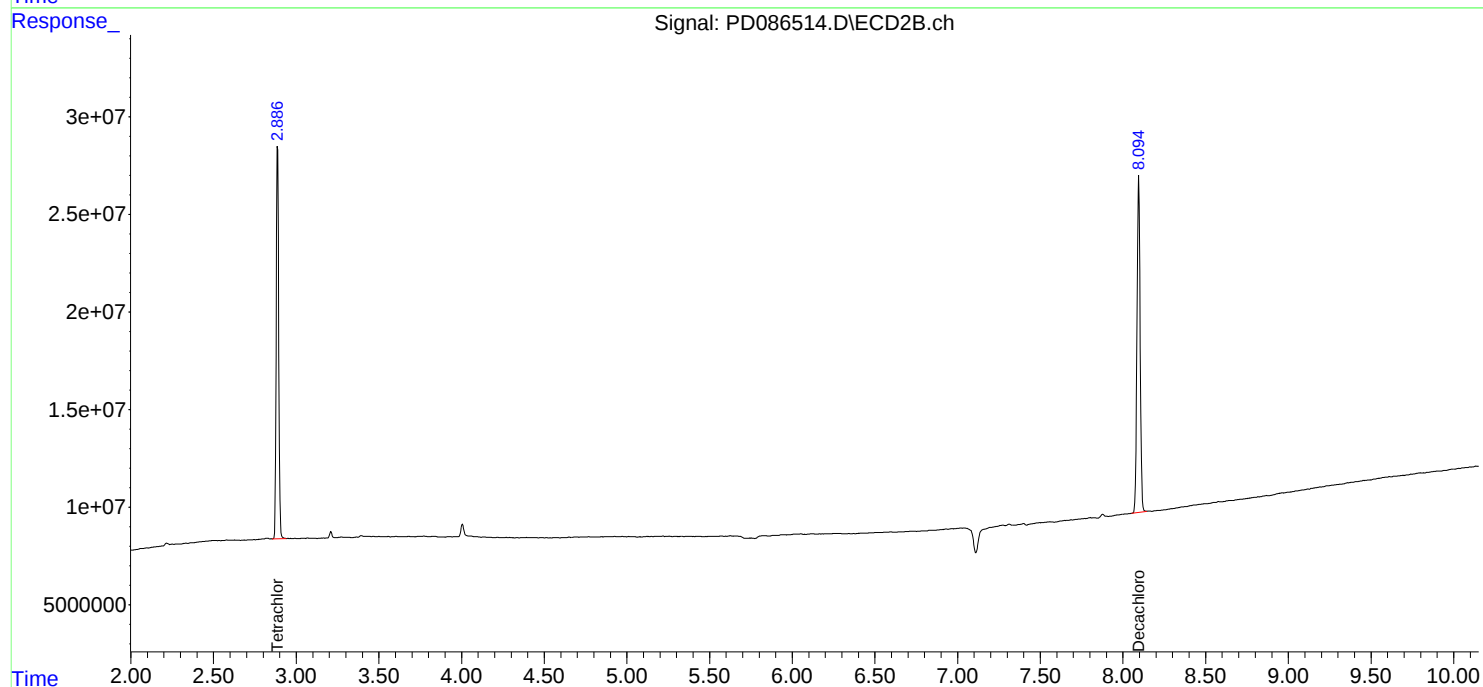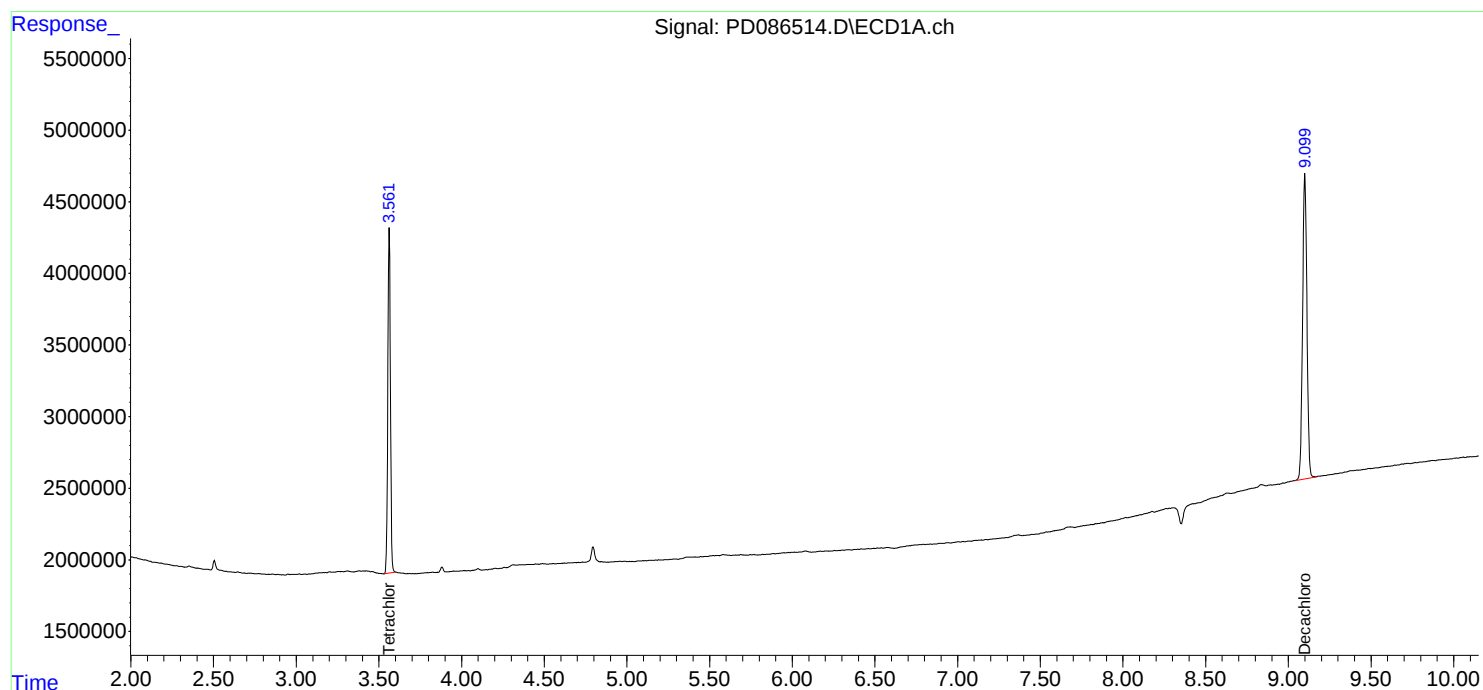


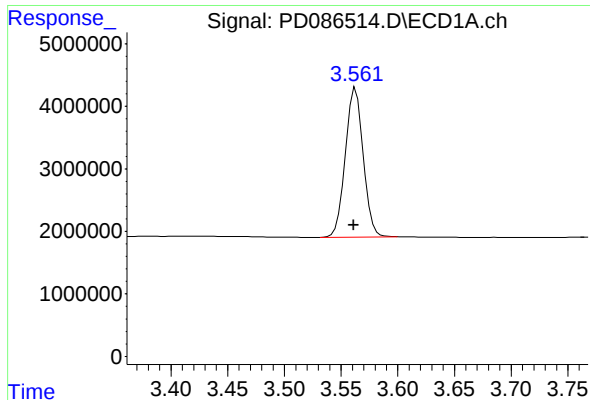

#1 Tetrachloro-m-xylene


R.T.: 3.563 min
Delta R.T.: 0.002 min
Response: 26192672
Conc: 17.93 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB164033BL

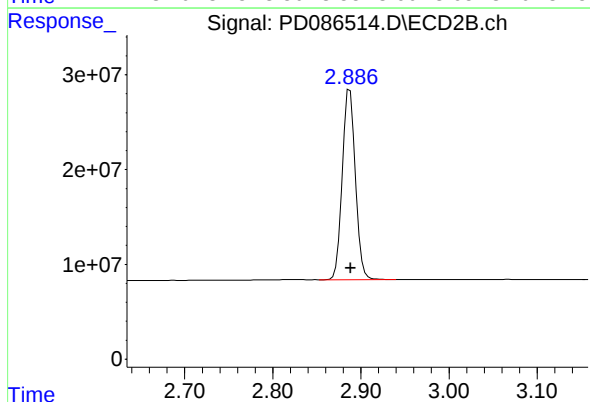


#1 Tetrachloro-m-xylene

R.T.: 2.887 min
Delta R.T.: -0.001 min
Response: 207675033
Conc: 21.00 ng/ml

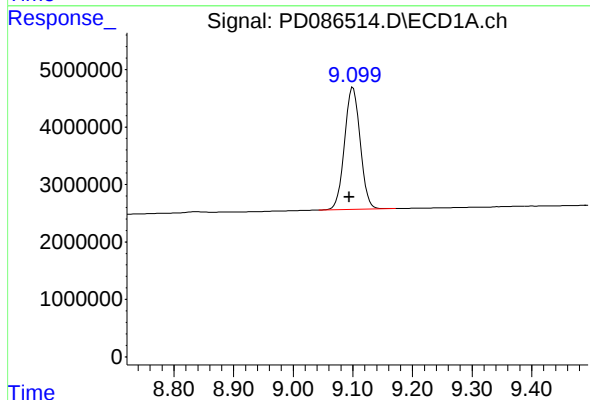

#28 Decachlorobiphenyl

R.T.: 9.100 min
Delta R.T.: 0.006 min
Response: 38797399
Conc: 20.24 ng/ml

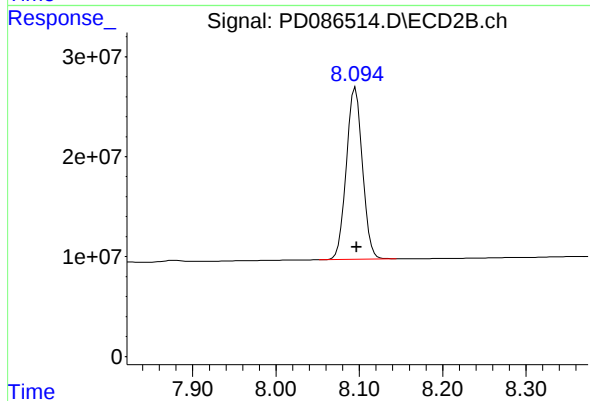

#28 Decachlorobiphenyl

R.T.: 8.095 min
Delta R.T.: -0.001 min
Response: 229298086
Conc: 21.41 ng/ml