

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111221\
 Data File : PD066904.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Nov 2021 13:14
 Operator : AR\AJ
 Sample : M4419-04DL 4X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0HF3DL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/15/2021
 Supervised By : mohammad ahmed 11/15/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 13 01:06:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 27 16:50:52 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.438	3.959	5582117	23955160	2.888	2.766m
27)	SA Decachlor...	8.164	9.027	6983384	34358771	5.960	6.588
Target Compounds							
2)	A alpha-BHC	3.875	4.362	30568796	145.8E6	10.444	13.330 #
6)	B beta-BHC	4.405	4.824	90083884	336.1E6	71.720	68.215
7)	B delta-BHC	4.603	5.018	11022518	265.2E6	4.159	26.807 #
8)	B Heptachlo...	5.128	5.824	23346493	84325575	9.185m	11.217m
9)	A Endosulfan I	5.468	6.210	33259162	23032439	14.510	2.944 #
10)	B trans-Chl...	5.359	6.073	89532355	153.5E6	34.639m	17.829 #
11)	B cis-Chlor...	5.419	6.145	52954418	240.0E6	20.786	27.968 #
12)	B 4,4'-DDE	5.583	6.305	470.7E6	1161.2E6	206.101	152.495 #
16)	A 4,4'-DDD	6.096	6.800	1945.9E6	5146.0E6	1075.044	797.092 #
17)	MA 4,4'-DDT	6.334	7.096	2325.3E6	6207.8E6	1229.810m	939.698m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111221\
Data File : PD066904.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Nov 2021 13:14
Operator : AR\AJ
Sample : M4419-04DL 4X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 13 01:06:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 27 16:50:52 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

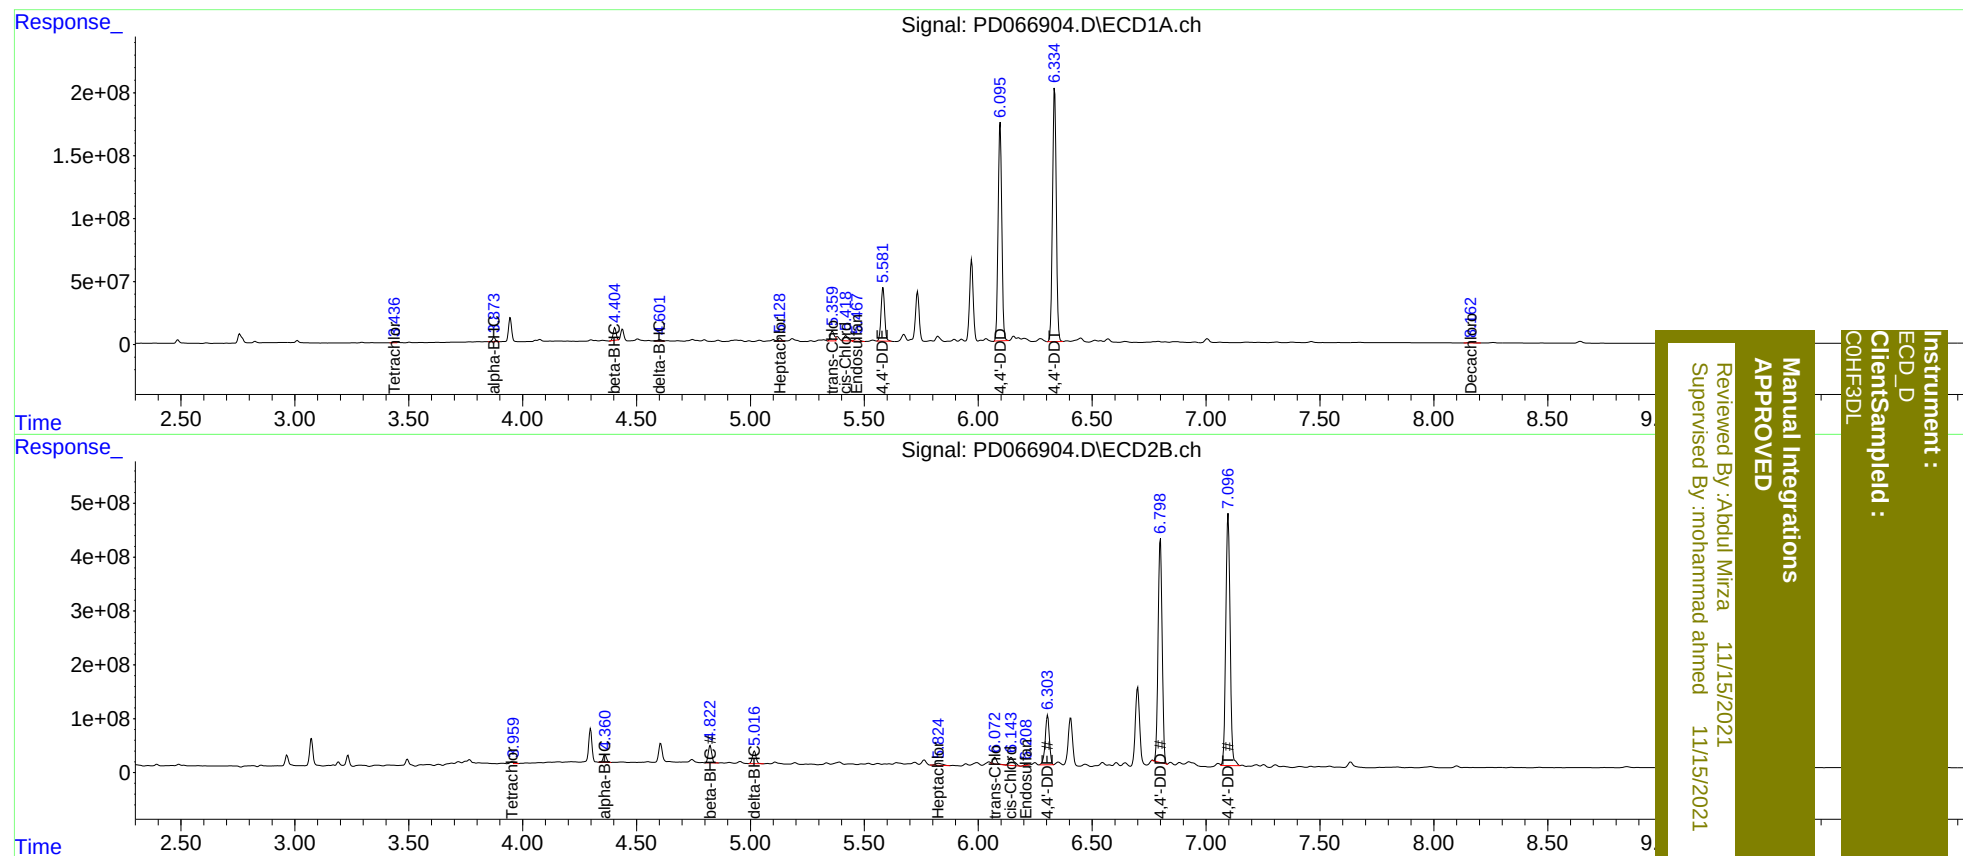

Reviewed By: Abdul Mirza 11/15/2021
Supervised By: mohammad ahmed 11/15/2021

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
COHF3DL