

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111223\
 Data File : PD079569.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Nov 2023 19:53
 Operator : AR\AJ
 Sample : PEM
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 20:22:06 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102023.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 20 04:44:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	2.804	29550999	47494454	18.303	20.514
28)	SA Decachlor...	9.115	7.948	37081067	49888664	18.485	20.467
Target Compounds							
2)	A alpha-BHC	4.025	3.306	23908870	36355842	8.981	10.485
3)	MA gamma-BHC...	4.359	3.636	23378095	35070869	8.996	10.328
4)	MA Heptachlor	4.966	0.000	309037	0	0.116	N.D. #
5)	MB Aldrin	0.000	4.265	0	114397	N.D.	0.035 #
6)	B beta-BHC	4.552	3.930	11203813	17021874	10.455	12.080
7)	B delta-BHC	0.000	4.185f	0	639779	N.D.	0.191 #
8)	B Heptachlo...	5.714	0.000	611662	0	0.261	N.D. #
12)	B 4,4'-DDE	6.230	5.268	240950	652058	0.114	0.245 #
13)	MA Dieldrin	6.400f	0.000	376549	0	0.162	N.D. #
14)	MA Endrin	6.614	5.670	80954648	129.2E6	41.566	50.496
15)	B Endosulfa...	6.845	5.980	872090	590078	0.428	0.236 #
16)	A 4,4'-DDD	6.745	5.819	1508819	2807997	0.858	1.229 #
17)	MA 4,4'-DDT	7.060	6.069	168.3E6	253.5E6	88.859	110.747
18)	B Endrin al...	6.962	6.143	2586094	5557328	1.675	2.989 #
19)	B Endosulfa...	0.000	6.352f	0	236274	N.D.	0.101 #
20)	A Methoxychlor	7.534	6.644	219.8E6	321.8E6	200.628	237.002
21)	B Endrin ke...	7.682	6.870	6239416	9946128	2.862	3.558
22)	Mirex	8.183f	0.000	37747	0	0.022	N.D. #
23)	Chlordane-1	0.000	3.837f	0	333458	N.D.	3.839 #
27)	Chlordane-5	0.000	5.980	0	590078	N.D.	5.921 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111223\
Data File : PD079569.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Nov 2023 19:53
Operator : AR\AJ
Sample : PEM
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 20:22:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102023.M
Quant Title : GC Extractables
QLast Update : Fri Oct 20 04:44:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

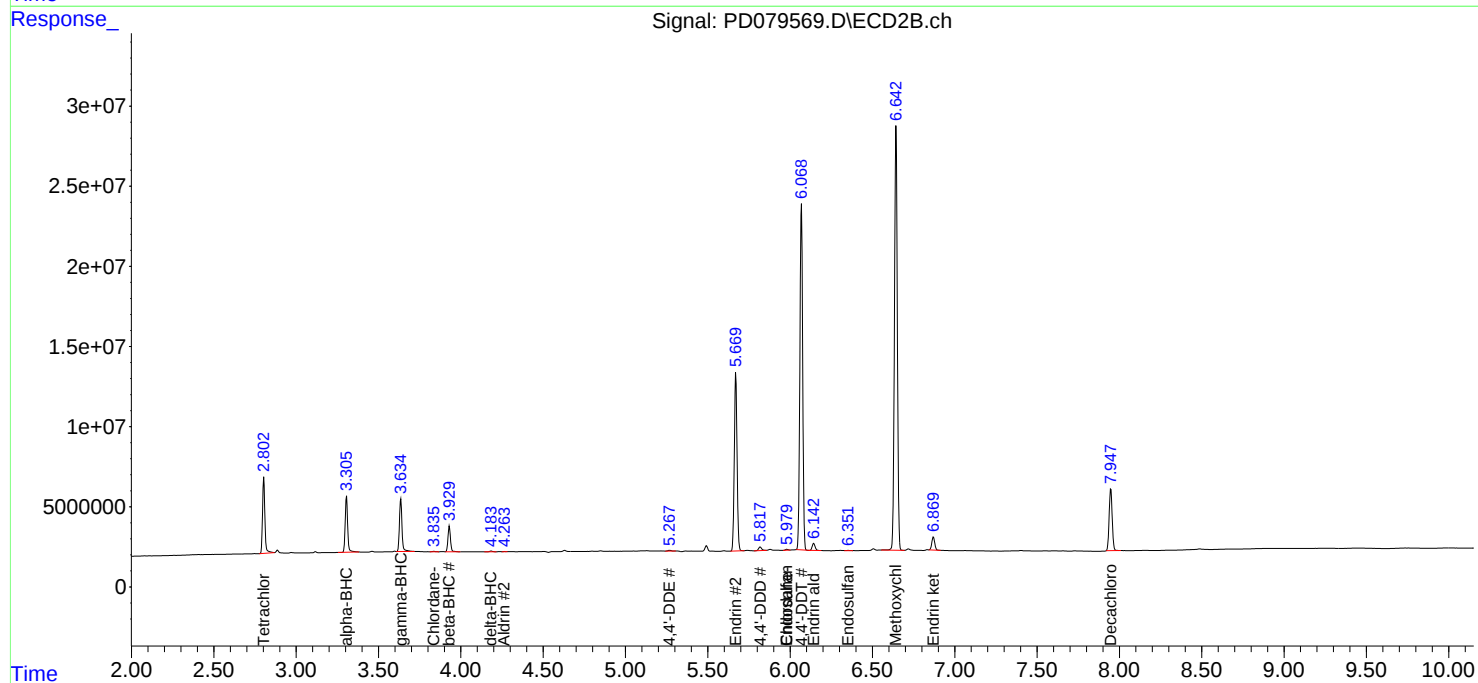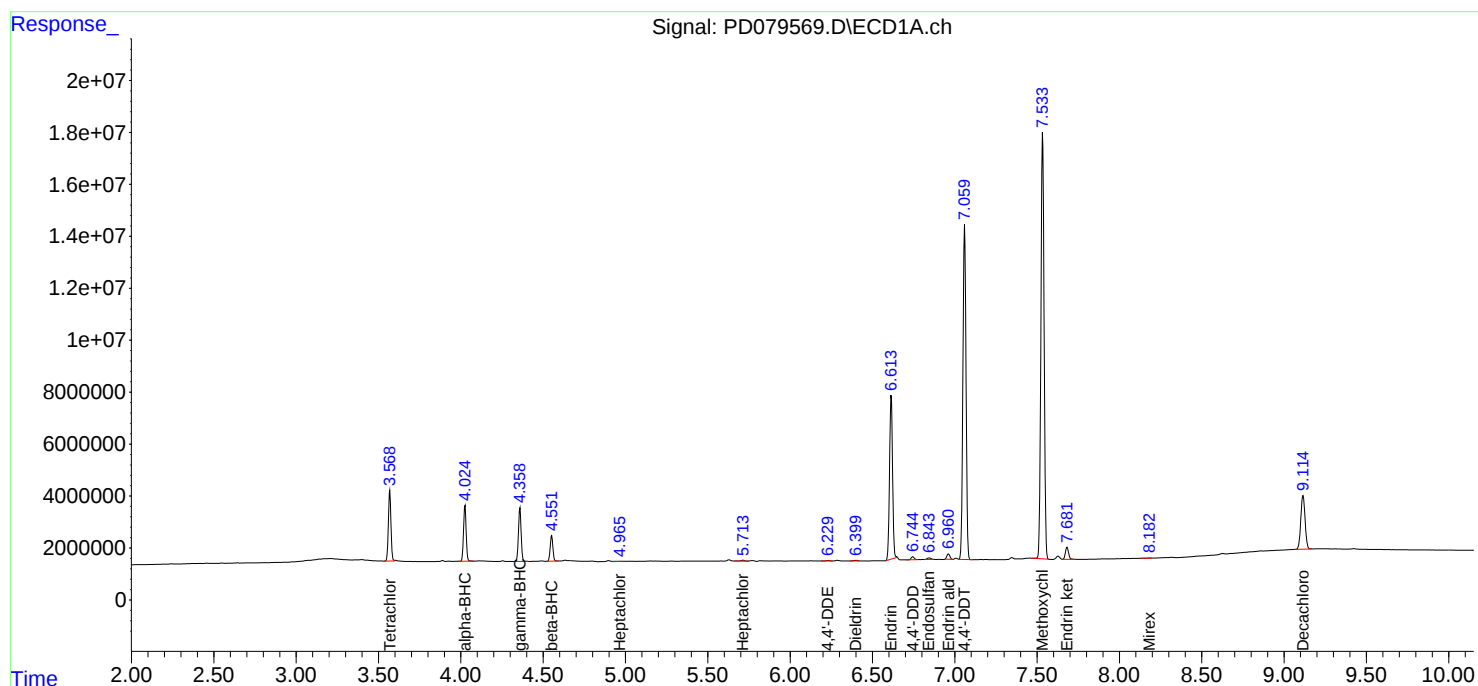


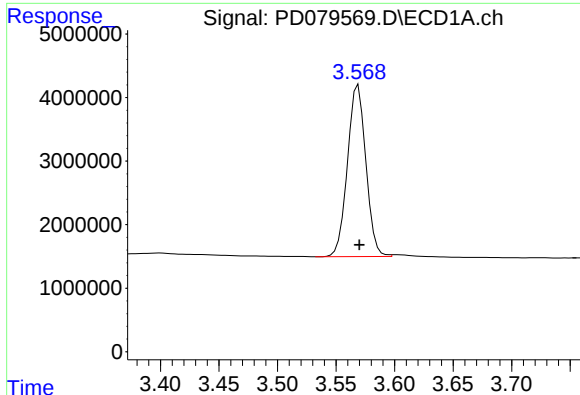

#1 Tetrachloro-m-xylene


R.T.: 3.569 min
Delta R.T.: -0.001 min
Response: 29550999
Conc: 18.30 ng/ml

Instrument :
ECD_D
ClientSampleId :

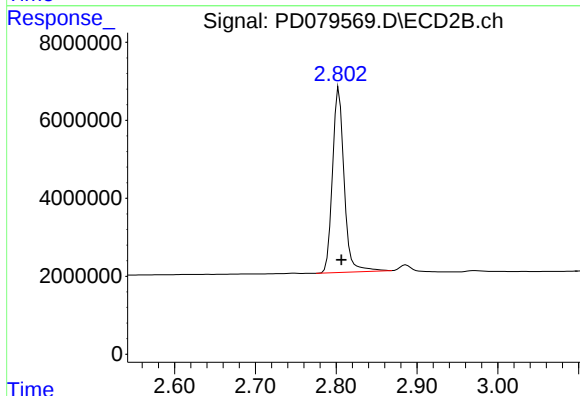


#1 Tetrachloro-m-xylene

R.T.: 2.804 min
Delta R.T.: -0.003 min
Response: 47494454
Conc: 20.51 ng/ml

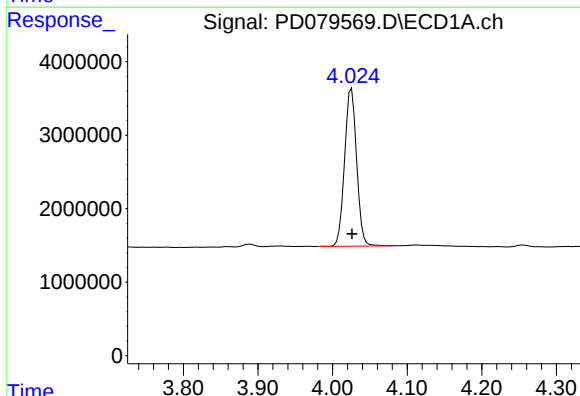


#2 alpha-BHC

R.T.: 4.025 min
Delta R.T.: 0.000 min
Response: 23908870
Conc: 8.98 ng/ml

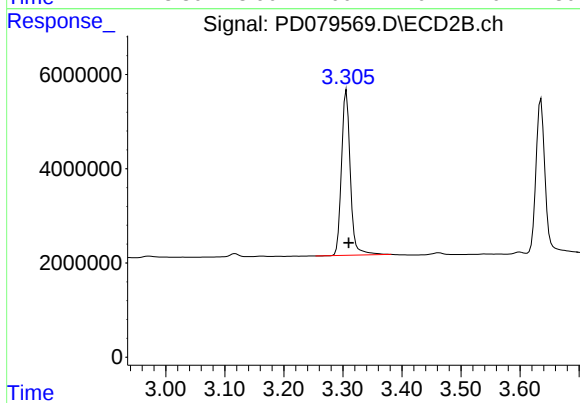

#2 alpha-BHC


R.T.: 3.306 min
Delta R.T.: -0.004 min
Response: 36355842
Conc: 10.48 ng/ml

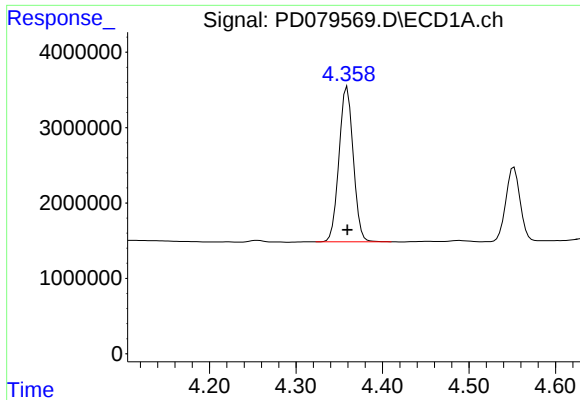

#3 gamma-BHC (Lindane)


R.T.: 4.359 min
Delta R.T.: 0.000 min
Response: 23378095
Conc: 9.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

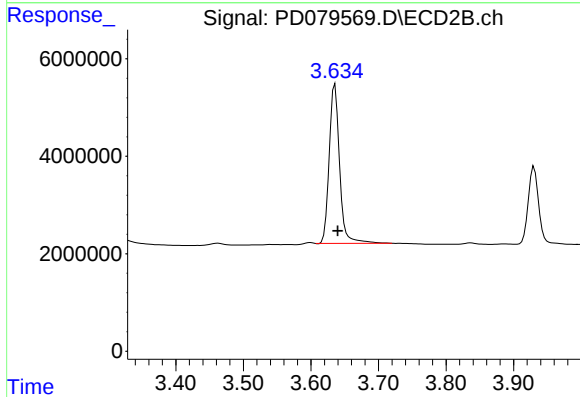


#3 gamma-BHC (Lindane)

R.T.: 3.636 min
Delta R.T.: -0.004 min
Response: 35070869
Conc: 10.33 ng/ml

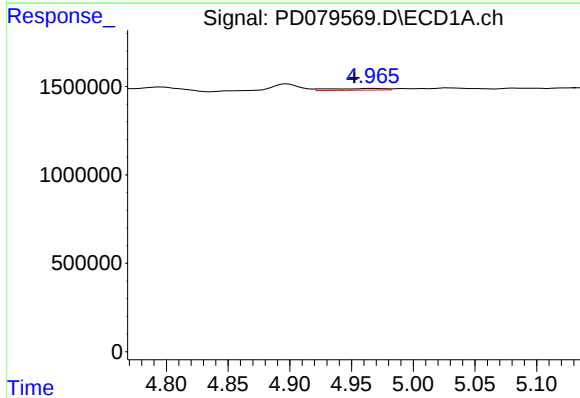


#4 Heptachlor

R.T.: 4.966 min
Delta R.T.: 0.014 min
Response: 309037
Conc: 0.12 ng/ml

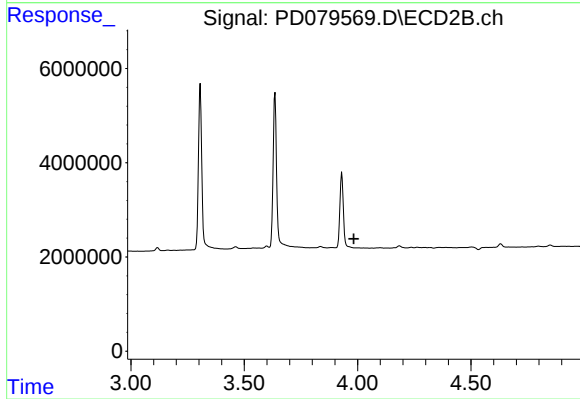

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 3.983 min
Response: 0
Conc: N.D.

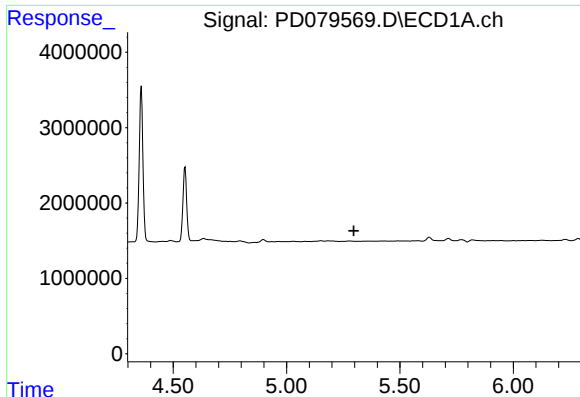

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.296 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

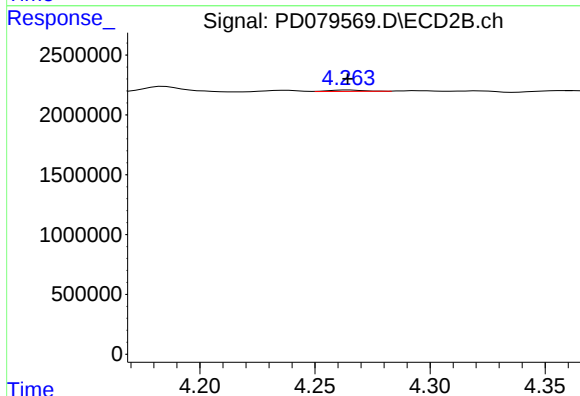


#5 Aldrin

R.T.: 4.265 min
Delta R.T.: 0.000 min
Response: 114397
Conc: 0.03 ng/ml

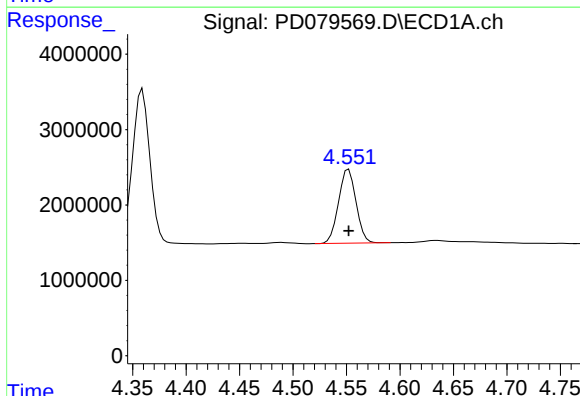


#6 beta-BHC

R.T.: 4.552 min
Delta R.T.: 0.000 min
Response: 11203813
Conc: 10.46 ng/ml

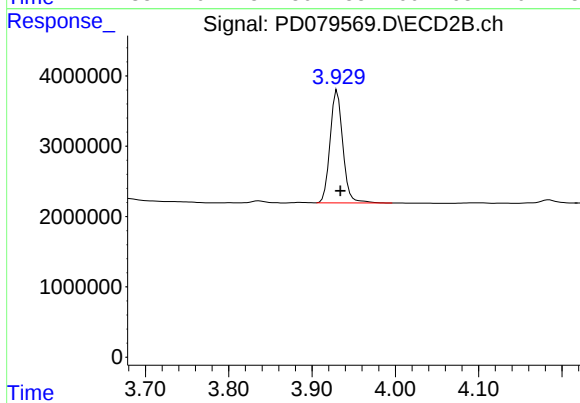

#6 beta-BHC


R.T.: 3.930 min
Delta R.T.: -0.004 min
Response: 17021874
Conc: 12.08 ng/ml

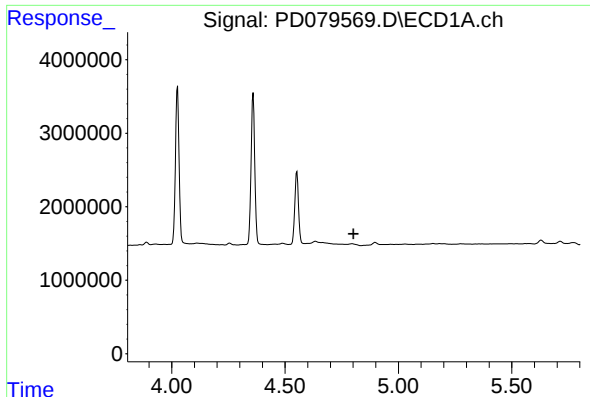

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.802 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

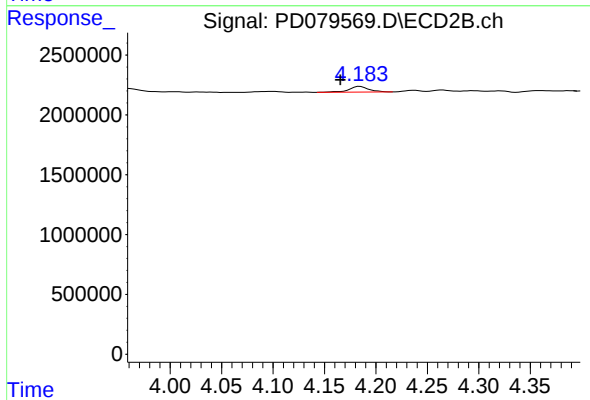


#7 delta-BHC

R.T.: 4.185 min
Delta R.T.: 0.019 min
Response: 639779
Conc: 0.19 ng/ml

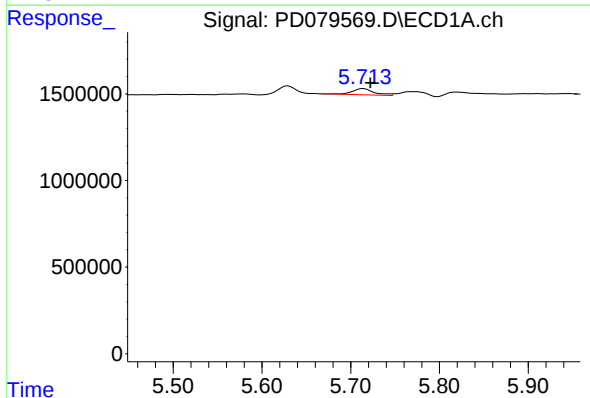


#8 Heptachlor epoxide

R.T.: 5.714 min
Delta R.T.: -0.008 min
Response: 611662
Conc: 0.26 ng/ml

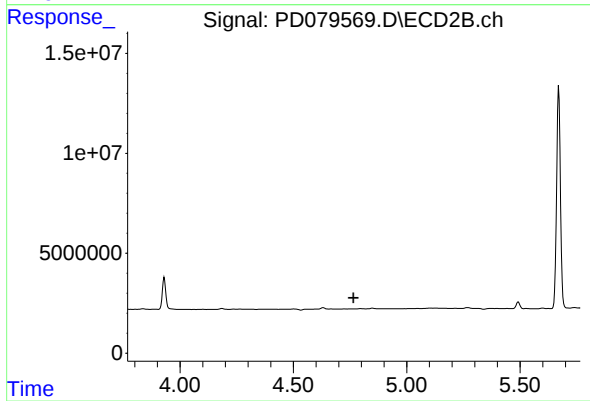

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.766 min
Response: 0
Conc: N.D.

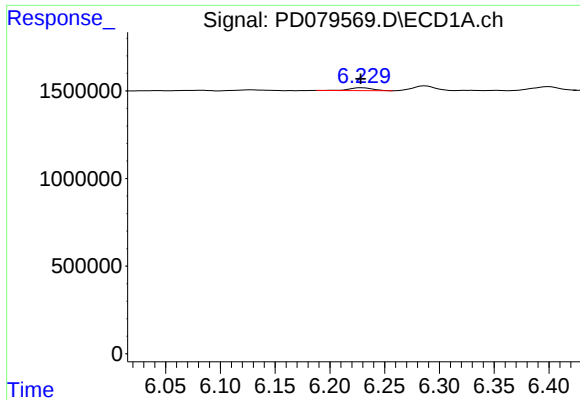

#12 4,4'-DDE


R.T.: 6.230 min
Delta R.T.: 0.001 min
Response: 240950
Conc: 0.11 ng/ml

Instrument :
ECD_D
ClientSampleId :

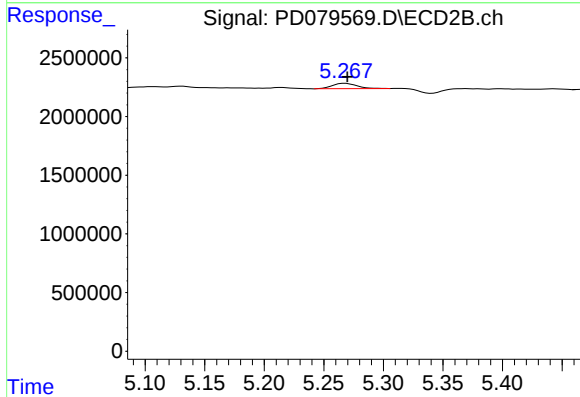


#12 4,4'-DDE

R.T.: 5.268 min
Delta R.T.: -0.002 min
Response: 652058
Conc: 0.24 ng/ml

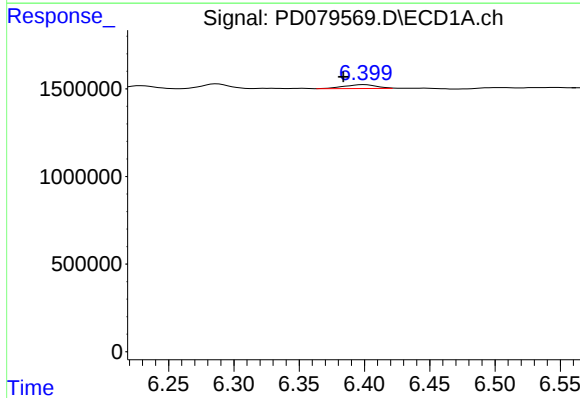


#13 Dieldrin

R.T.: 6.400 min
Delta R.T.: 0.016 min
Response: 376549
Conc: 0.16 ng/ml

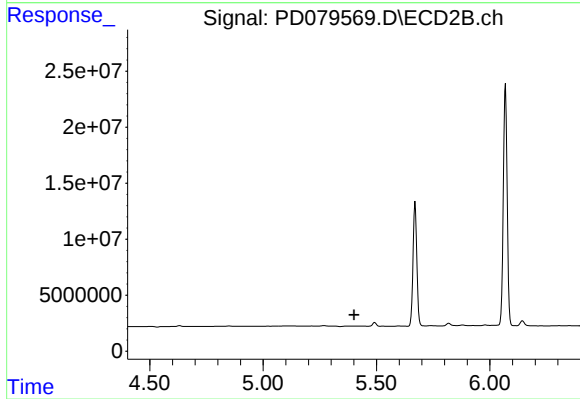

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 5.401 min
Response: 0
Conc: N.D.

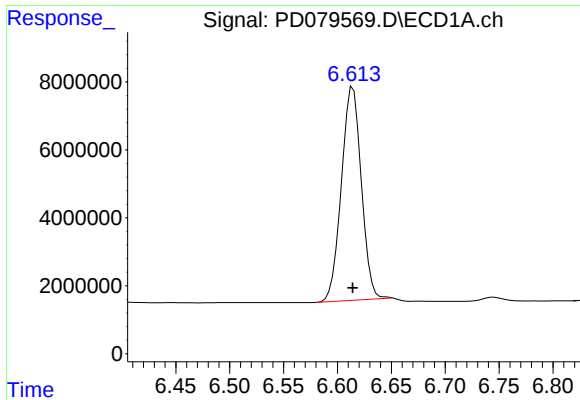

#14 Endrin


R.T.: 6.614 min
Delta R.T.: 0.000 min
Response: 80954648
Conc: 41.57 ng/ml

Instrument :
ECD_D
ClientSampleId :

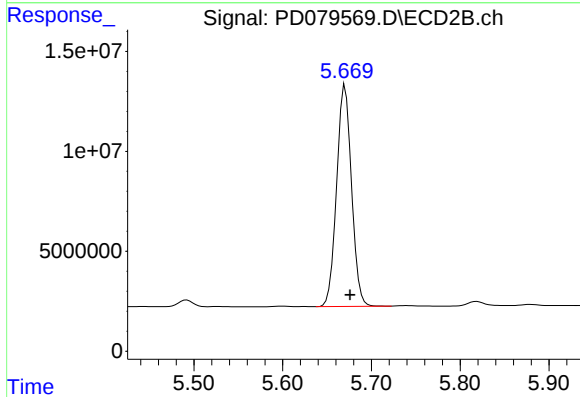


#14 Endrin

R.T.: 5.670 min
Delta R.T.: -0.006 min
Response: 129224957
Conc: 50.50 ng/ml

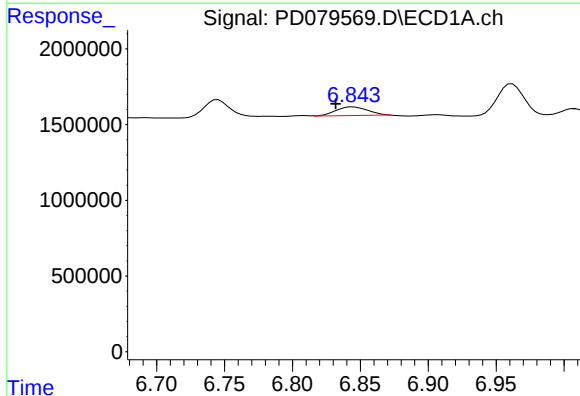


#15 Endosulfan II

R.T.: 6.845 min
Delta R.T.: 0.013 min
Response: 872090
Conc: 0.43 ng/ml

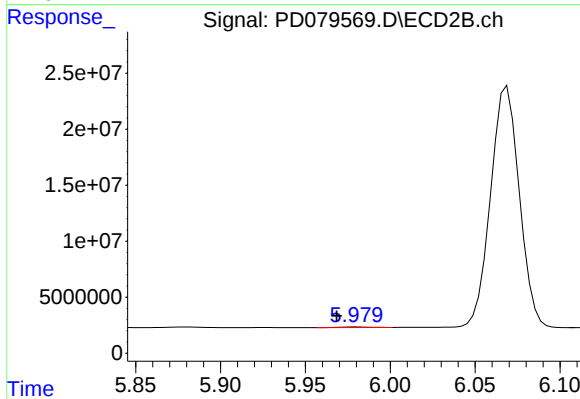

#15 Endosulfan II


R.T.: 5.980 min
Delta R.T.: 0.012 min
Response: 590078
Conc: 0.24 ng/ml

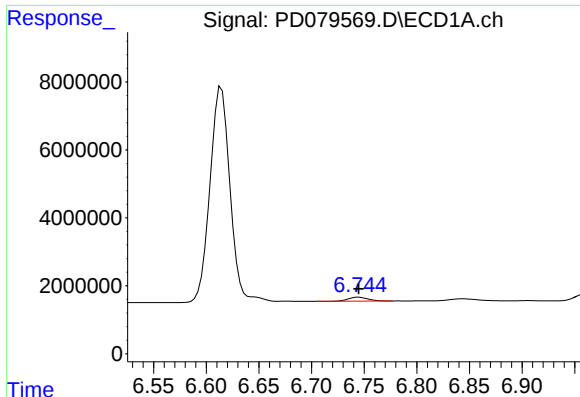

#16 4,4'-DDD


R.T.: 6.745 min
Delta R.T.: 0.000 min
Response: 1508819
Conc: 0.86 ng/ml

Instrument :
ECD_D
ClientSampleId :

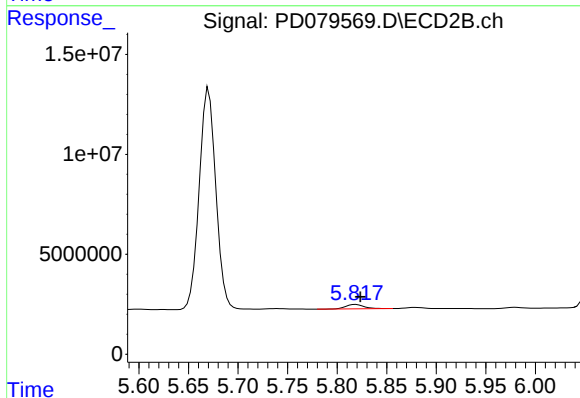


#16 4,4'-DDD

R.T.: 5.819 min
Delta R.T.: -0.005 min
Response: 2807997
Conc: 1.23 ng/ml

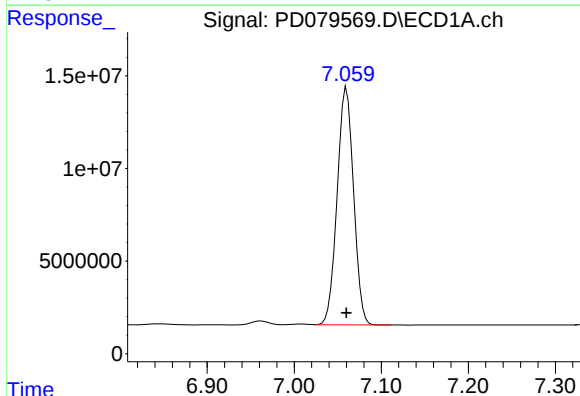


#17 4,4'-DDT

R.T.: 7.060 min
Delta R.T.: 0.000 min
Response: 168270580
Conc: 88.86 ng/ml

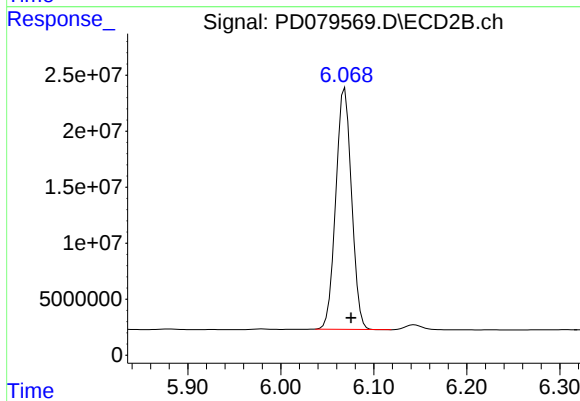

#17 4,4'-DDT


R.T.: 6.069 min
Delta R.T.: -0.007 min
Response: 253542184
Conc: 110.75 ng/ml

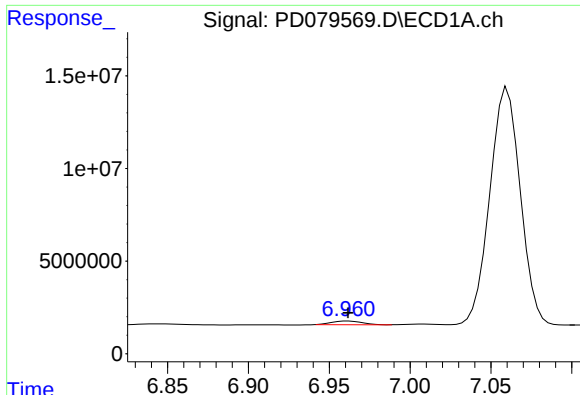

#18 Endrin aldehyde


R.T.: 6.962 min
Delta R.T.: 0.000 min
Response: 2586094
Conc: 1.67 ng/ml

Instrument :
ECD_D
ClientSampleId :

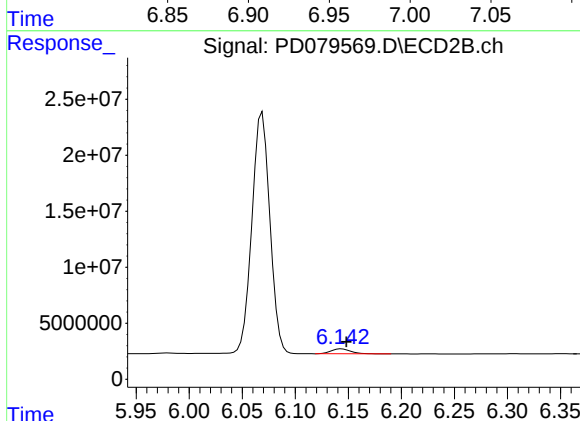


#18 Endrin aldehyde

R.T.: 6.143 min
Delta R.T.: -0.005 min
Response: 5557328
Conc: 2.99 ng/ml

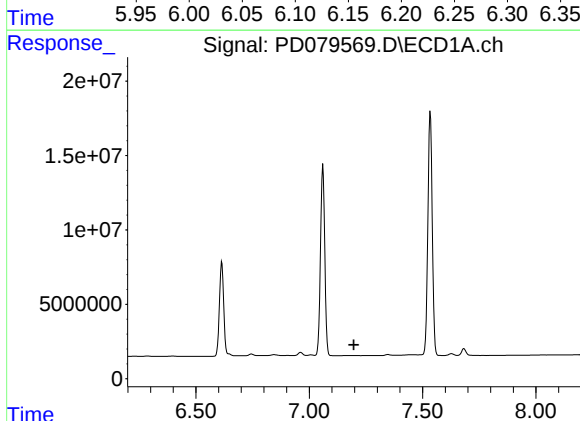


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.196 min
Response: 0
Conc: N.D.

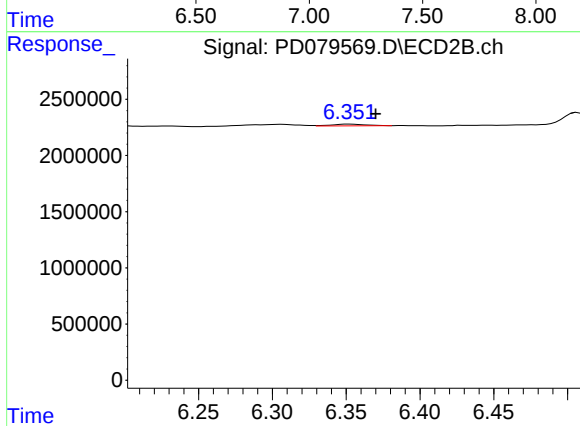

#19 Endosulfan Sulfate


R.T.: 6.352 min
Delta R.T.: -0.018 min
Response: 236274
Conc: 0.10 ng/ml

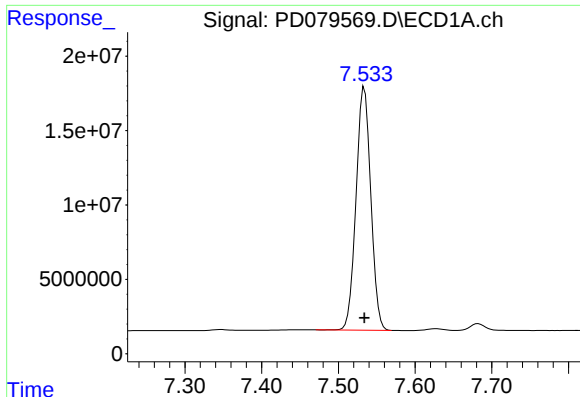

#20 Methoxychlor


R.T.: 7.534 min
Delta R.T.: 0.000 min
Response: 219843873
Conc: 200.63 ng/ml

Instrument :
ECD_D
ClientSampleId :

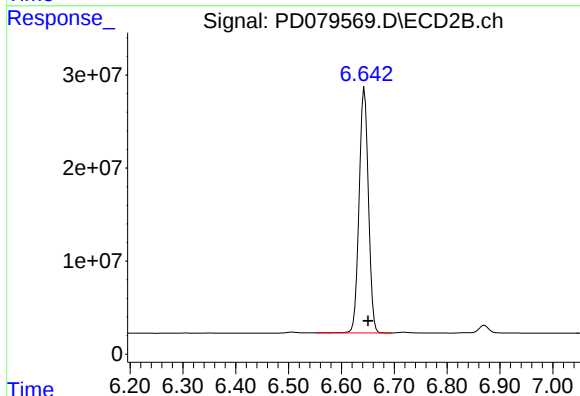


#20 Methoxychlor

R.T.: 6.644 min
Delta R.T.: -0.006 min
Response: 321760764
Conc: 237.00 ng/ml

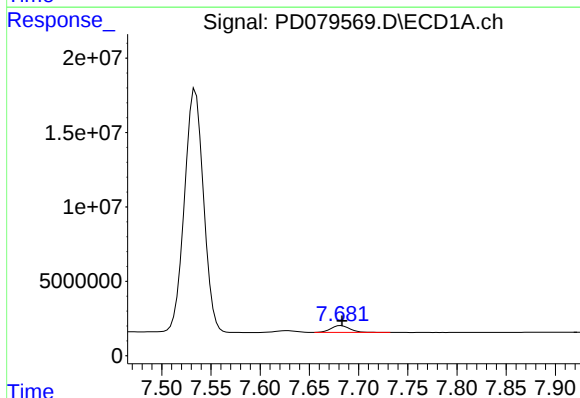


#21 Endrin ketone

R.T.: 7.682 min
Delta R.T.: 0.000 min
Response: 6239416
Conc: 2.86 ng/ml

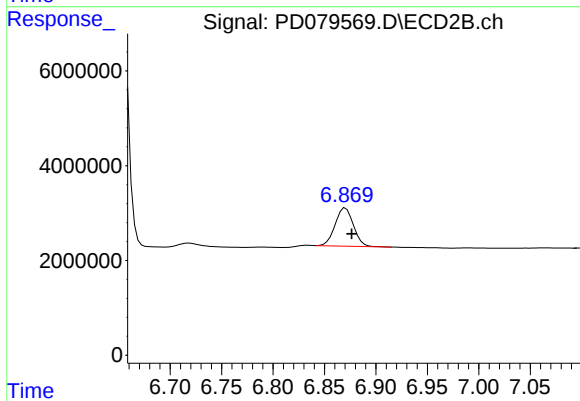

#21 Endrin ketone


R.T.: 6.870 min
Delta R.T.: -0.006 min
Response: 9946128
Conc: 3.56 ng/ml

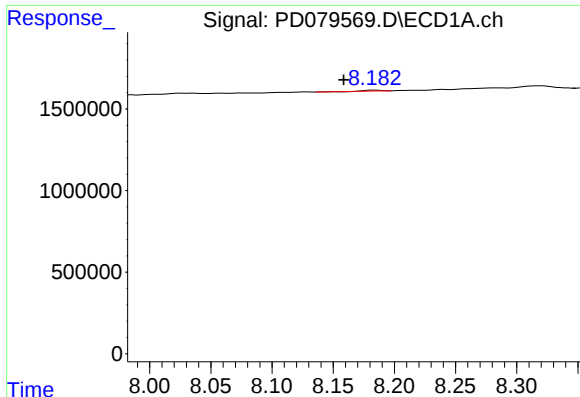

#22 Mirex


R.T.: 8.183 min
Delta R.T.: 0.025 min
Response: 37747
Conc: 0.02 ng/ml

Instrument :
ECD_D
ClientSampleId :

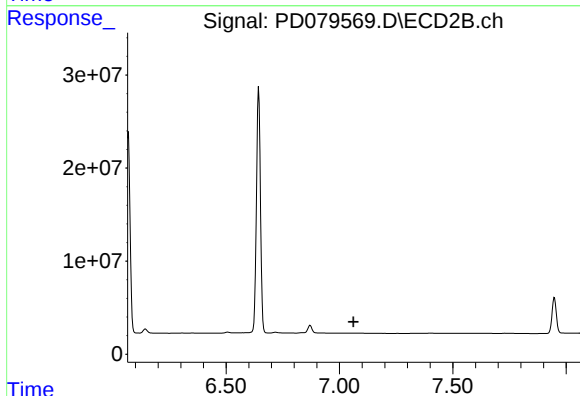


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 7.062 min
Response: 0
Conc: N.D.

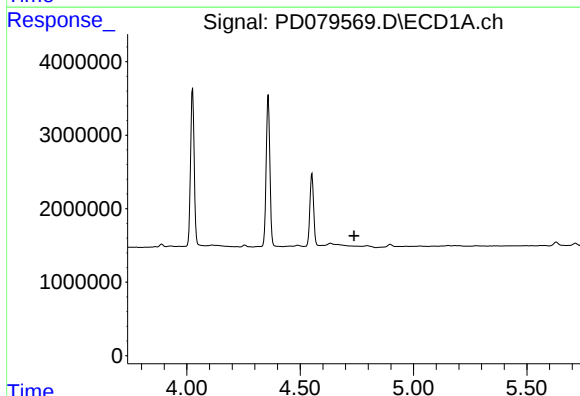


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.738 min
Response: 0
Conc: N.D.

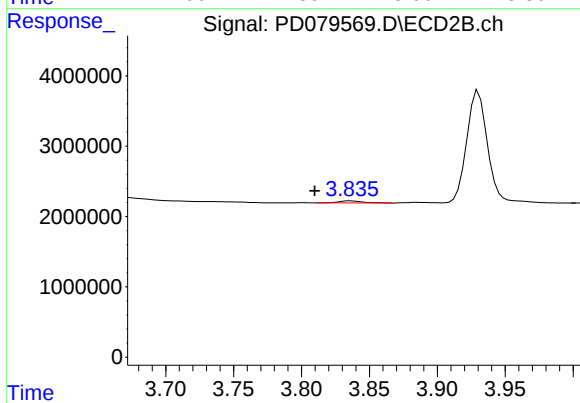

#23 Chlordane-1


R.T.: 3.837 min
Delta R.T.: 0.027 min
Response: 333458
Conc: 3.84 ng/ml

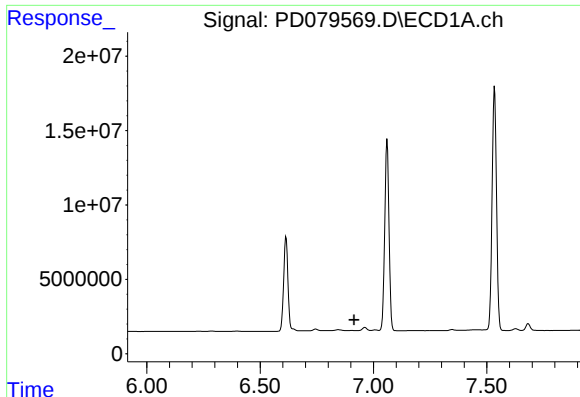

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.914 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

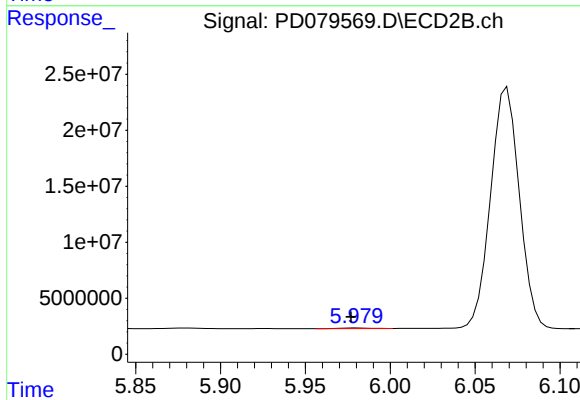


#27 Chlordane-5

R.T.: 5.980 min
Delta R.T.: 0.003 min
Response: 590078
Conc: 5.92 ng/ml

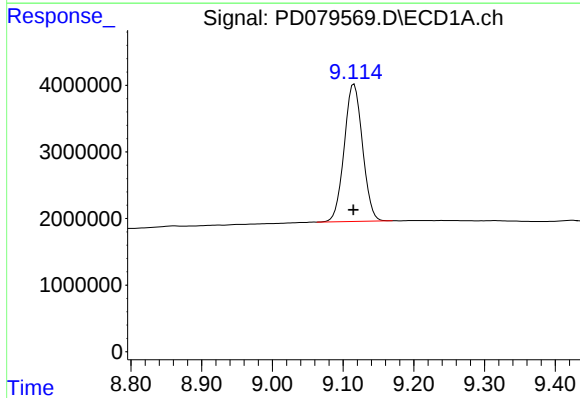

#28 Decachlorobiphenyl

R.T.: 9.115 min
Delta R.T.: 0.000 min
Response: 37081067
Conc: 18.48 ng/ml

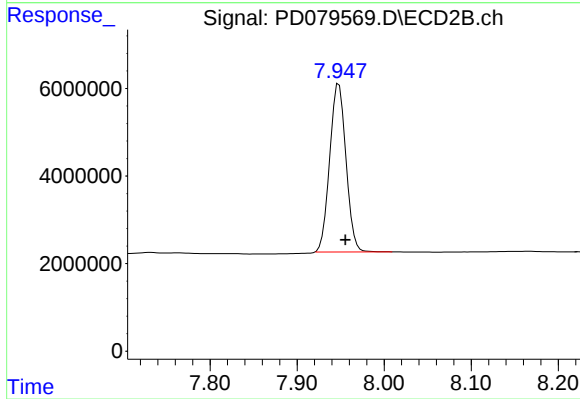

#28 Decachlorobiphenyl

R.T.: 7.948 min
Delta R.T.: -0.007 min
Response: 49888664
Conc: 20.47 ng/ml