

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111223\
 Data File : PD079553.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Nov 2023 14:44
 Operator : AR\AJ
 Sample : PB156875BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB156875BL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/09/2023
 Supervised By : Ankita Jodhani 11/09/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 05:12:07 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX102023.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 20 02:45:52 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.573	2.803	27222920	43632751	18.180	19.788
7) SA Decachlor...	9.120	7.948	38837462	50429360	20.699	22.065m


Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111223\
Data File : PD079553.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Nov 2023 14:44
Operator : AR\AJ
Sample : PB156875BL
Misc :
ALS Vial : 10 Sample Multiplier: 1


Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 05:12:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX102023.M
Quant Title : GC Extractables
QLast Update : Fri Oct 20 02:45:52 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x0.25µm

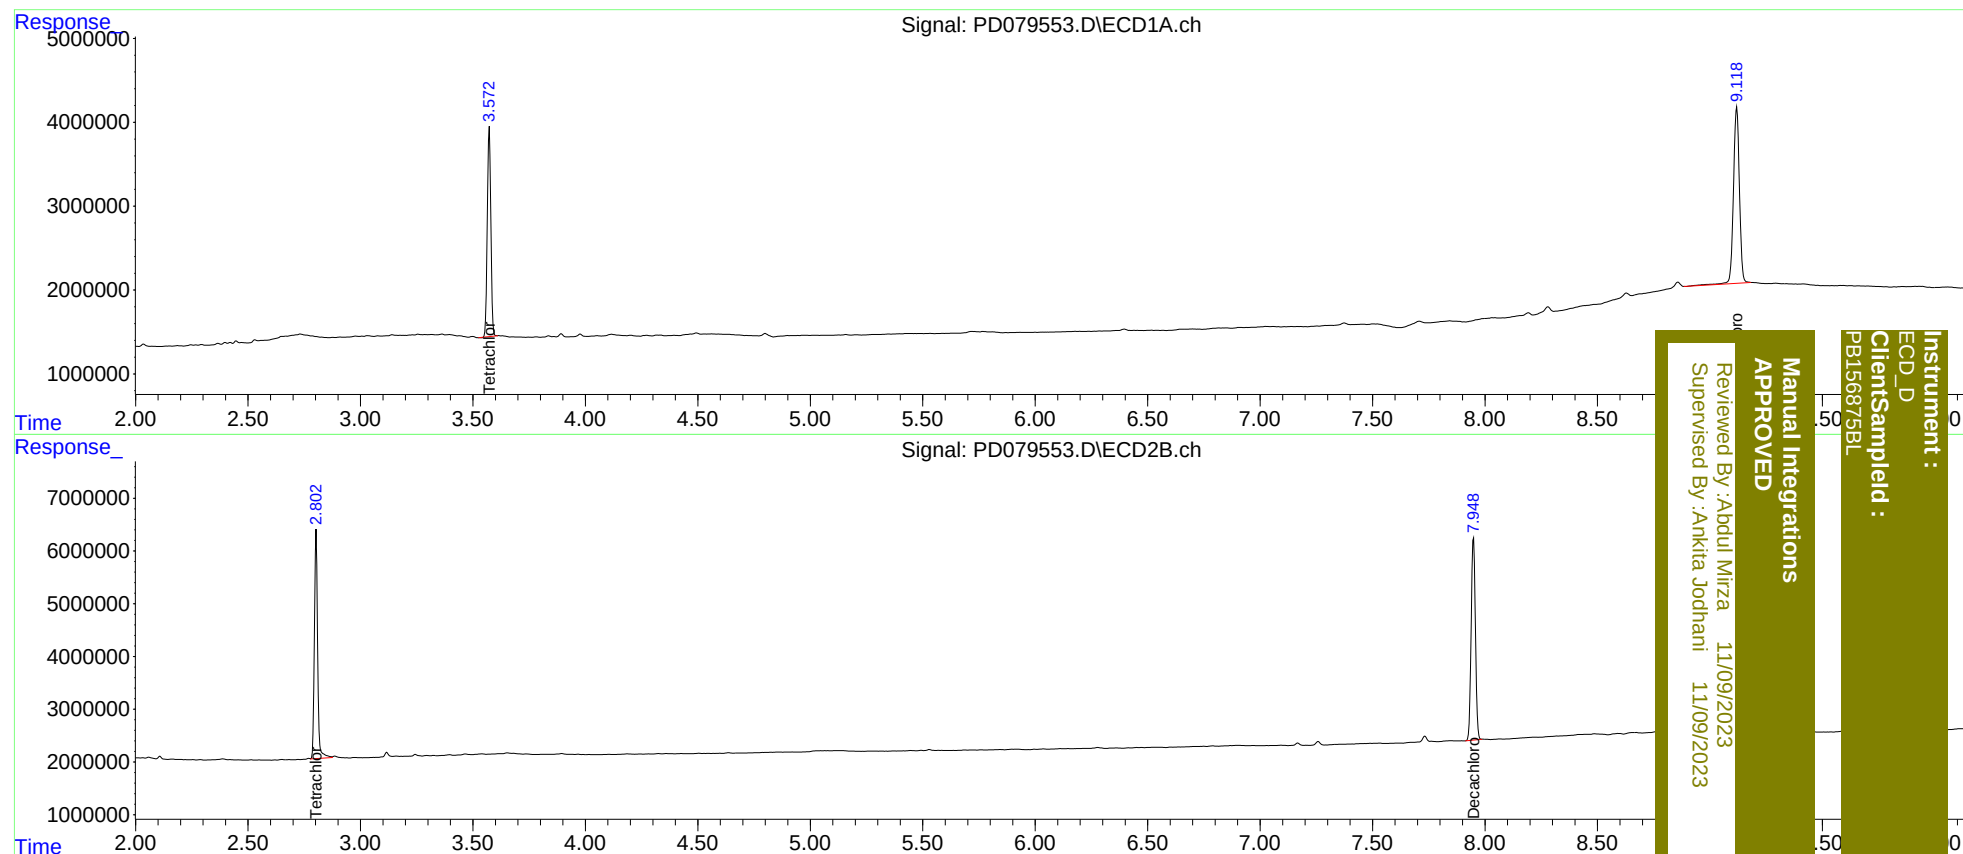

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 11/09/2023
Supervised By: Ankita Jodhani 11/09/2023

Instrument :
ECD_D
Client Sampled :
PB156875BL

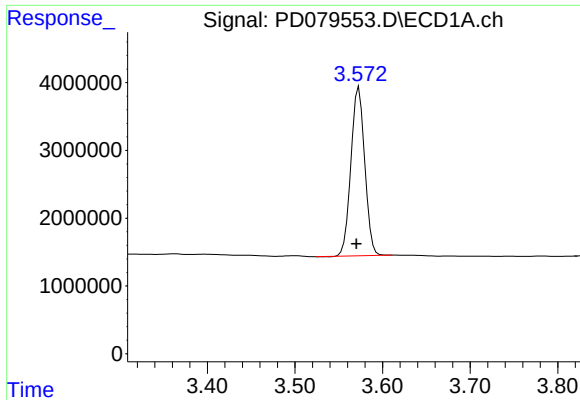


#1 Tetrachloro-m-xylene

R.T.: 3.573 min
Delta R.T.: 0.003 min
Response: 27222920
Conc: 18.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB156875BL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/09/2023
Supervised By :Ankita Jodhani 11/09/2023

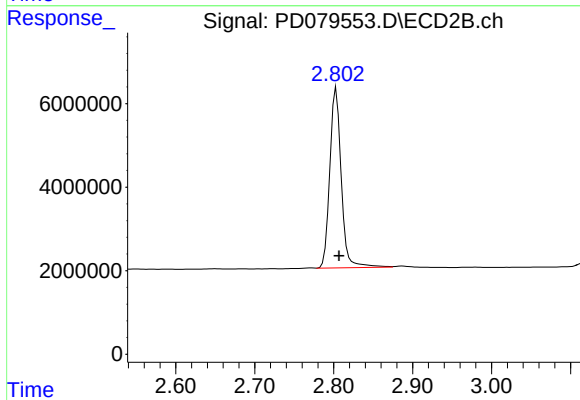


#1 Tetrachloro-m-xylene

R.T.: 2.803 min
Delta R.T.: -0.004 min
Response: 43632751
Conc: 19.79 ng/ml

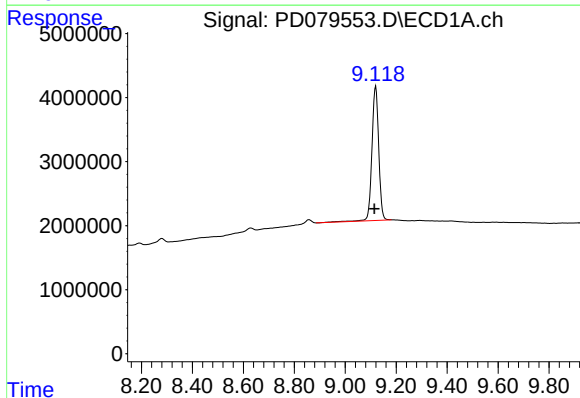

#7 Decachlorobiphenyl

R.T.: 9.120 min
Delta R.T.: 0.005 min
Response: 38837462
Conc: 20.70 ng/ml

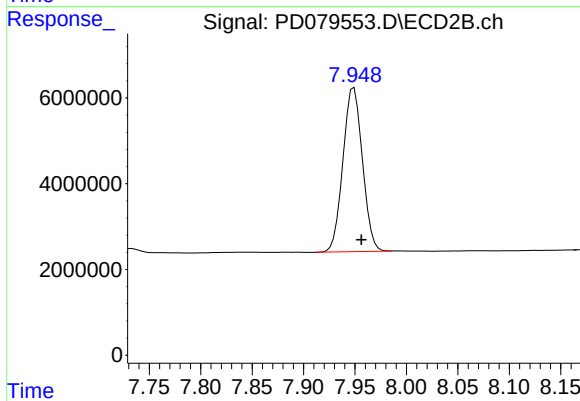

#7 Decachlorobiphenyl

R.T.: 7.948 min
Delta R.T.: -0.009 min
Response: 50429360
Conc: 22.06 ng/ml m