

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111223\
 Data File : PD079586.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Nov 2023 00:07
 Operator : AR\AJ
 Sample : 05102-01
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 67S-IDW-01

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/09/2023
 Supervised By : Ankita Jodhani 11/09/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 04:10:49 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102023.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 20 04:44:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.568	2.804	26001735	46954582	16.104m	20.280 #
28) SA Decachlor...	9.117	7.949	36870083	49846589	18.380	20.450

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111223\
Data File : PD079586.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Nov 2023 00:07
Operator : AR\AJ
Sample : 05102-01
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
67S-IDW-01


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 11/09/2023
Supervised By : Ankita Jodhani 11/09/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 04:10:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102023.M
Quant Title : GC Extractables
QLast Update : Fri Oct 20 04:44:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

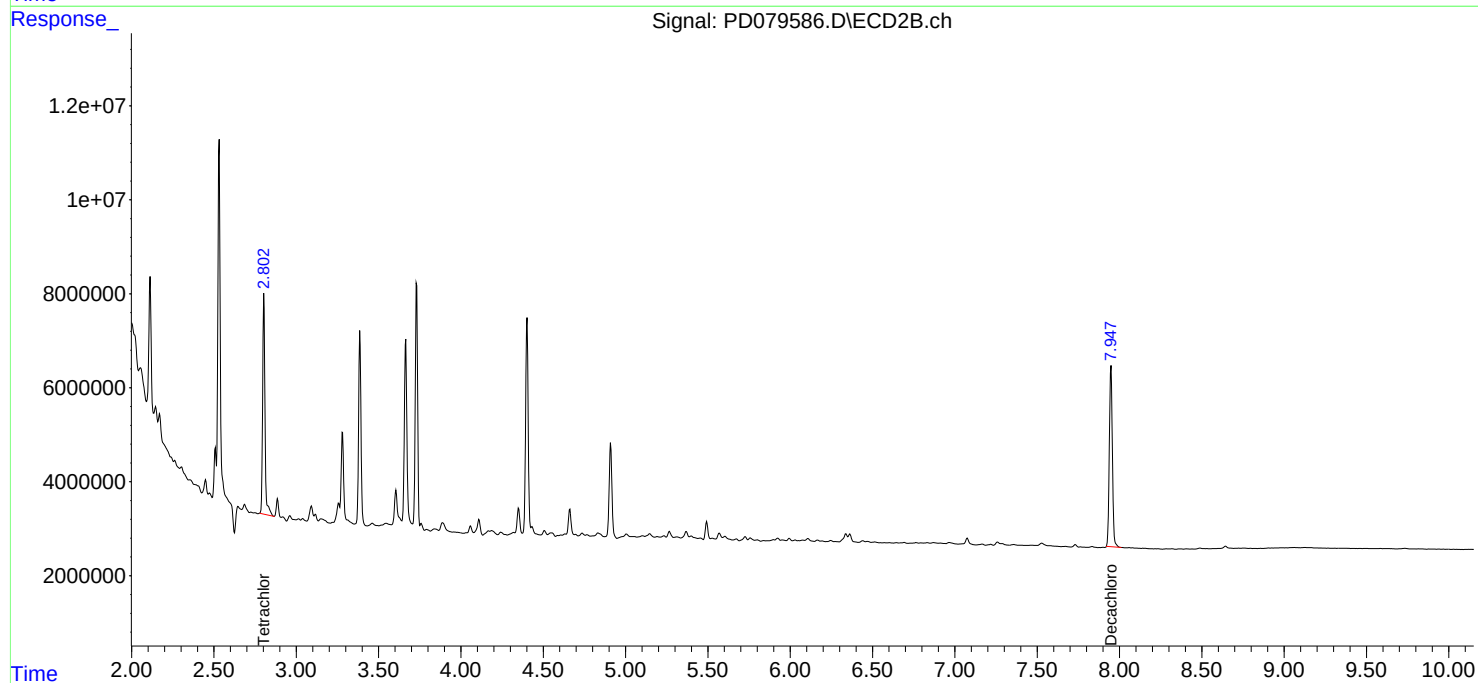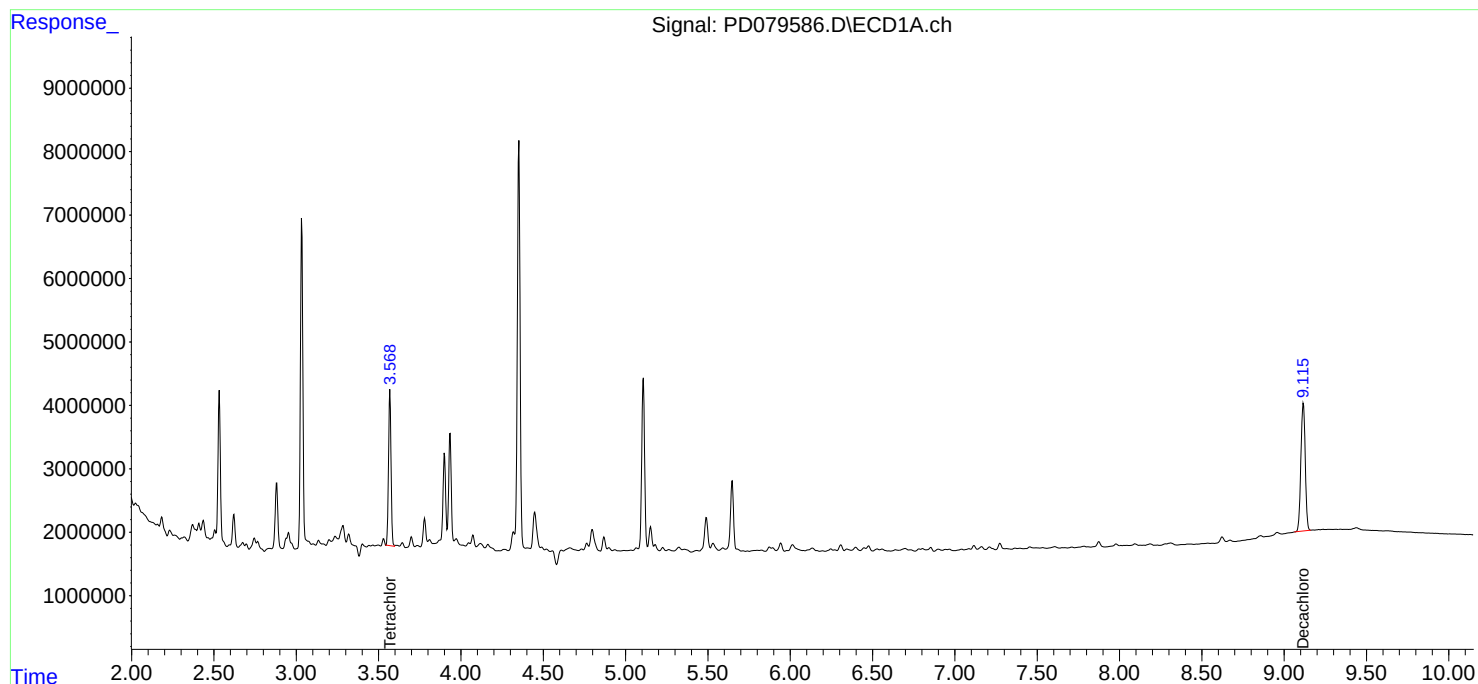

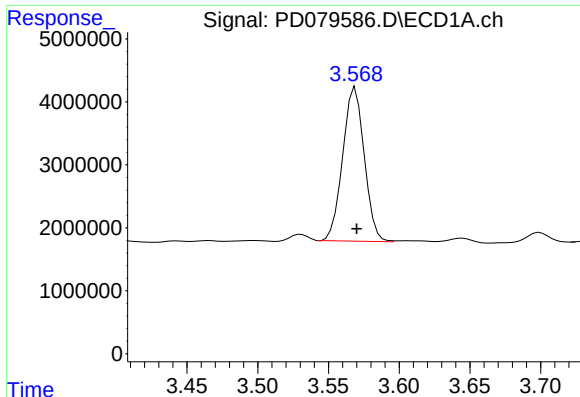


#1 Tetrachloro-m-xylene

R.T.: 3.568 min
Delta R.T.: -0.002 min
Response: 26001735
Conc: 16.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
67S-IDW-01


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/09/2023
Supervised By :Ankita Jodhani 11/09/2023

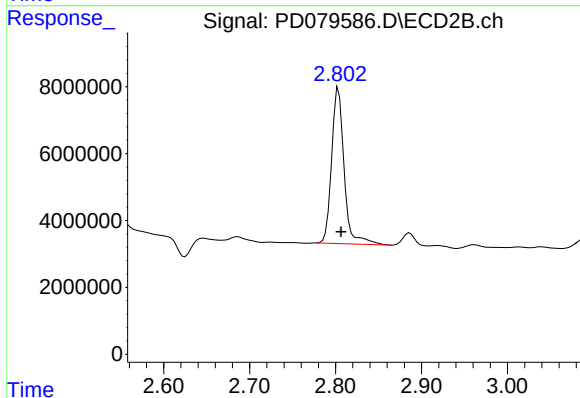


#1 Tetrachloro-m-xylene

R.T.: 2.804 min
Delta R.T.: -0.003 min
Response: 46954582
Conc: 20.28 ng/ml

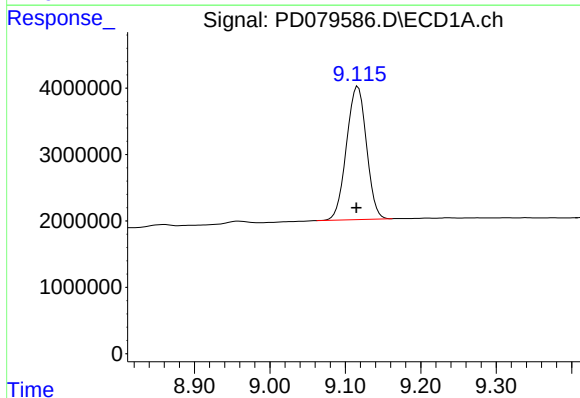

#28 Decachlorobiphenyl

R.T.: 9.117 min
Delta R.T.: 0.002 min
Response: 36870083
Conc: 18.38 ng/ml

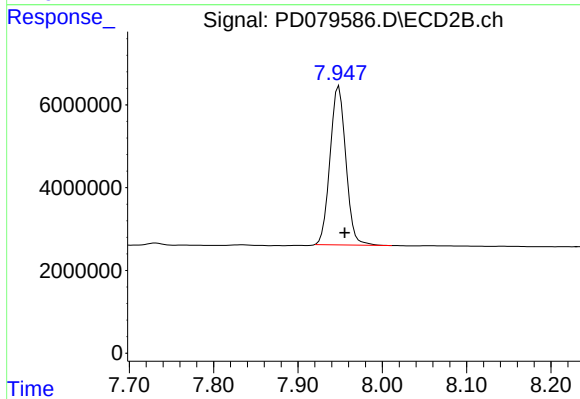

#28 Decachlorobiphenyl

R.T.: 7.949 min
Delta R.T.: -0.007 min
Response: 49846589
Conc: 20.45 ng/ml