

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111225\
 Data File : PD091091.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Nov 2025 11:19
 Operator : AR\AJ
 Sample : Q3593-08
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C-LAW-25-0156-0166-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 11:32:11 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101725.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 17 17:43:28 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	2.876	34024089	209.7E6	10.926	7.043 #
28)	SA Decachlor...	9.083	8.056	186.4E6	842.5E6	39.854	27.812 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111225\
Data File : PD091091.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Nov 2025 11:19
Operator : AR\AJ
Sample : Q3593-08
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
C-LAW-25-0156-0166-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 11:32:11 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101725.M
Quant Title : GC Extractables
QLast Update : Fri Oct 17 17:43:28 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

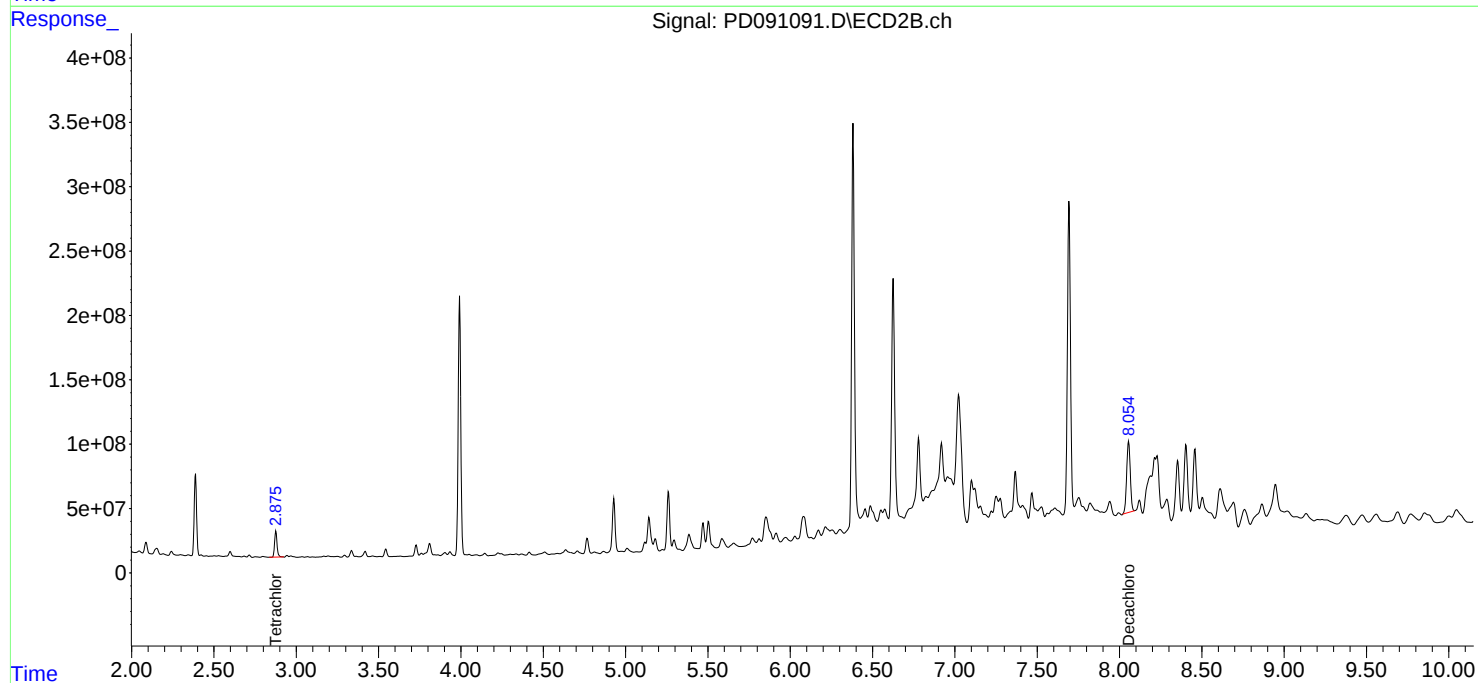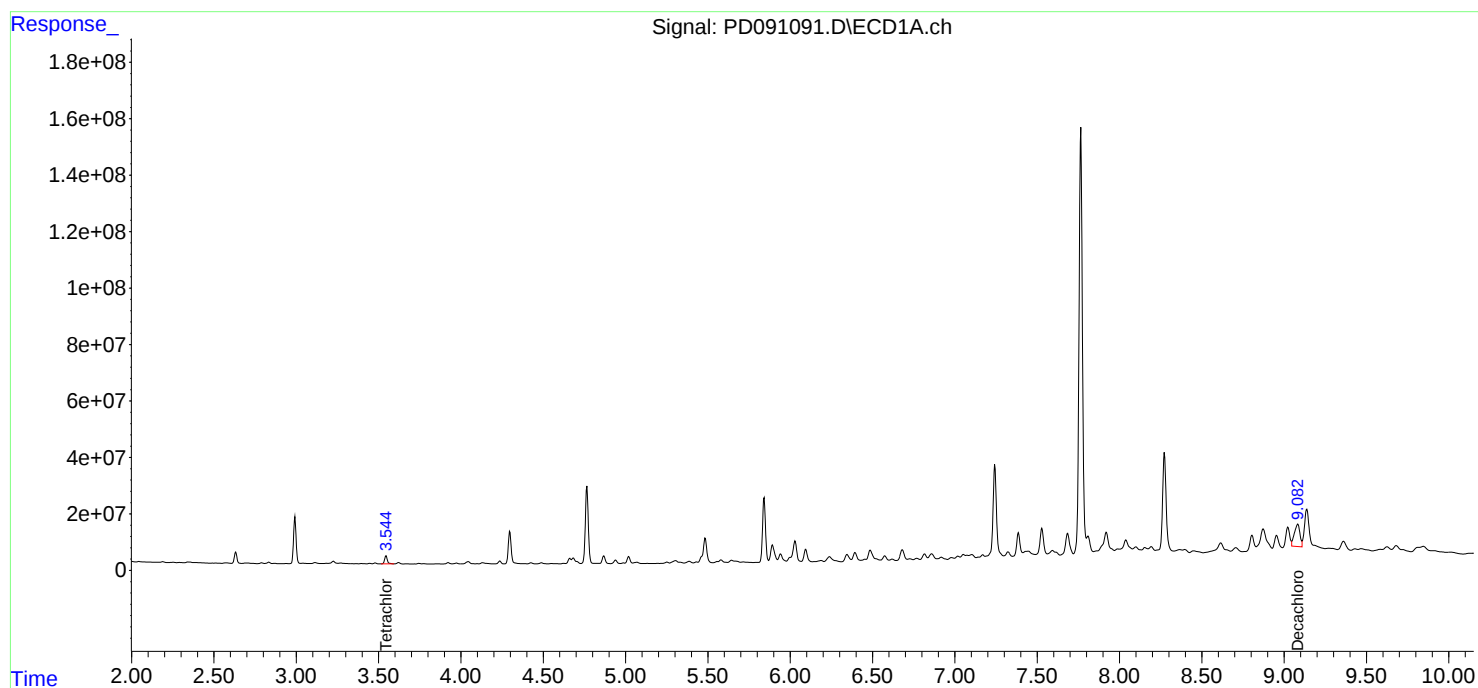


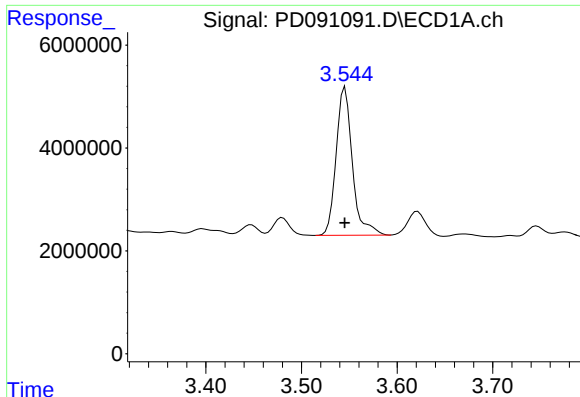

#1 Tetrachloro-m-xylene


R.T.: 3.546 min
Delta R.T.: 0.000 min
Response: 34024089
Conc: 10.93 ng/ml

Instrument :
ECD_D
ClientSampleId :
C-LAW-25-0156-0166-COMP

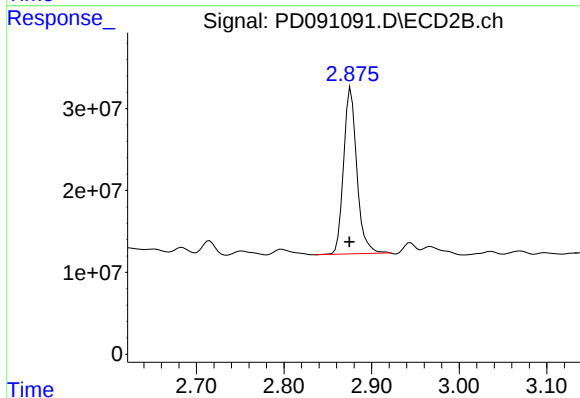


#1 Tetrachloro-m-xylene

R.T.: 2.876 min
Delta R.T.: 0.002 min
Response: 209724088
Conc: 7.04 ng/ml

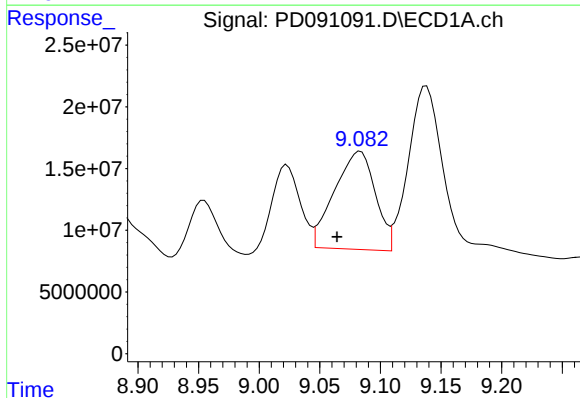

#28 Decachlorobiphenyl

R.T.: 9.083 min
Delta R.T.: 0.019 min
Response: 186434562
Conc: 39.85 ng/ml

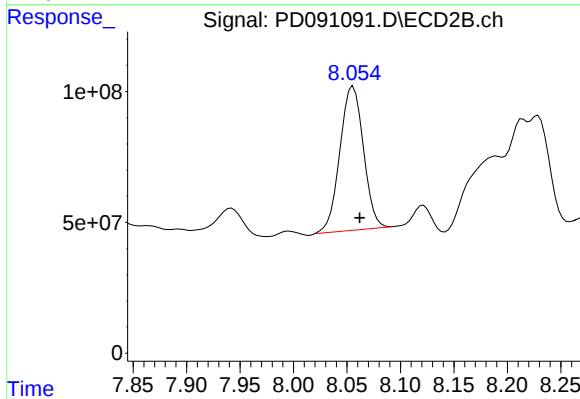

#28 Decachlorobiphenyl

R.T.: 8.056 min
Delta R.T.: -0.006 min
Response: 842473760
Conc: 27.81 ng/ml