

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111225\
 Data File : PD091126.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Nov 2025 19:45
 Operator : AR\AJ
 Sample : Q3590-01 10X
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MOO-25-0314-0316-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 21:33:26 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101725.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 17 17:43:28 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.544	2.874	3394631	29961834	1.090	1.006
28) SA Decachlor...	9.066	8.059	5833464	45381316	1.247	1.498

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111225\
Data File : PD091126.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Nov 2025 19:45
Operator : AR\AJ
Sample : Q3590-01 10X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
MOO-25-0314-0316-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 21:33:26 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101725.M
Quant Title : GC Extractables
QLast Update : Fri Oct 17 17:43:28 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

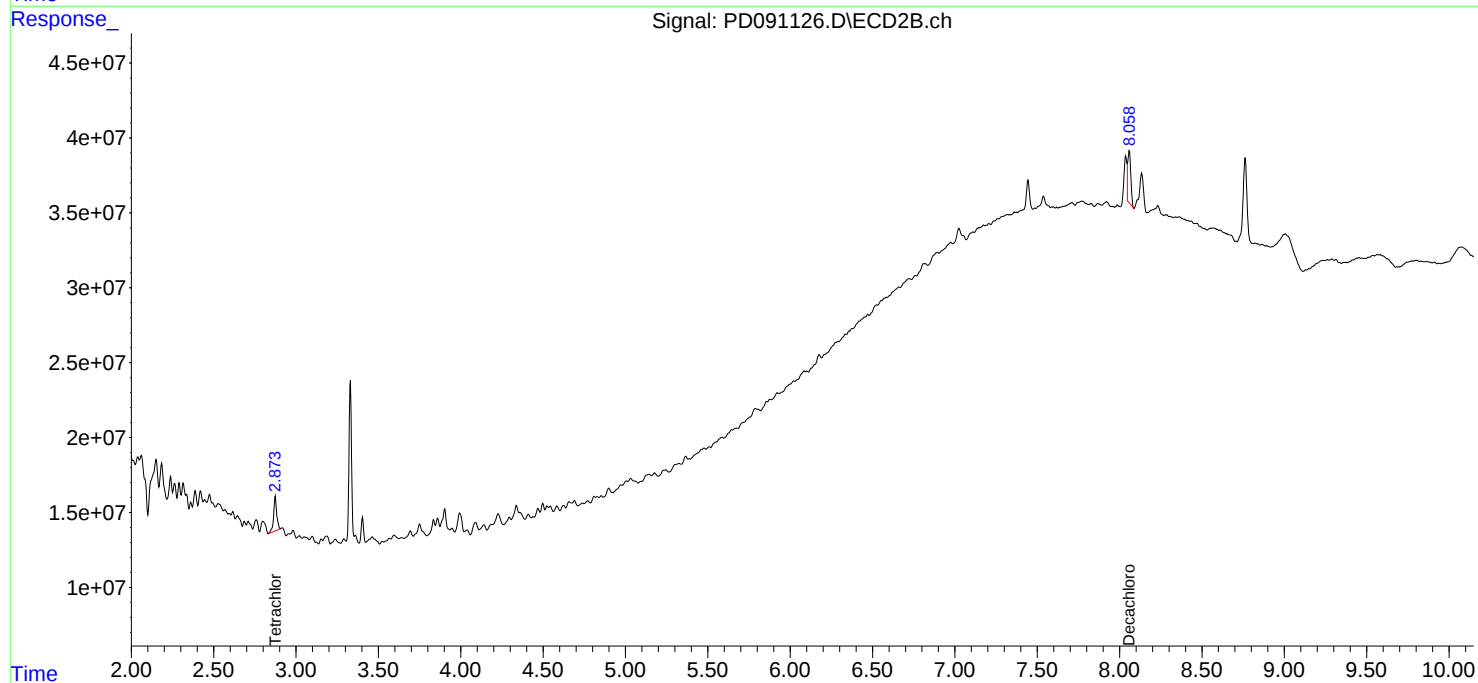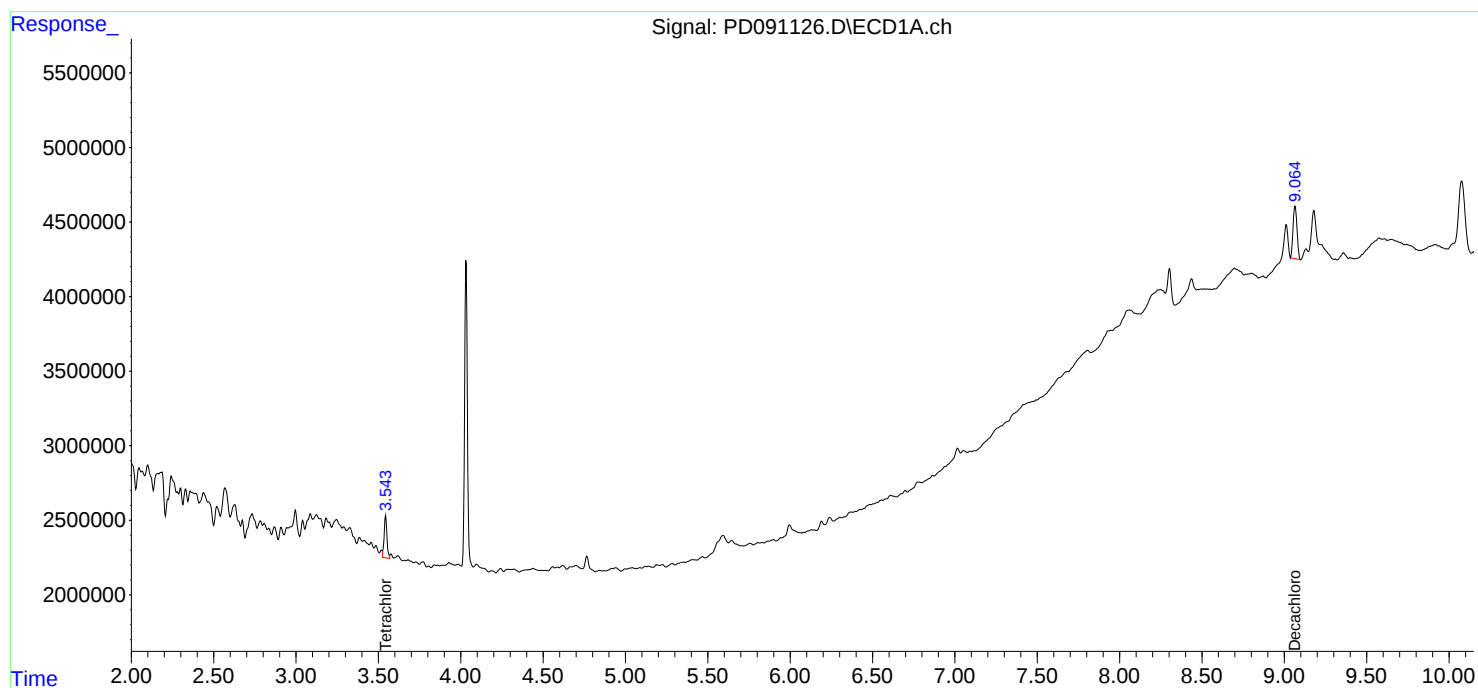


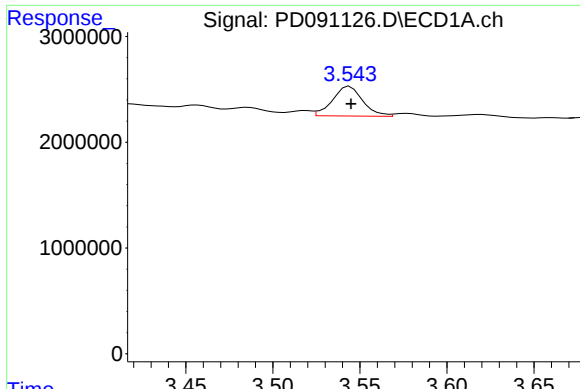

#1 Tetrachloro-m-xylene


R.T.: 3.544 min
Delta R.T.: 0.000 min
Response: 3394631
Conc: 1.09 ng/ml

Instrument :
ECD_D
ClientSampleId :
MOO-25-0314-0316-COMP

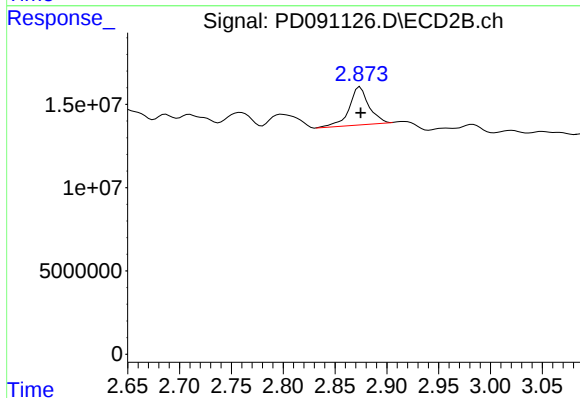


#1 Tetrachloro-m-xylene

R.T.: 2.874 min
Delta R.T.: 0.000 min
Response: 29961834
Conc: 1.01 ng/ml

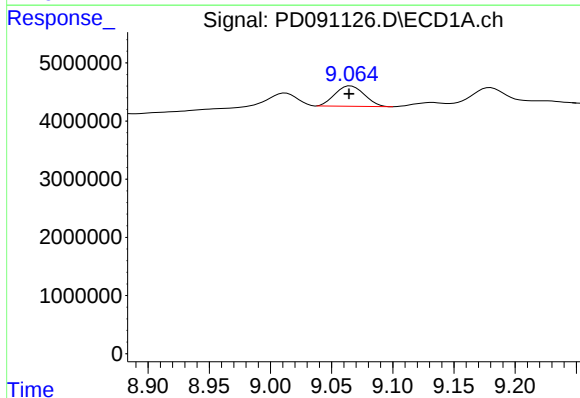

#28 Decachlorobiphenyl

R.T.: 9.066 min
Delta R.T.: 0.002 min
Response: 5833464
Conc: 1.25 ng/ml

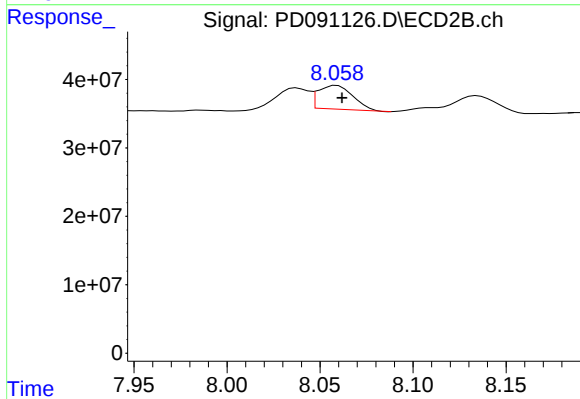

#28 Decachlorobiphenyl

R.T.: 8.059 min
Delta R.T.: -0.003 min
Response: 45381316
Conc: 1.50 ng/ml