

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111225\
 Data File : PD091127.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Nov 2025 19:59
 Operator : AR\AJ
 Sample : Q3590-03 10X
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MOO-25-0317-0318-COMP

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 11/13/2025
 Supervised By :Sohil Jodhani 11/14/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 21:34:00 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101725.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 17 17:43:28 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.544	2.873	3246554	39025572	1.043	1.311m#
2) SA Decachlor...	9.067	8.060	6779663	36320503	1.449	1.199

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111225\
Data File : PD091127.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Nov 2025 19:59
Operator : AR\AJ
Sample : Q3590-03 10X
Misc :
ALS Vial : 59 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
MOO-25-0317-0318-COMP


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/13/2025
Supervised By :Sohil Jodhani 11/14/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 21:34:00 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101725.M
Quant Title : GC Extractables
QLast Update : Fri Oct 17 17:43:28 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

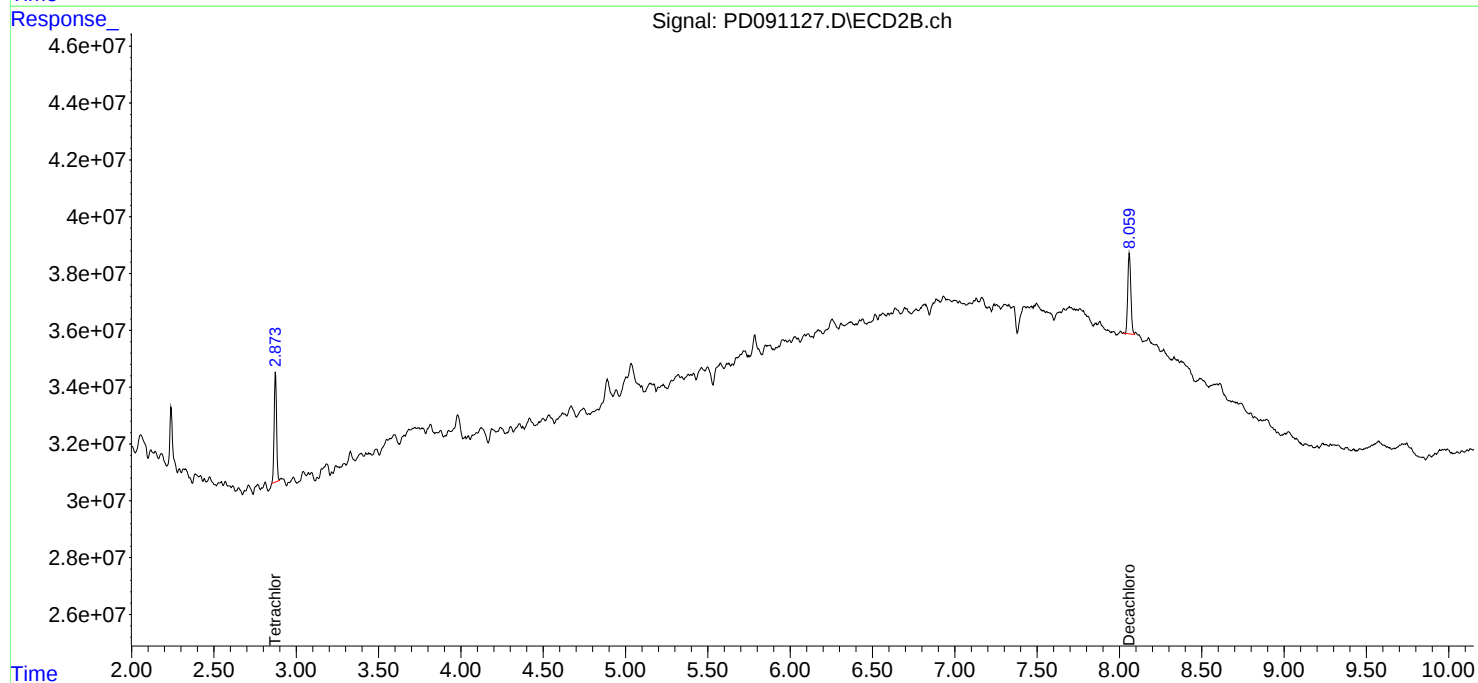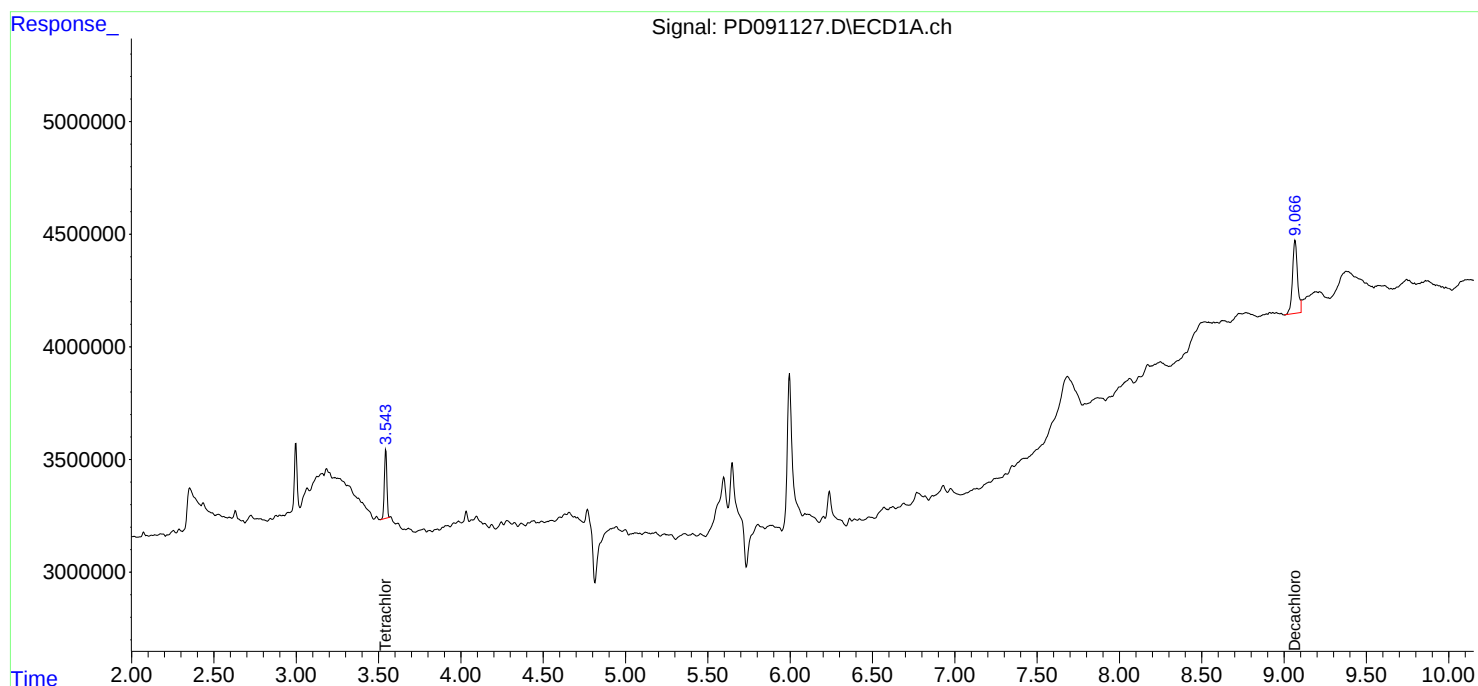

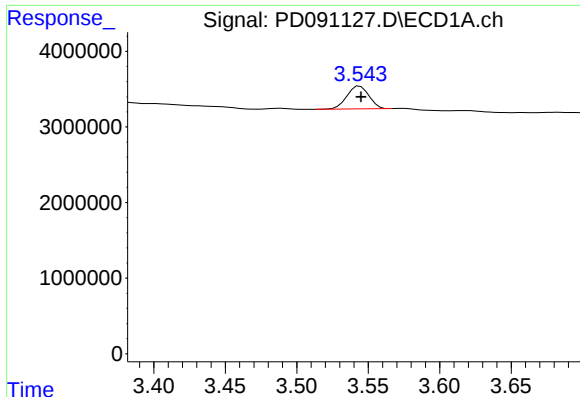


#1 Tetrachloro-m-xylene

R.T.: 3.544 min
Delta R.T.: 0.000 min
Response: 3246554
Conc: 1.04 ng/ml

Instrument :
ECD_D
ClientSampleId :
MOO-25-0317-0318-COMP


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/13/2025
Supervised By :Sohil Jodhani 11/14/2025

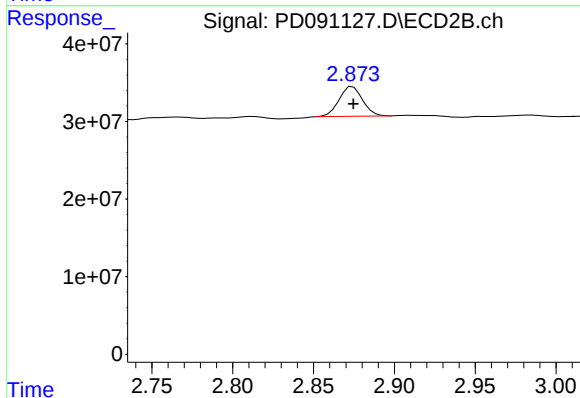


#1 Tetrachloro-m-xylene

R.T.: 2.873 min
Delta R.T.: -0.002 min
Response: 39025572
Conc: 1.31 ng/ml m

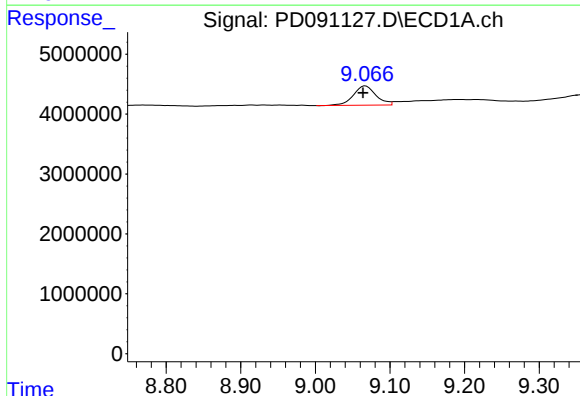

#28 Decachlorobiphenyl

R.T.: 9.067 min
Delta R.T.: 0.003 min
Response: 6779663
Conc: 1.45 ng/ml

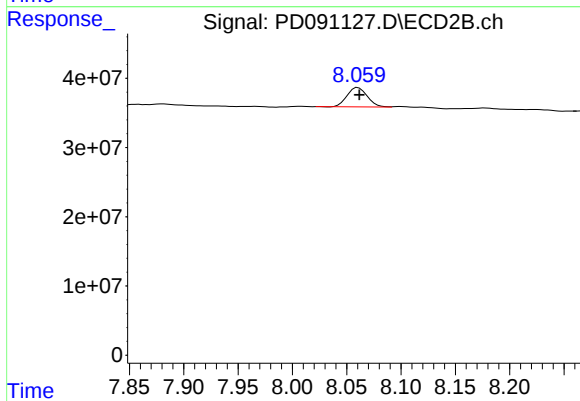

#28 Decachlorobiphenyl

R.T.: 8.060 min
Delta R.T.: -0.001 min
Response: 36320503
Conc: 1.20 ng/ml