

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111225\
 Data File : PD091128.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Nov 2025 20:12
 Operator : AR\AJ
 Sample : Q3590-05 10X
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MOO-25-0319

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 11/13/2025
 Supervised By :Sohil Jodhani 11/14/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 21:34:32 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101725.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 17 17:43:28 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.545	2.874	2703976	18876716	0.868	0.634m#
2) SA Decachlor...	9.065	8.060	8147385	45365091	1.742	1.498

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111225\
Data File : PD091128.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Nov 2025 20:12
Operator : AR\AJ
Sample : Q3590-05 10X
Misc :
ALS Vial : 60 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
MOO-25-0319


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/13/2025
Supervised By :Sohil Jodhani 11/14/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 21:34:32 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101725.M
Quant Title : GC Extractables
QLast Update : Fri Oct 17 17:43:28 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

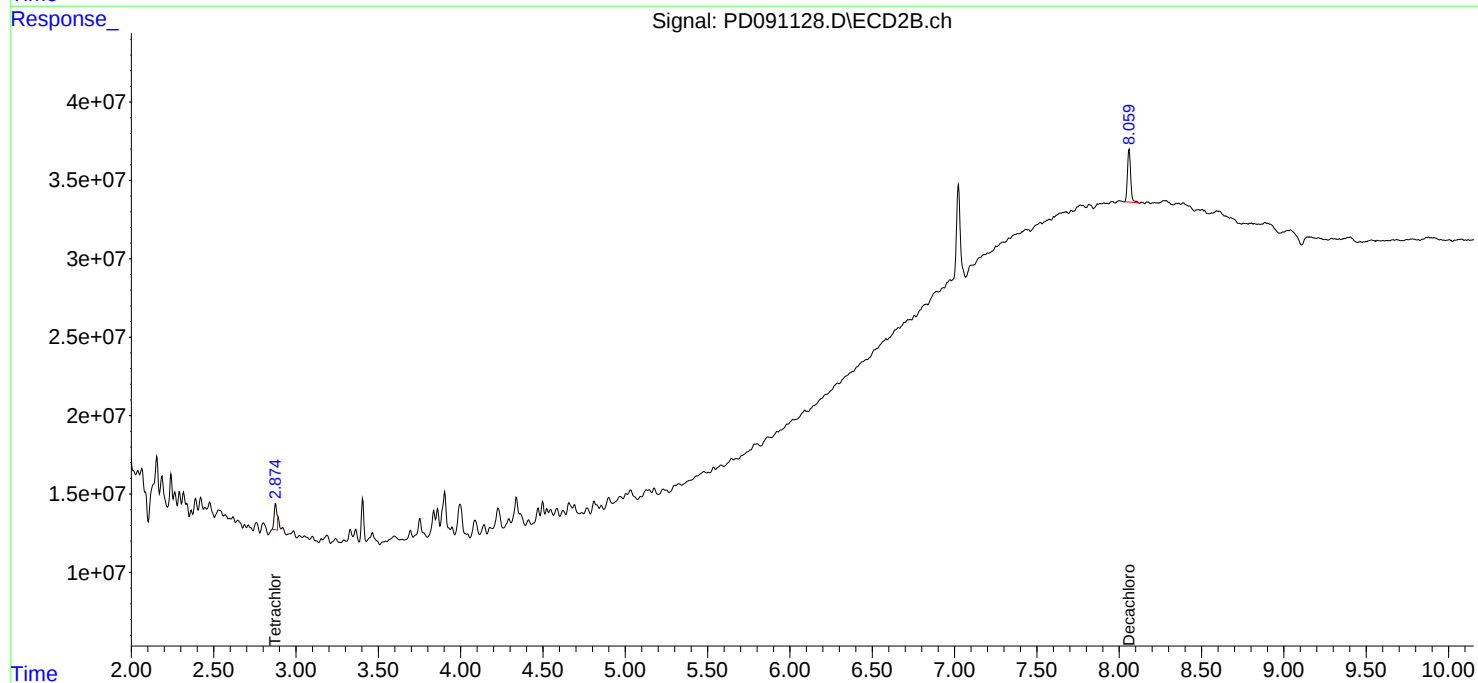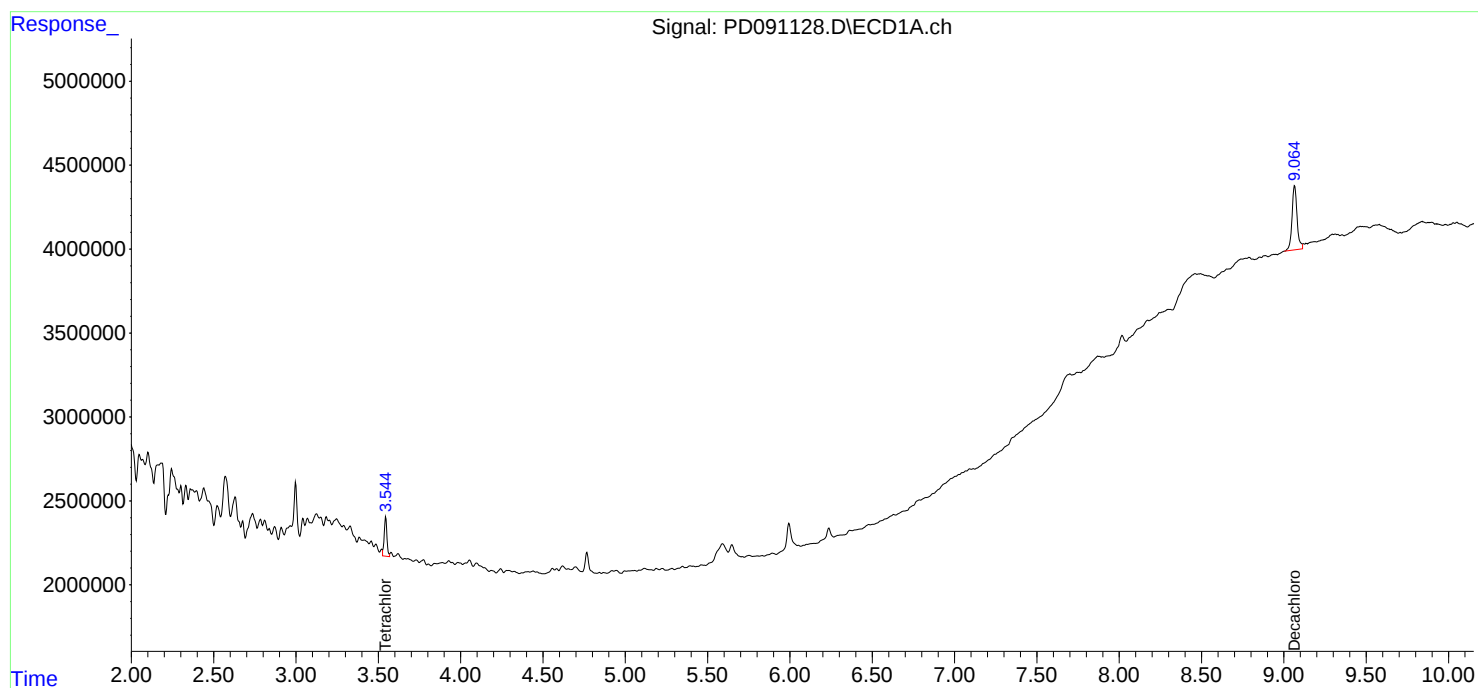

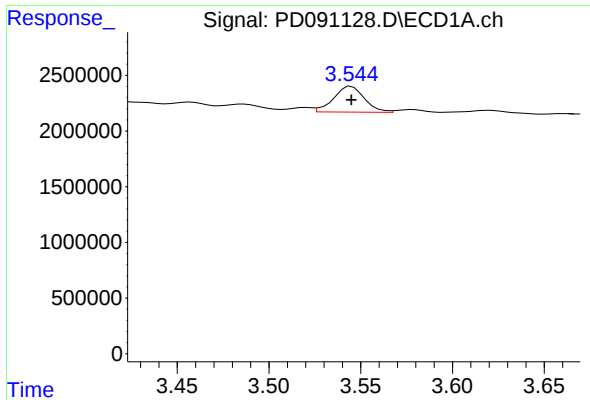

#1 Tetrachloro-m-xylene

R.T.: 3.545 min
Delta R.T.: 0.000 min
Response: 2703976
Conc: 0.87 ng/ml

Instrument :

ECD_D


ClientSampleId :

MOO-25-0319

Manual Integrations


APPROVED

Reviewed By :Rahul Chavli 11/13/2025
Supervised By :Sohil Jodhani 11/14/2025

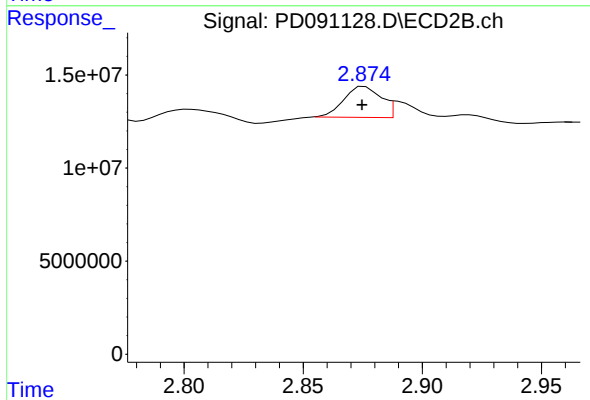


#1 Tetrachloro-m-xylene

R.T.: 2.874 min
Delta R.T.: 0.000 min
Response: 18876716
Conc: 0.63 ng/ml m

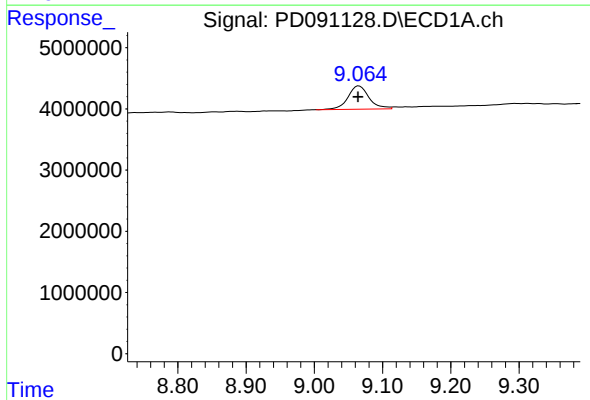

#28 Decachlorobiphenyl

R.T.: 9.065 min
Delta R.T.: 0.001 min
Response: 8147385
Conc: 1.74 ng/ml

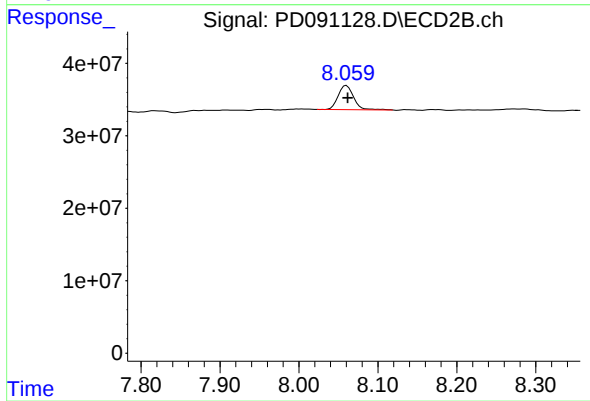

#28 Decachlorobiphenyl

R.T.: 8.060 min
Delta R.T.: -0.002 min
Response: 45365091
Conc: 1.50 ng/ml