

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111319\
 Data File : PD055918.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Nov 2019 11:14
 Operator : SG\AJ
 Sample : K5772-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AP1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 00:40:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 02 07:20:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.289	3.962	9659688	12867764	12.832	12.279
27)	SA Decachlor...	7.963	8.996	15899991	19863628	19.506	17.492
Target Compounds							
2)	A alpha-BHC	0.000	4.389f	0	109897	N.D.	<MDL
10)	B trans-Chl...	0.000	6.043	0	2293612	N.D.	1.608


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111319\
Data File : PD055918.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Nov 2019 11:14
Operator : SG\AJ
Sample : K5772-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
C0AP1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 00:40:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 02 07:20:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

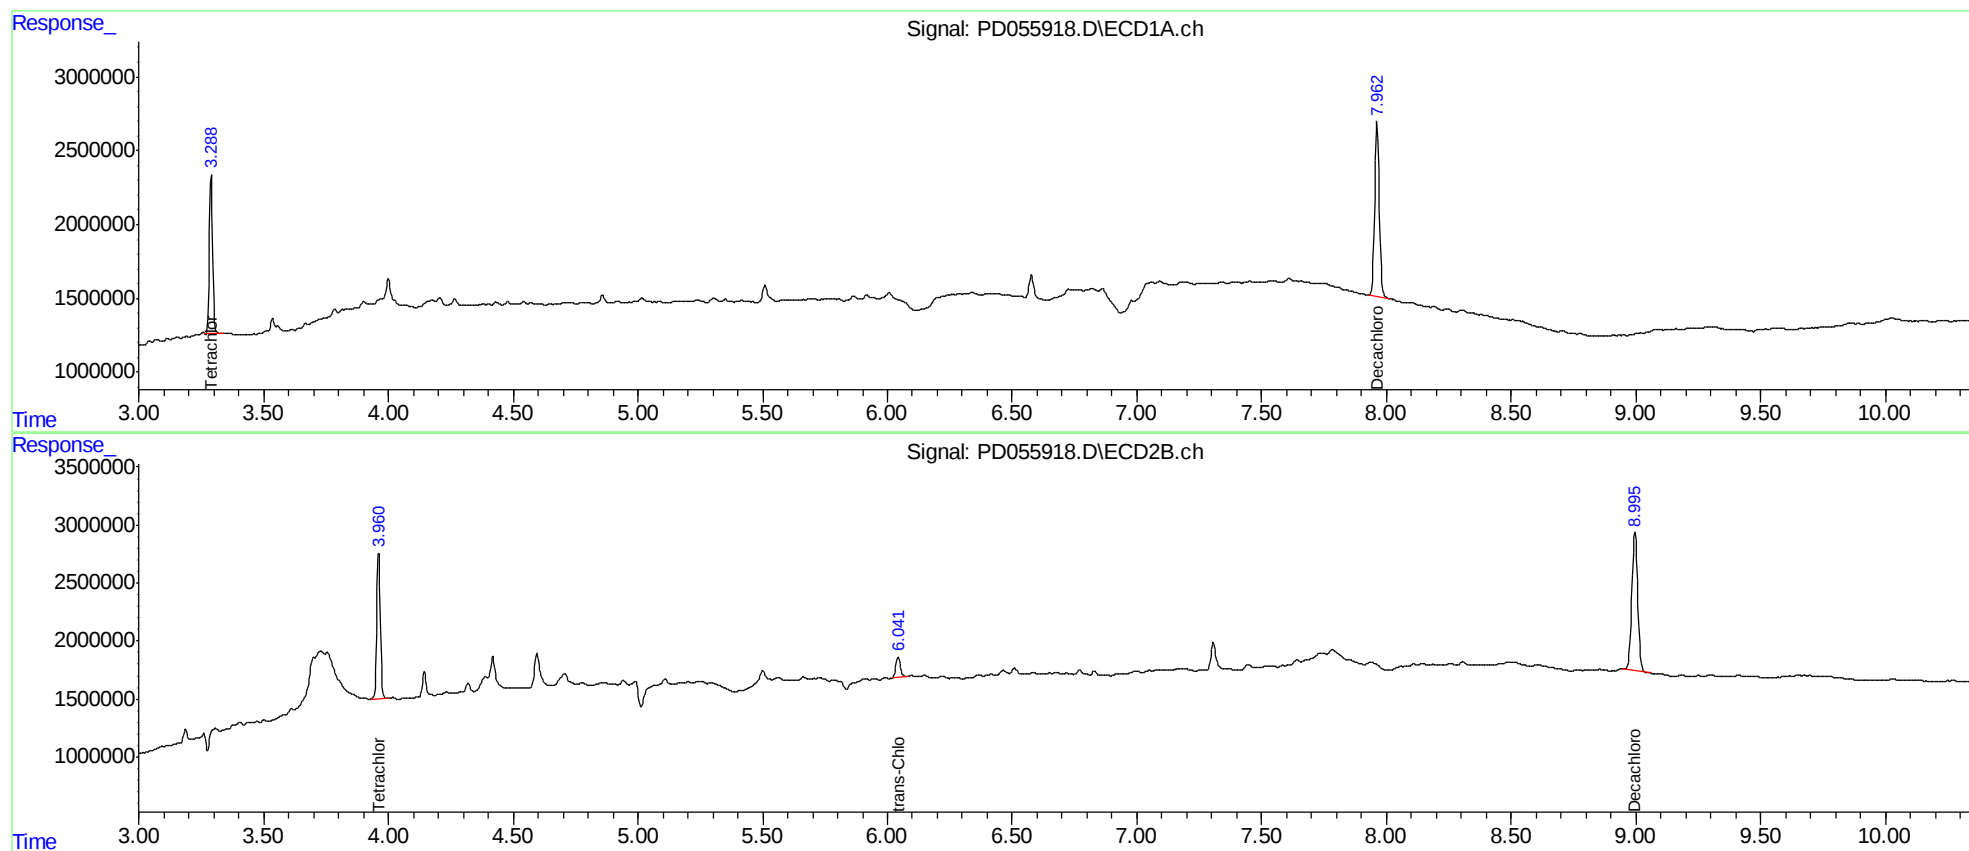


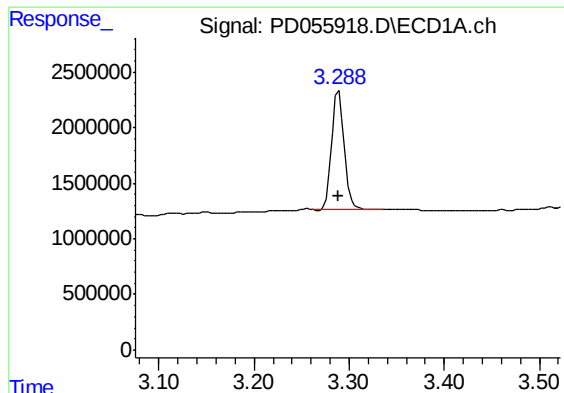

#1 Tetrachloro-m-xylene


R.T.: 3.289 min
Delta R.T.: 0.000 min
Response: 9659688
Conc: 12.83 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AP1

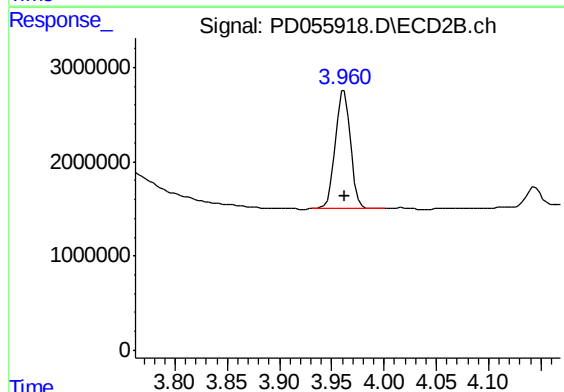


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: 0.000 min
Response: 12867764
Conc: 12.28 ng/ml

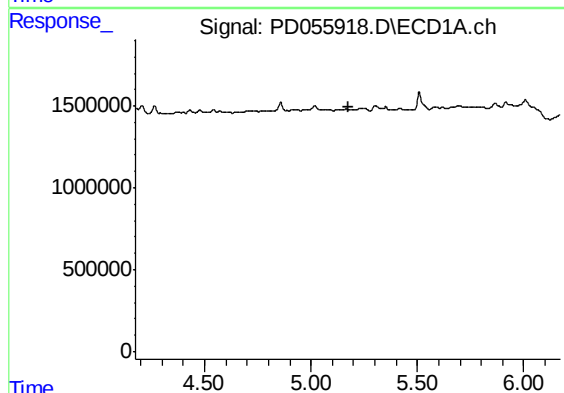


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.174 min
Response: 0
Conc: N.D.

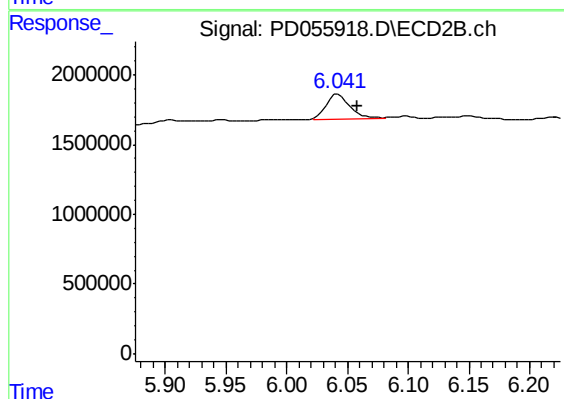

#10 trans-Chlordane


R.T.: 6.043 min
Delta R.T.: -0.015 min
Response: 2293612
Conc: 1.61 ng/ml

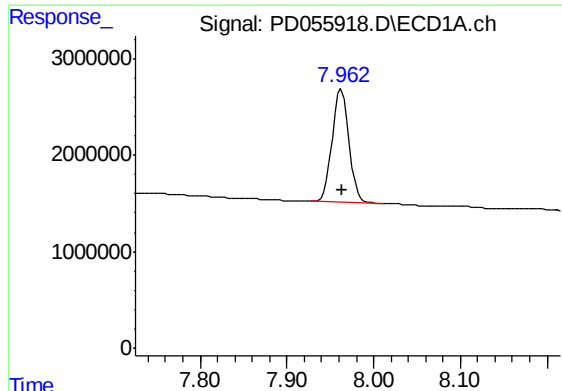

#27 Decachlorobiphenyl

R.T.: 7.963 min
Delta R.T.: 0.000 min
Response: 15899991
Conc: 19.51 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AP1

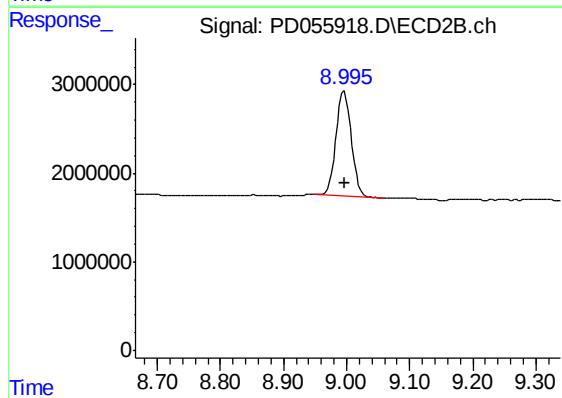

#27 Decachlorobiphenyl

R.T.: 8.996 min
Delta R.T.: 0.000 min
Response: 19863628
Conc: 17.49 ng/ml