

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111319\
 Data File : PD055928.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Nov 2019 13:34
 Operator : SG\AJ
 Sample : K5772-21
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AQ5

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 00:42:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 02 07:20:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.289	3.961	11890934	15677793	15.796	14.960
27) SA Decachlor...	7.962	8.996	19568775	25383818	24.007	22.354
Target Compounds						
15) B Endosulfa...	0.000	6.870	0	1986239	N.D.	1.534


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111319\
Data File : PD055928.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Nov 2019 13:34
Operator : SG\AJ
Sample : K5772-21
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
C0AQ5

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 00:42:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 02 07:20:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

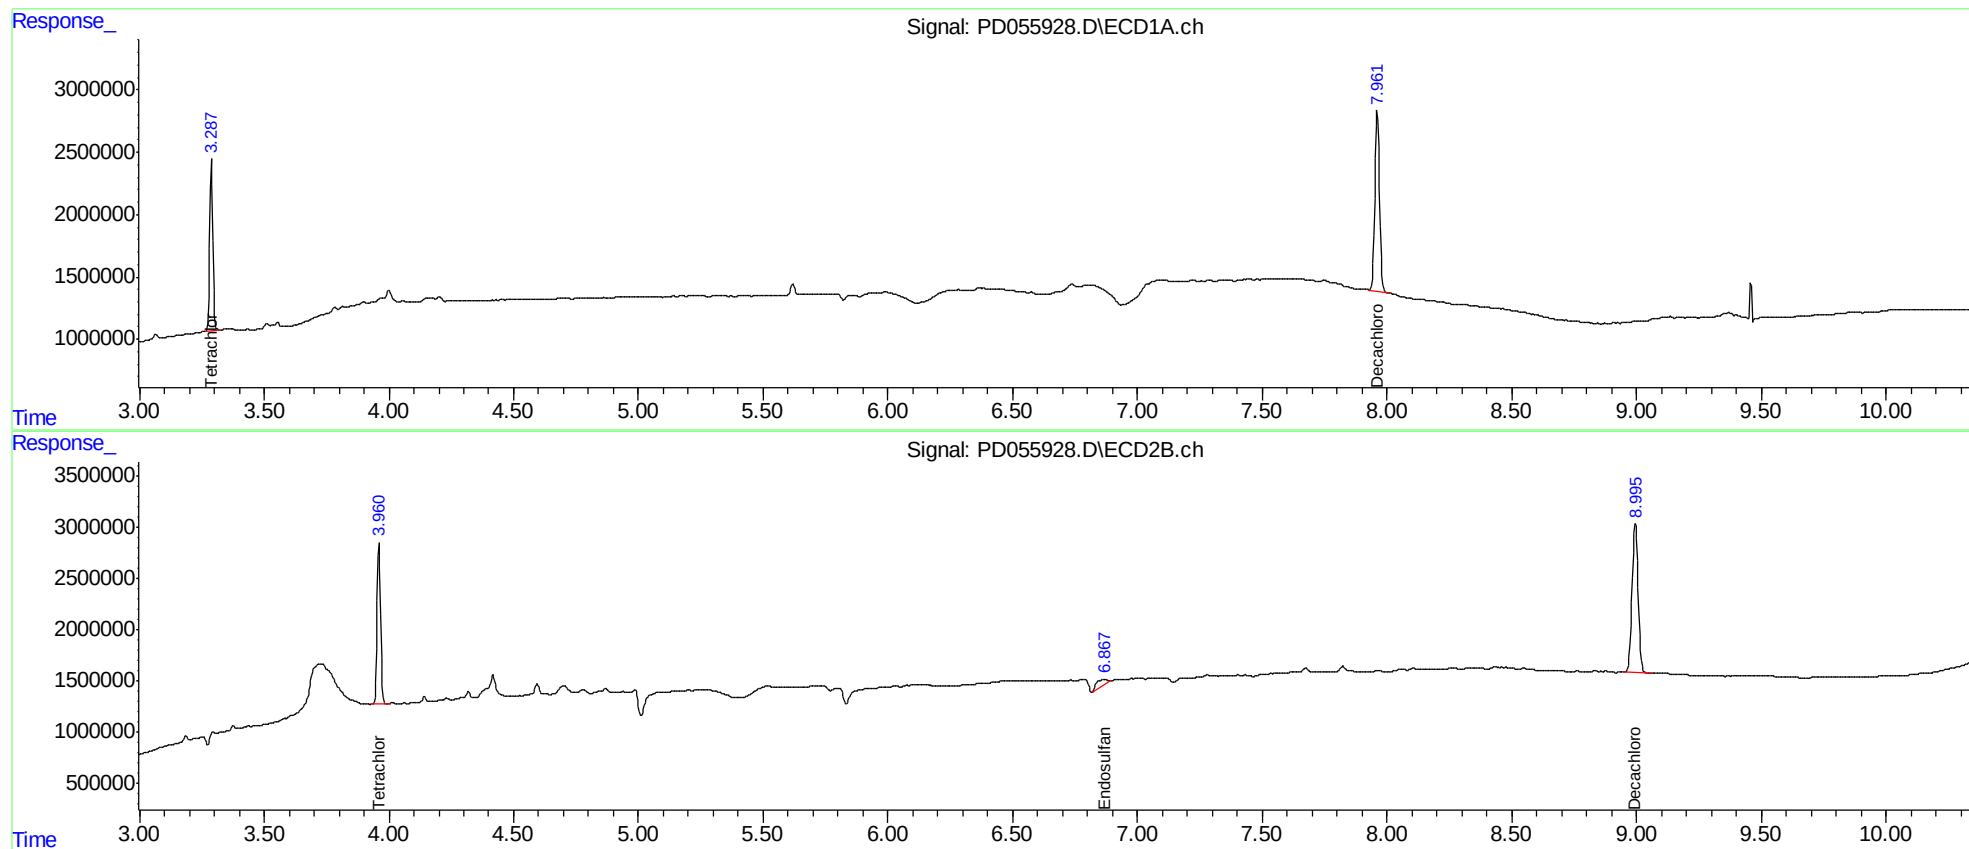


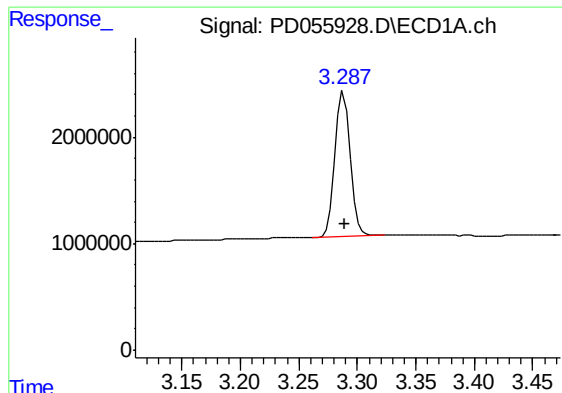

#1 Tetrachloro-m-xylene


R.T.: 3.289 min
Delta R.T.: 0.000 min
Response: 11890934
Conc: 15.80 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AQ5

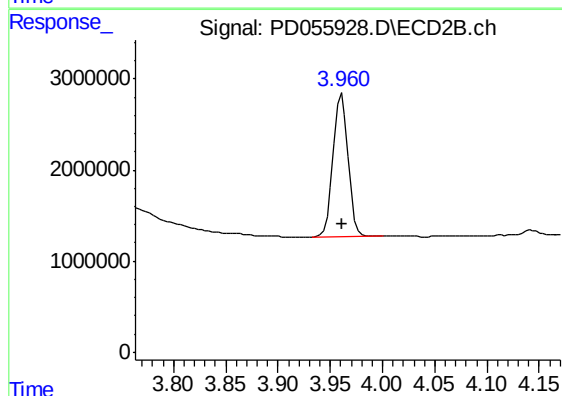


#1 Tetrachloro-m-xylene

R.T.: 3.961 min
Delta R.T.: 0.000 min
Response: 15677793
Conc: 14.96 ng/ml

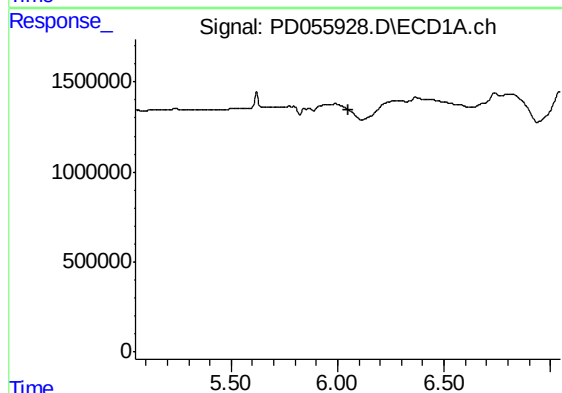


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.049 min
Response: 0
Conc: N.D.

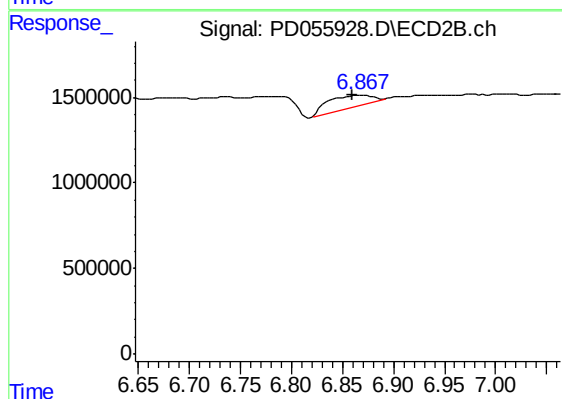

#15 Endosulfan II


R.T.: 6.870 min
Delta R.T.: 0.009 min
Response: 1986239
Conc: 1.53 ng/ml

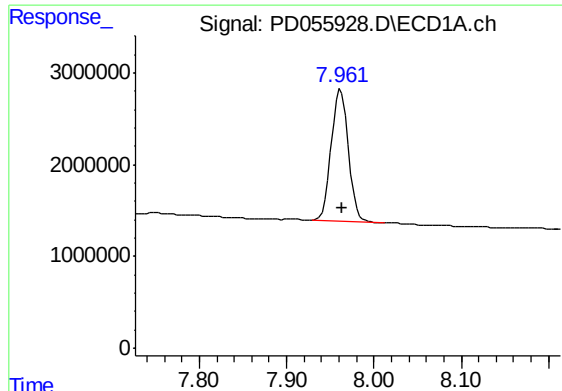

#27 Decachlorobiphenyl

R.T.: 7.962 min
Delta R.T.: 0.000 min
Response: 19568775
Conc: 24.01 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AQ5

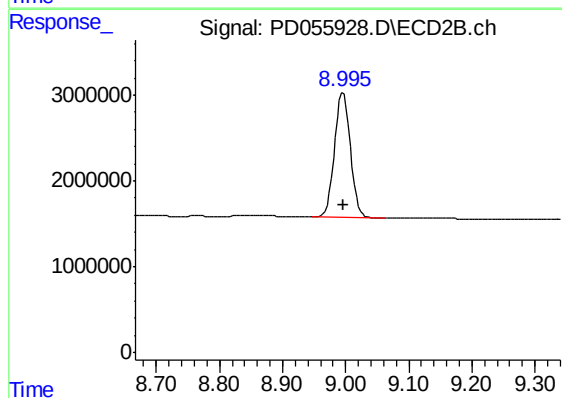

#27 Decachlorobiphenyl

R.T.: 8.996 min
Delta R.T.: 0.000 min
Response: 25383818
Conc: 22.35 ng/ml