

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111319\
 Data File : PD055929.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Nov 2019 13:48
 Operator : SG\AJ
 Sample : K5772-22
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AQ6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 00:43:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 02 07:20:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.289	3.962	12148780	16128370	16.139	15.390
27)	SA Decachlor...	7.963	8.996	18665517	23785932	22.899	20.946
Target Compounds							
4)	MA Heptachlor	0.000	5.158	0	1248783	N.D.	0.859
9)	A Endosulfan I	5.297	0.000	4099452	0	4.892	N.D. #
10)	B trans-Chl...	0.000	6.044	0	6350668	N.D.	4.452
11)	B cis-Chlor...	5.297f	0.000	4099452	0	4.630	N.D. #
15)	B Endosulfa...	0.000	6.876	0	1681648	N.D.	1.299


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111319\
Data File : PD055929.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Nov 2019 13:48
Operator : SG\AJ
Sample : K5772-22
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
C0AQ6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 00:43:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 02 07:20:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

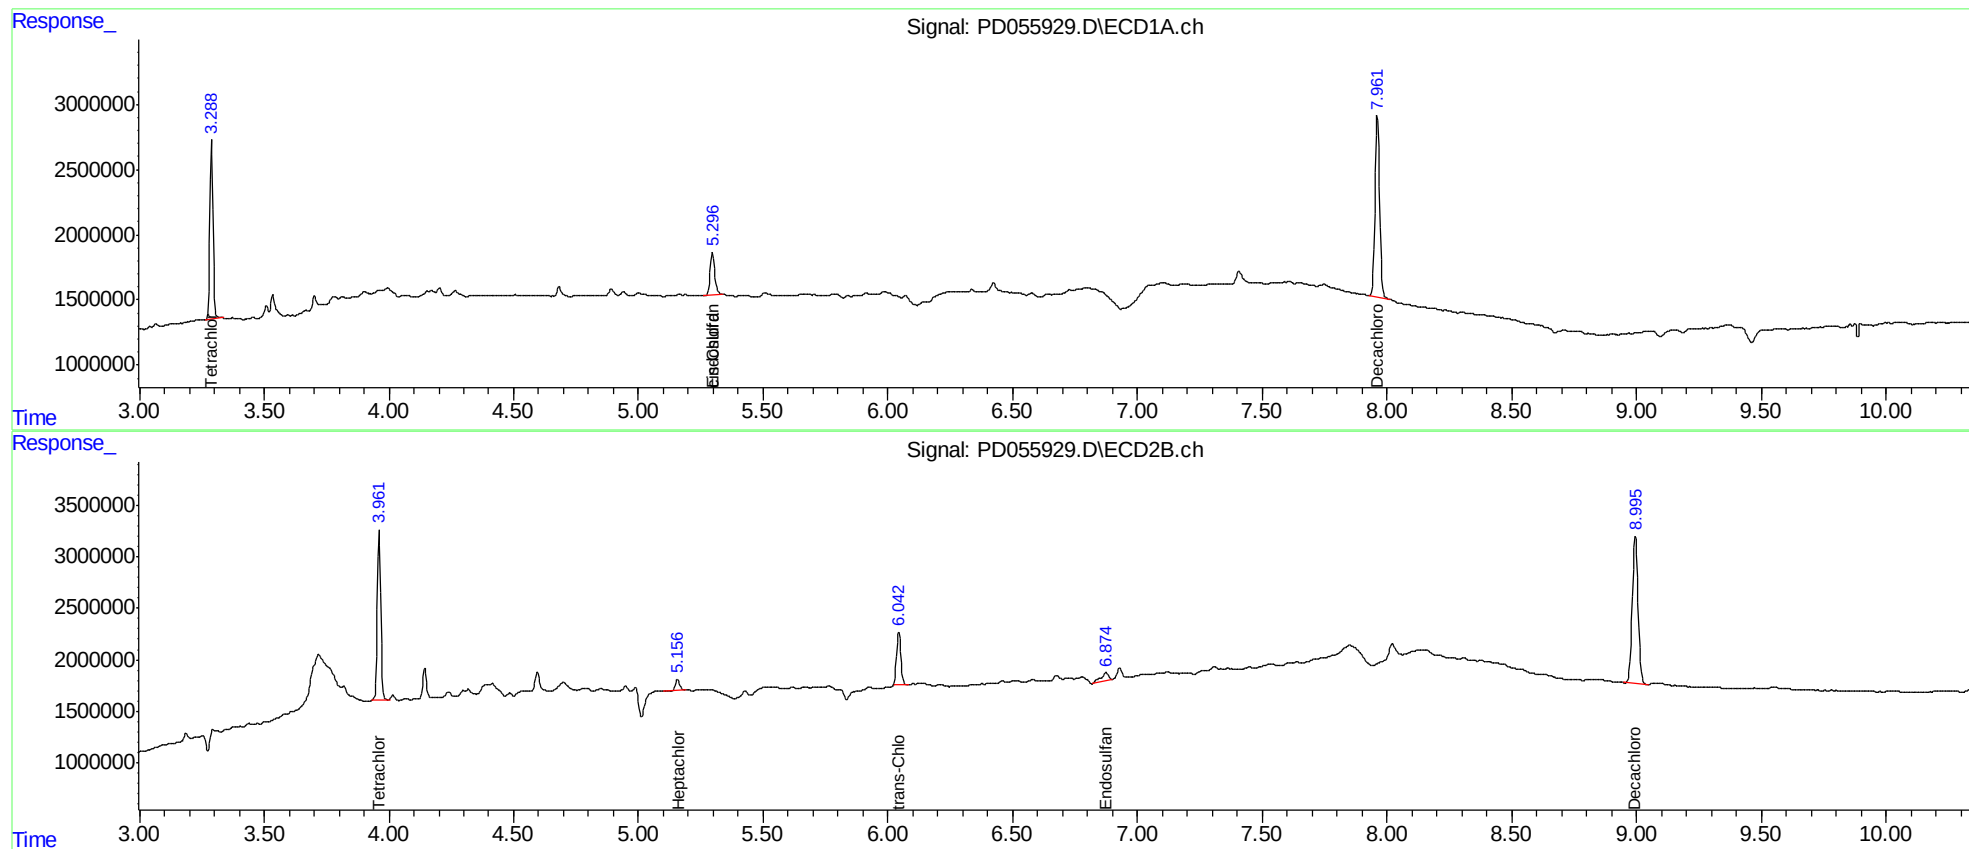


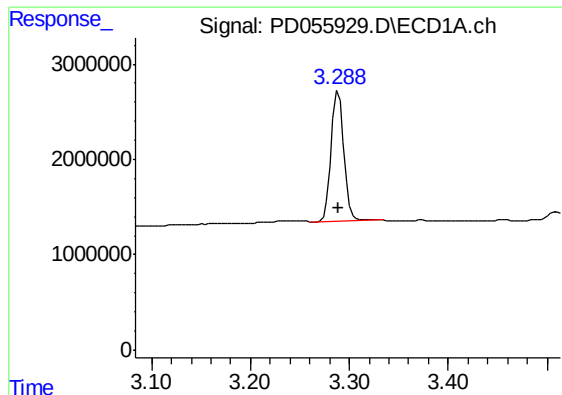

#1 Tetrachloro-m-xylene


R.T.: 3.289 min
Delta R.T.: 0.000 min
Response: 12148780
Conc: 16.14 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AQ6

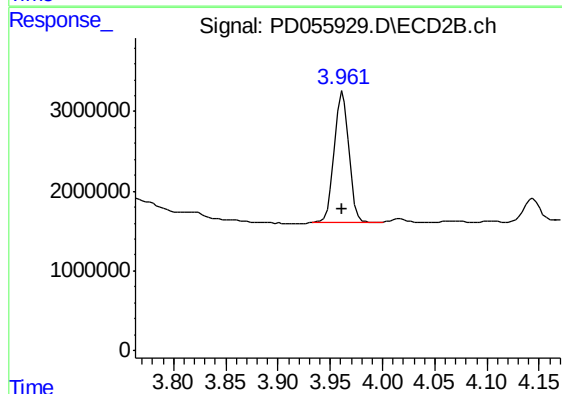


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: 0.000 min
Response: 16128370
Conc: 15.39 ng/ml

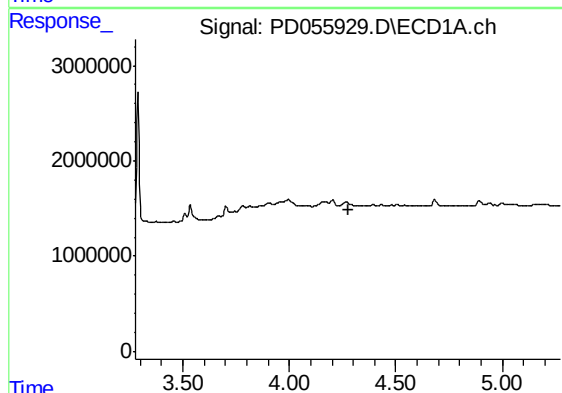


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.277 min
Response: 0
Conc: N.D.

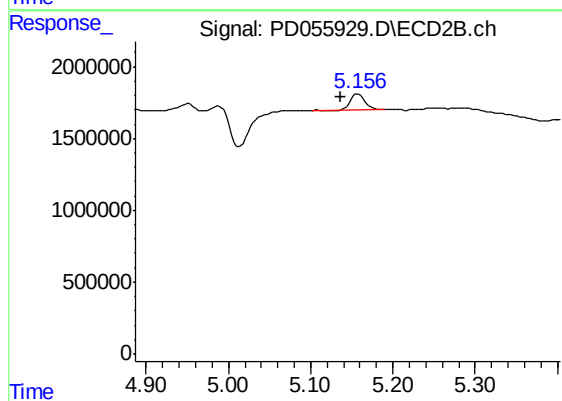

#4 Heptachlor


R.T.: 5.158 min
Delta R.T.: 0.021 min
Response: 1248783
Conc: 0.86 ng/ml

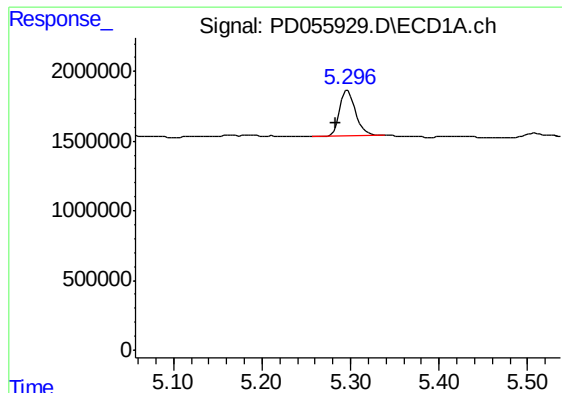

#9 Endosulfan I


R.T.: 5.297 min
Delta R.T.: 0.014 min
Response: 4099452
Conc: 4.89 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AQ6

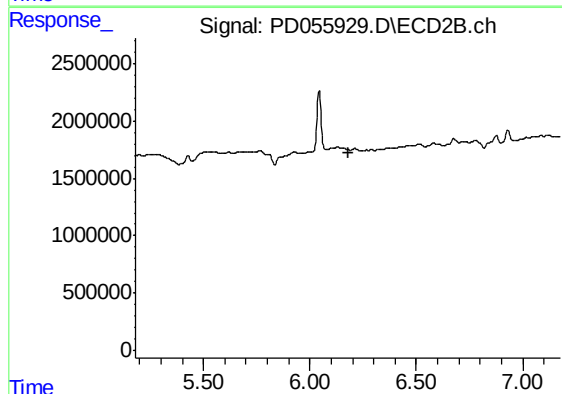


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.180 min
Response: 0
Conc: N.D.

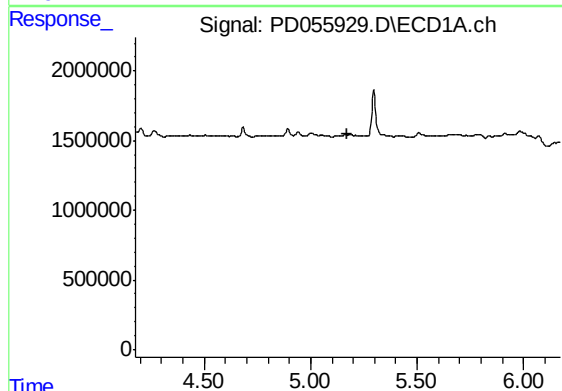


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.174 min
Response: 0
Conc: N.D.

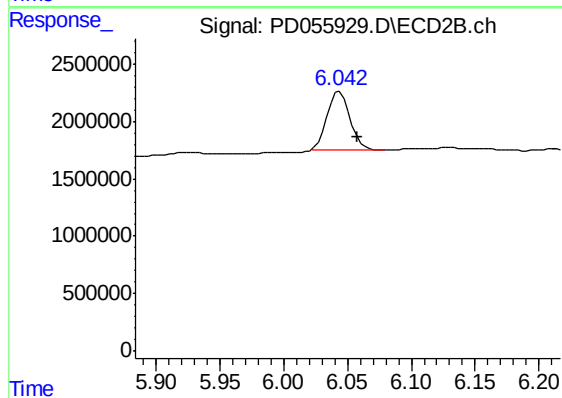

#10 trans-Chlordane


R.T.: 6.044 min
Delta R.T.: -0.014 min
Response: 6350668
Conc: 4.45 ng/ml

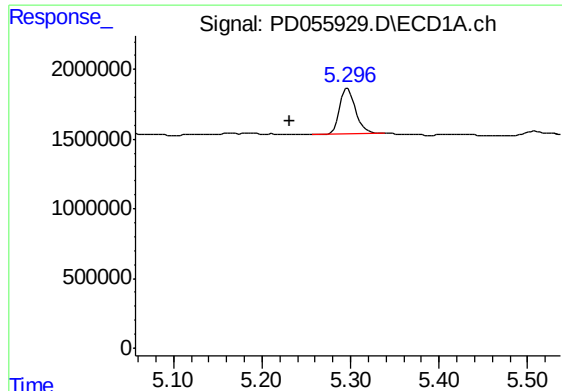

#11 cis-Chlordane


R.T.: 5.297 min
Delta R.T.: 0.066 min
Response: 4099452
Conc: 4.63 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AQ6

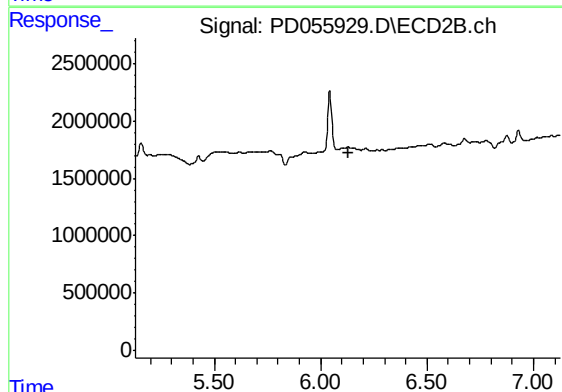


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.130 min
Response: 0
Conc: N.D.

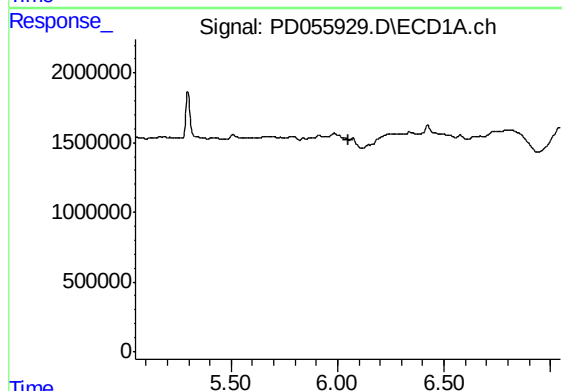


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.049 min
Response: 0
Conc: N.D.

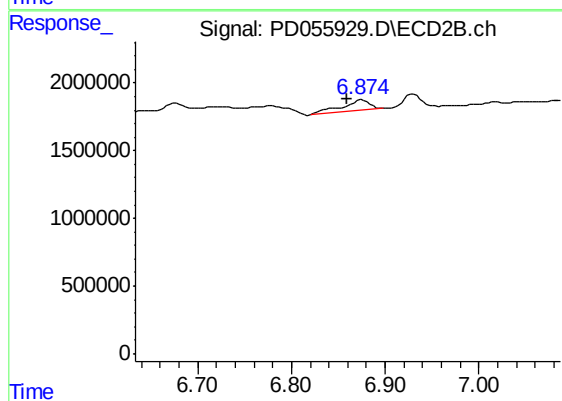

#15 Endosulfan II


R.T.: 6.876 min
Delta R.T.: 0.015 min
Response: 1681648
Conc: 1.30 ng/ml

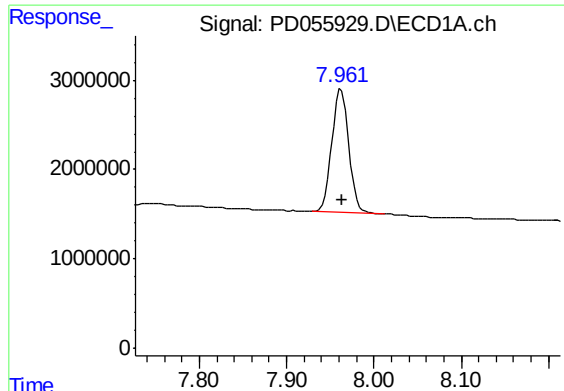

#27 Decachlorobiphenyl

R.T.: 7.963 min
Delta R.T.: 0.000 min
Response: 18665517
Conc: 22.90 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AQ6

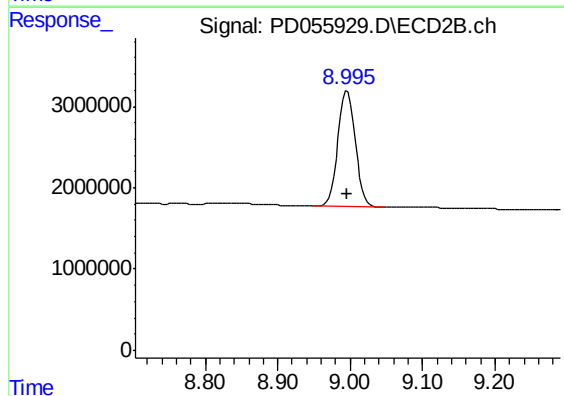

#27 Decachlorobiphenyl

R.T.: 8.996 min
Delta R.T.: 0.000 min
Response: 23785932
Conc: 20.95 ng/ml