

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111319\
 Data File : PD055935.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Nov 2019 15:19
 Operator : SG\AJ
 Sample : K5774-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AQ7

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 00:44:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 02 07:20:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.292	3.961	13045408	17430492	17.330	16.633
27)	SA Decachlor...	7.967	8.998	24124062	31792388	29.596	27.997
Target Compounds							
10)	B trans-Chl...	0.000	5.988f	0	5917066	N.D.	4.148
15)	B Endosulfa...	0.000	6.871	0	2627904	N.D.	2.029


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111319\
Data File : PD055935.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Nov 2019 15:19
Operator : SG\AJ
Sample : K5774-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
C0AQ7

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 00:44:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 02 07:20:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

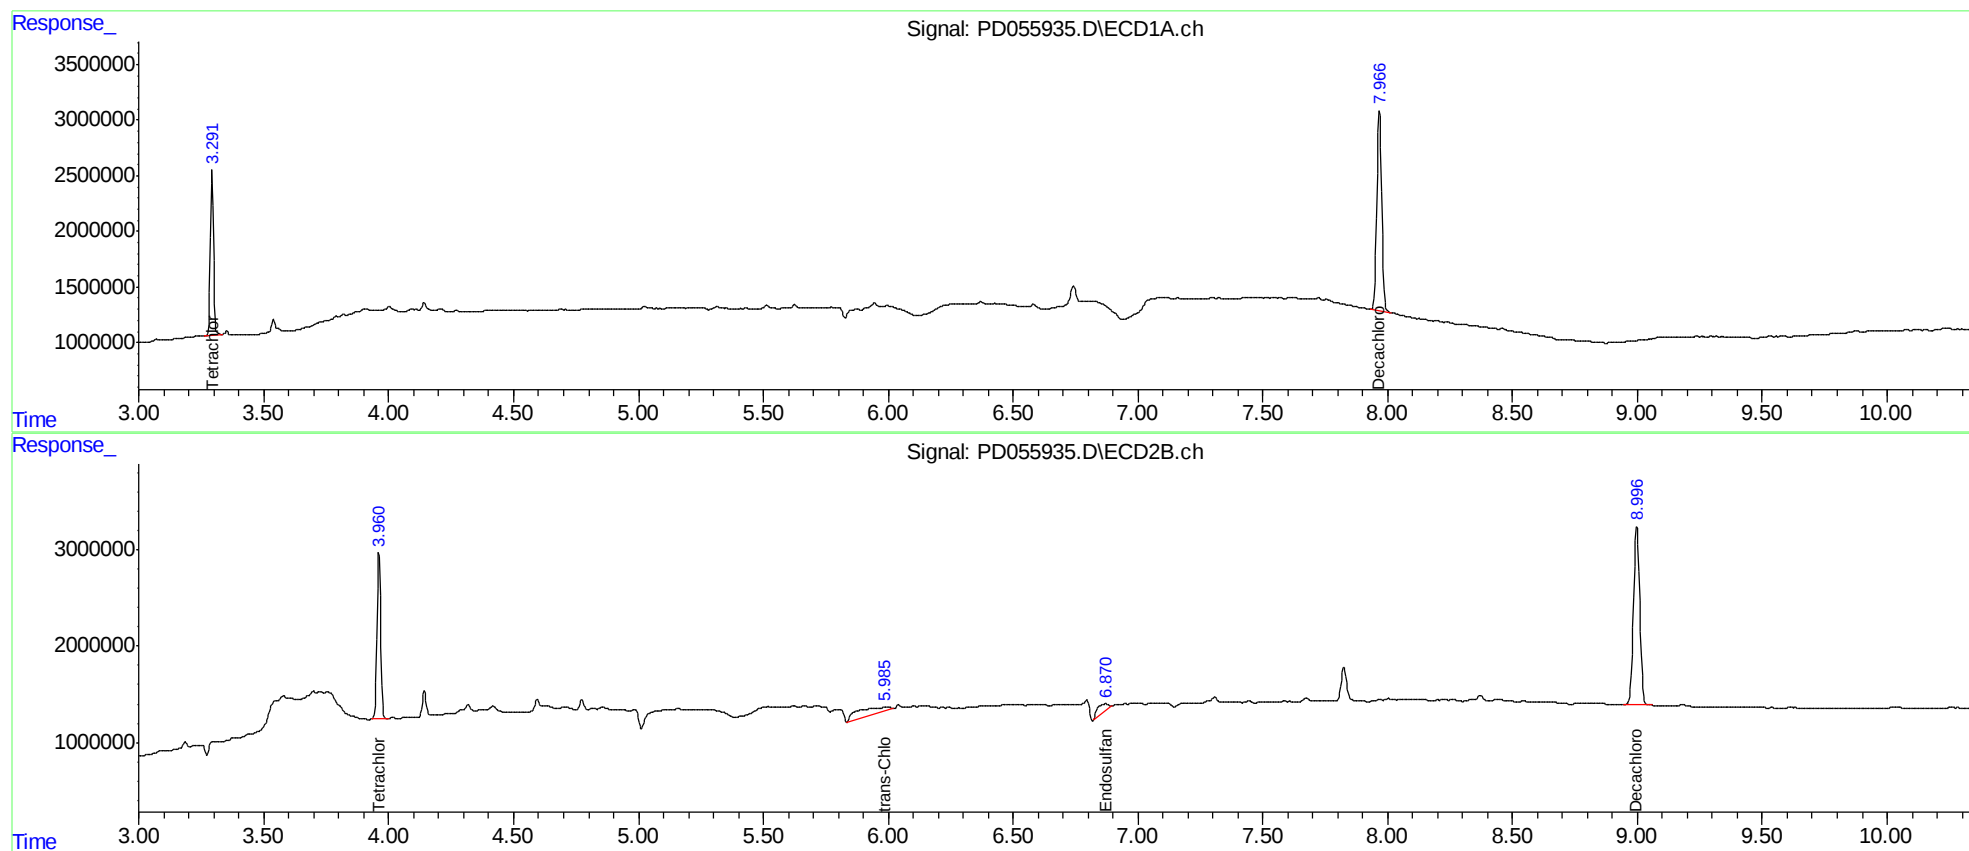


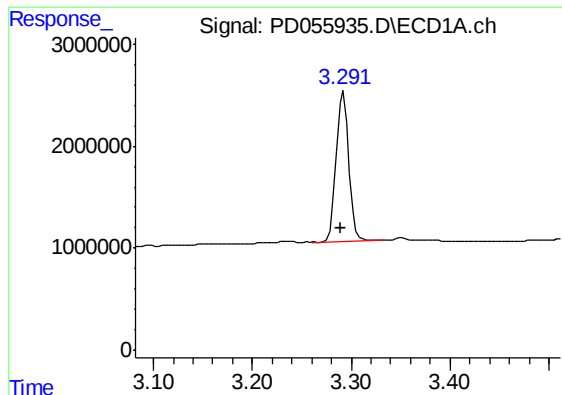

#1 Tetrachloro-m-xylene


R.T.: 3.292 min
Delta R.T.: 0.003 min
Response: 13045408
Conc: 17.33 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AQ7

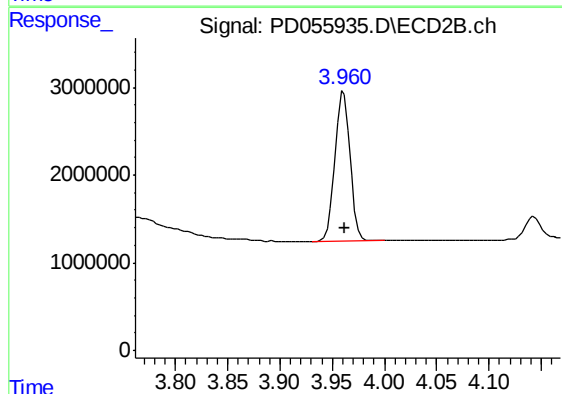


#1 Tetrachloro-m-xylene

R.T.: 3.961 min
Delta R.T.: 0.000 min
Response: 17430492
Conc: 16.63 ng/ml

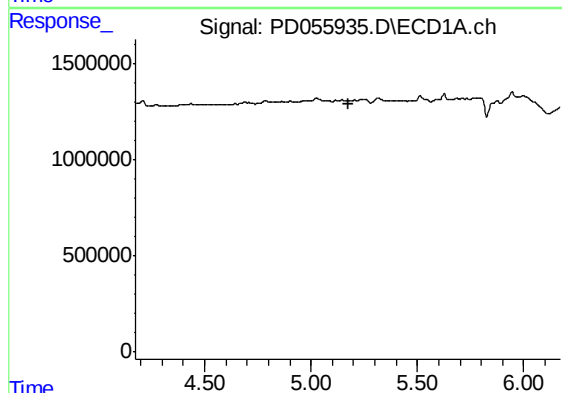


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.174 min
Response: 0
Conc: N.D.

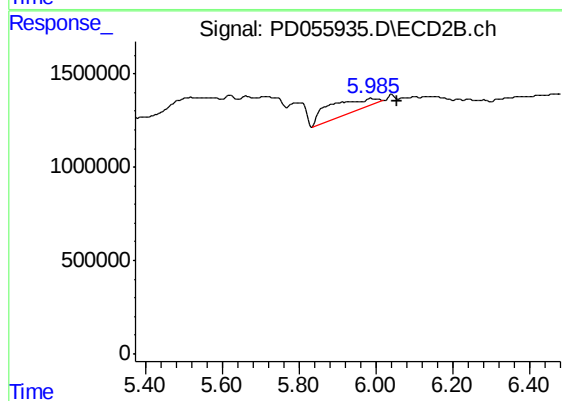

#10 trans-Chlordane


R.T.: 5.988 min
Delta R.T.: -0.070 min
Response: 5917066
Conc: 4.15 ng/ml

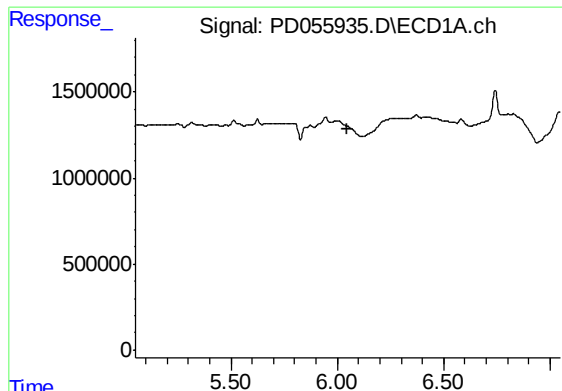

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.049 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C0AQ7

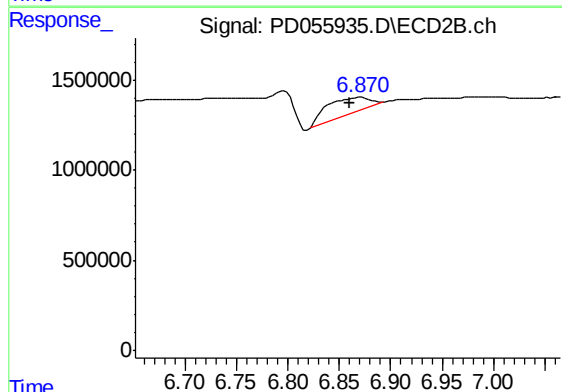


#15 Endosulfan II

R.T.: 6.871 min
Delta R.T.: 0.011 min
Response: 2627904
Conc: 2.03 ng/ml

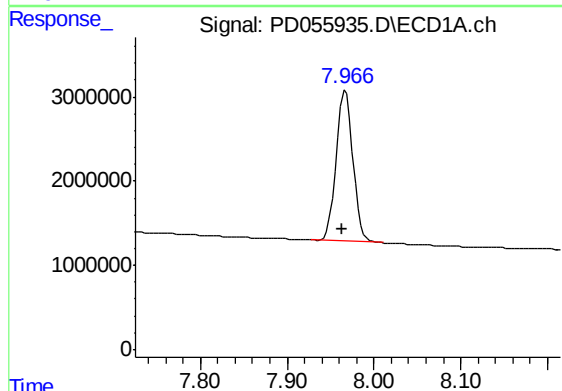

#27 Decachlorobiphenyl

R.T.: 7.967 min
Delta R.T.: 0.004 min
Response: 24124062
Conc: 29.60 ng/ml

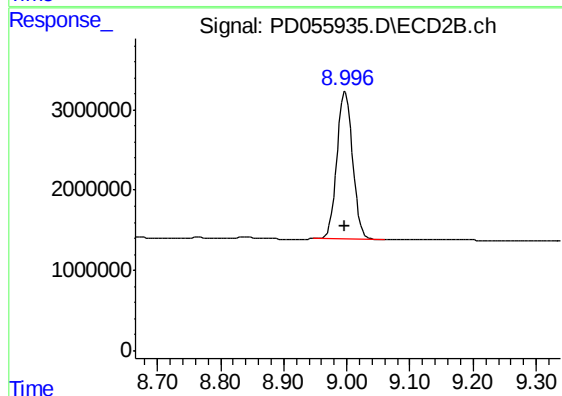

#27 Decachlorobiphenyl

R.T.: 8.998 min
Delta R.T.: 0.001 min
Response: 31792388
Conc: 28.00 ng/ml