

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111319\
 Data File : PD055936.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Nov 2019 15:33
 Operator : SG\AJ
 Sample : K5774-02
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AQ8

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 00:44:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 02 07:20:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.289	3.962	12717657	16981719	16.894	16.205
27)	SA Decachlor...	7.963	8.997	24578152	32406567	30.153	28.538
Target Compounds							
9)	A Endosulfan I	5.298	0.000	5115967	0	6.105	N.D. #
10)	B trans-Chl...	0.000	6.044	0	8614102	N.D.	6.039
11)	B cis-Chlor...	5.298f	0.000	5115967	0	5.778	N.D. #
15)	B Endosulfa...	0.000	6.874	0	2644296	N.D.	2.042
19)	B Endosulfa...	0.000	7.198	0	1327322	N.D.	1.101


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111319\
Data File : PD055936.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Nov 2019 15:33
Operator : SG\AJ
Sample : K5774-02
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
C0AQ8

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 00:44:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 02 07:20:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

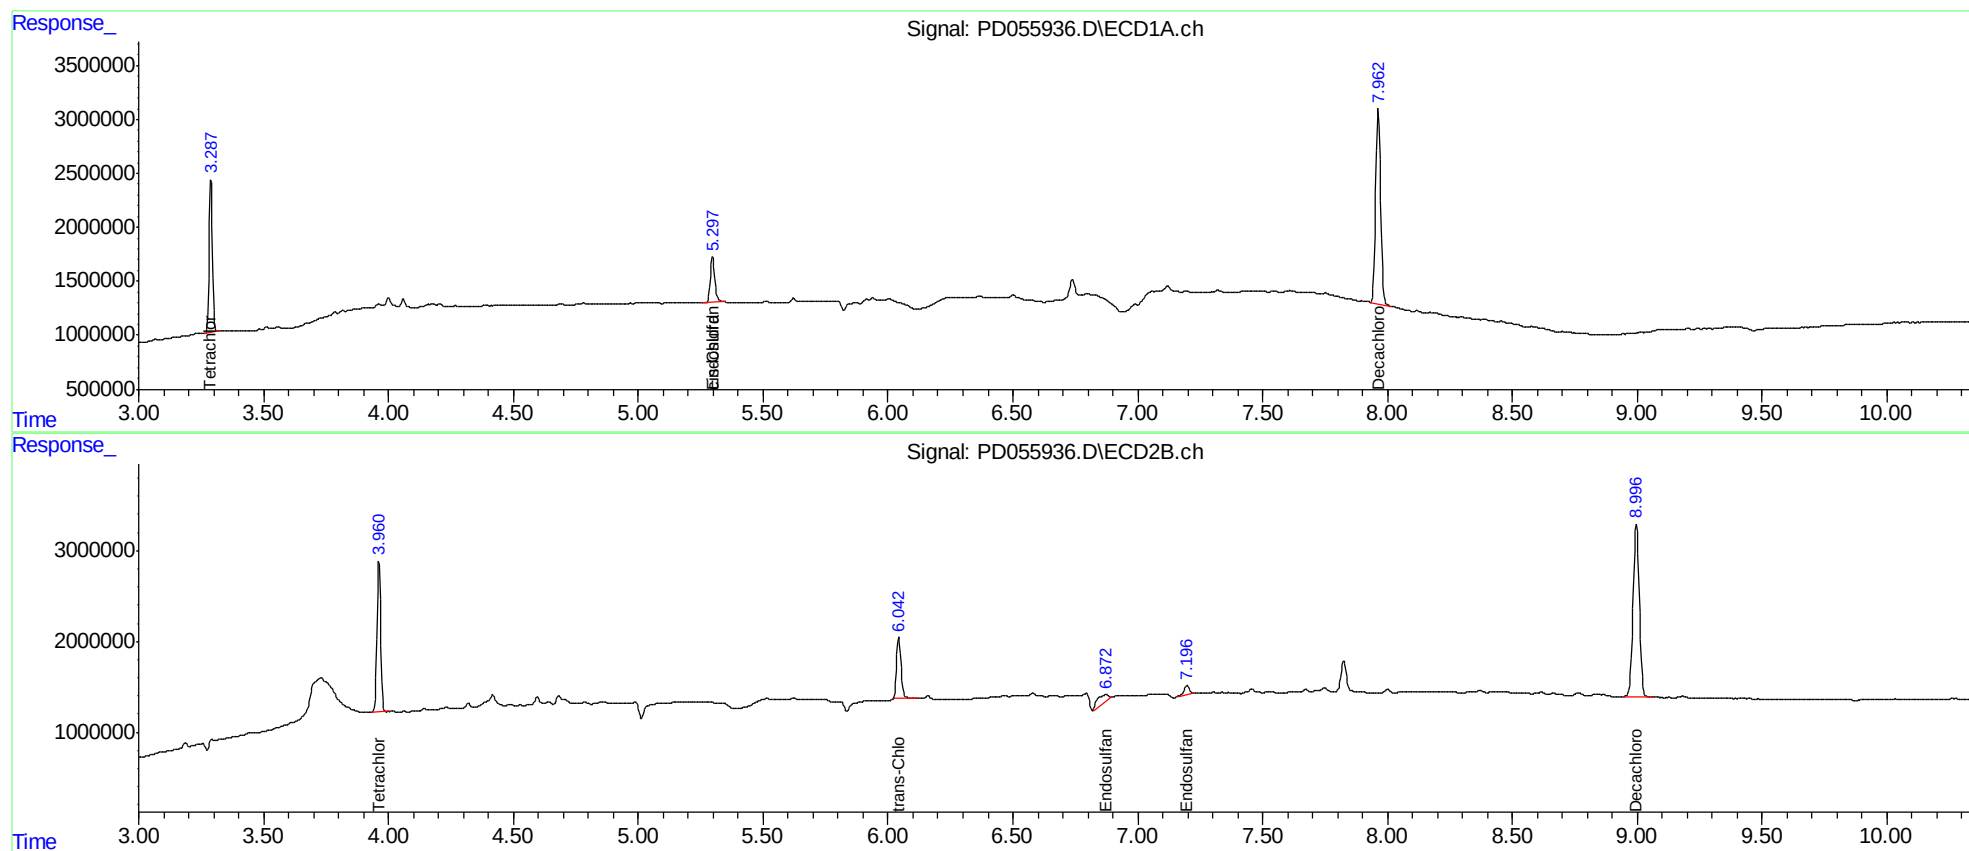


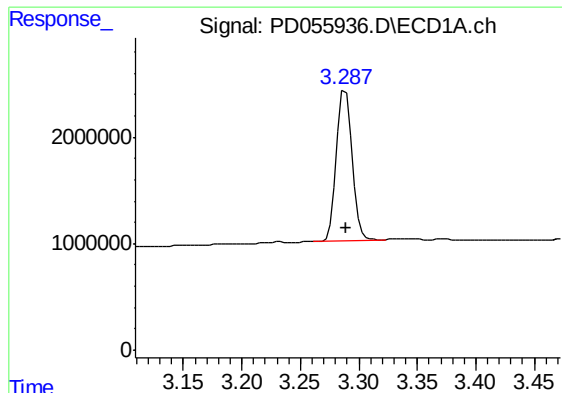

#1 Tetrachloro-m-xylene


R.T.: 3.289 min
Delta R.T.: 0.000 min
Response: 12717657
Conc: 16.89 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AQ8

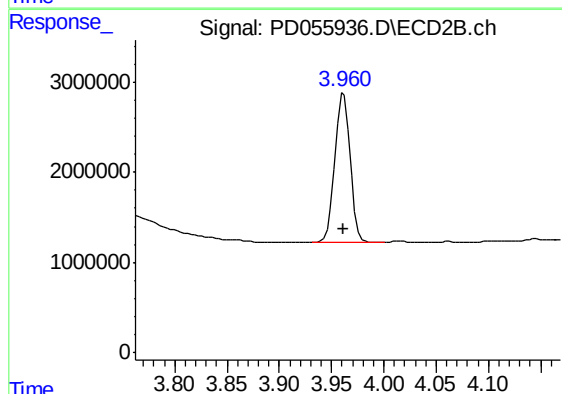


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: 0.000 min
Response: 16981719
Conc: 16.20 ng/ml

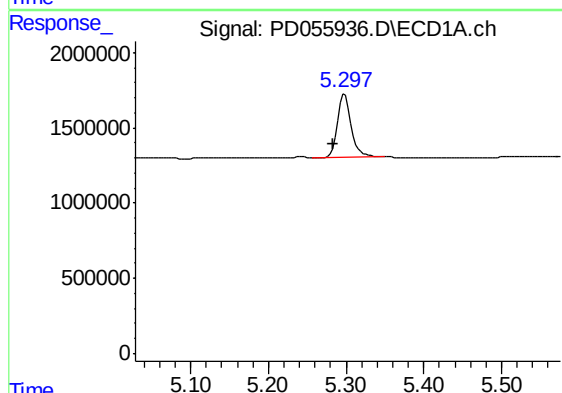


#9 Endosulfan I

R.T.: 5.298 min
Delta R.T.: 0.015 min
Response: 5115967
Conc: 6.10 ng/ml

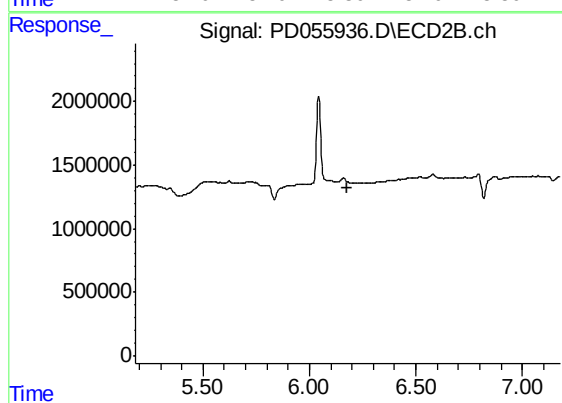

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.180 min
Response: 0
Conc: N.D.

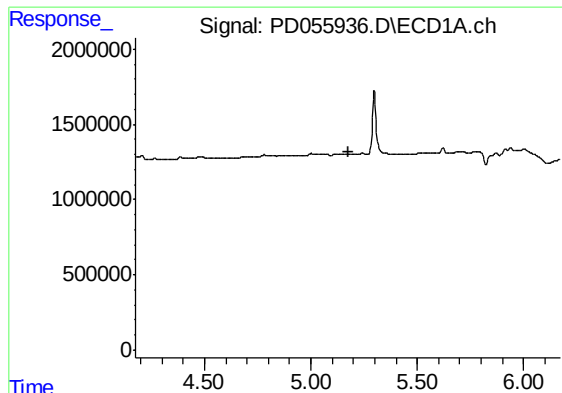

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.174 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C0AQ8

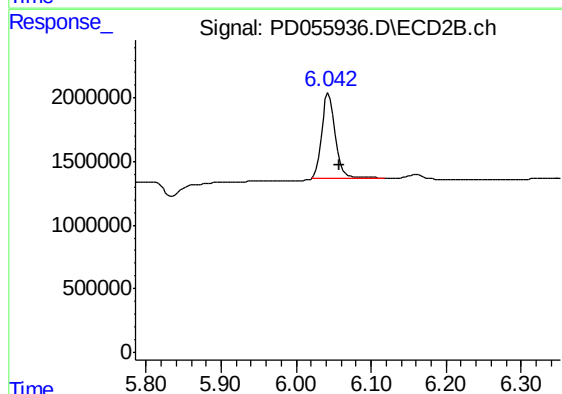


#10 trans-Chlordane

R.T.: 6.044 min
Delta R.T.: -0.014 min
Response: 8614102
Conc: 6.04 ng/ml

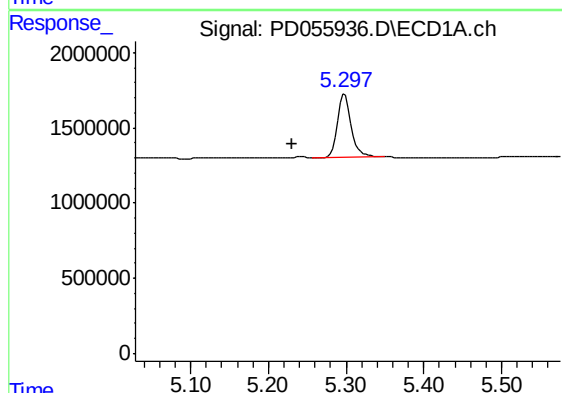


#11 cis-Chlordane

R.T.: 5.298 min
Delta R.T.: 0.067 min
Response: 5115967
Conc: 5.78 ng/ml

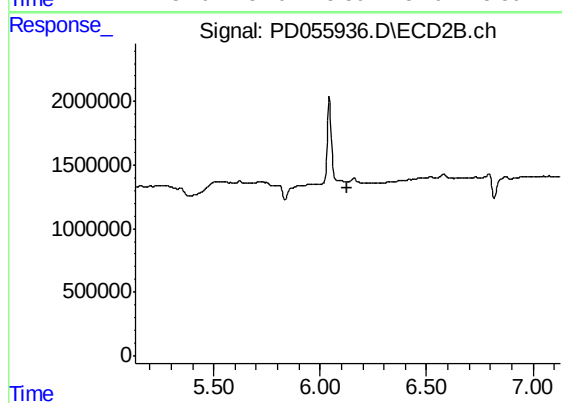

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.130 min
Response: 0
Conc: N.D.

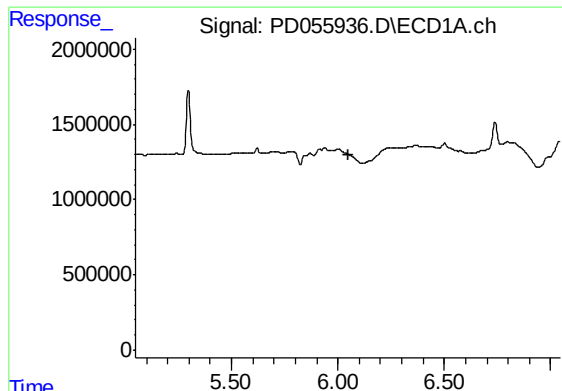

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.049 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C0AQ8

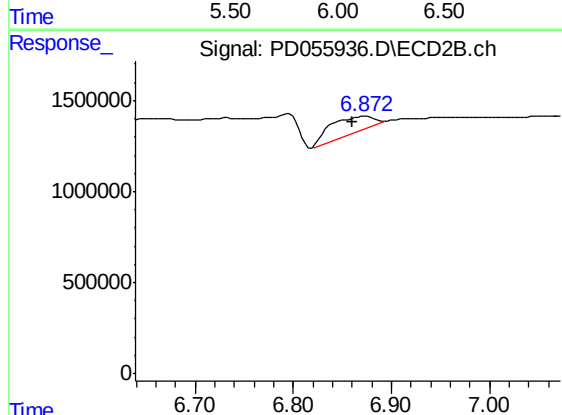


#15 Endosulfan II

R.T.: 6.874 min
Delta R.T.: 0.014 min
Response: 2644296
Conc: 2.04 ng/ml

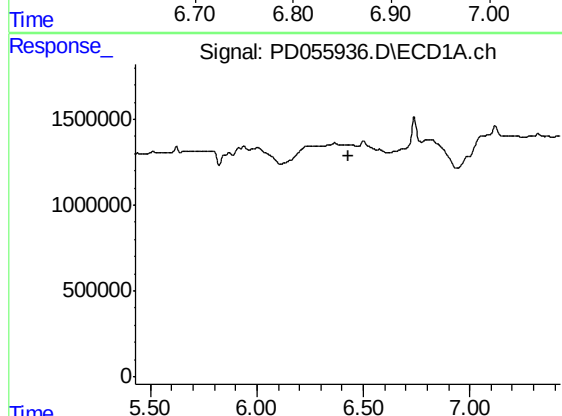


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 6.428 min
Response: 0
Conc: N.D.

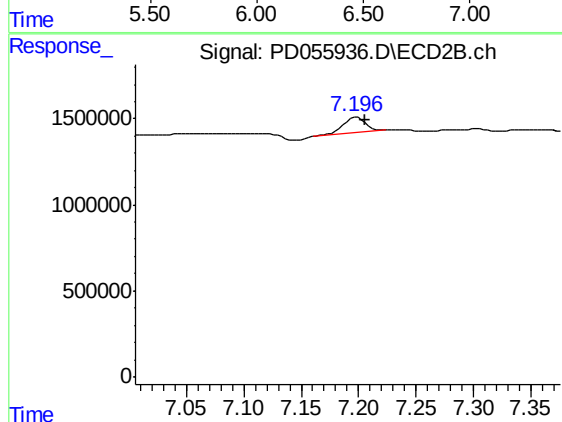

#19 Endosulfan Sulfate


R.T.: 7.198 min
Delta R.T.: -0.008 min
Response: 1327322
Conc: 1.10 ng/ml

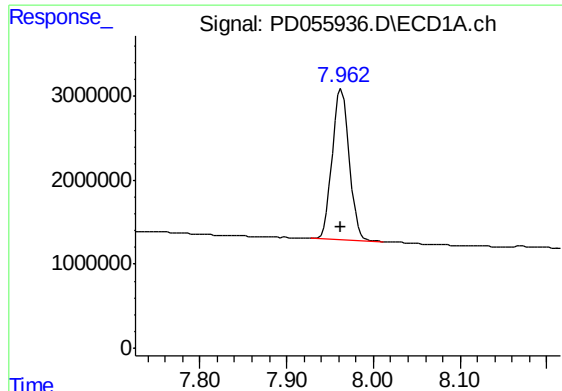

#27 Decachlorobiphenyl

R.T.: 7.963 min
Delta R.T.: 0.000 min
Response: 24578152
Conc: 30.15 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AQ8

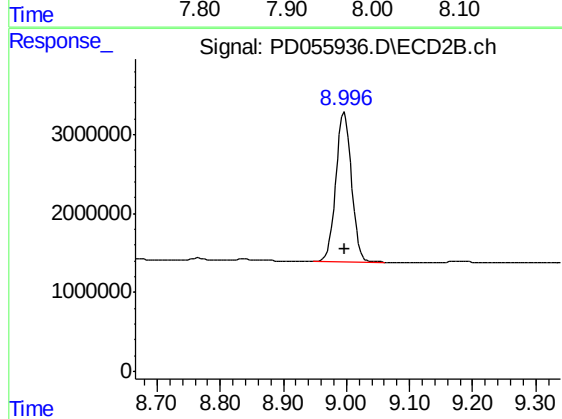

#27 Decachlorobiphenyl

R.T.: 8.997 min
Delta R.T.: 0.000 min
Response: 32406567
Conc: 28.54 ng/ml