

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111319\
 Data File : PD055951.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Nov 2019 19:30
 Operator : SG\AJ
 Sample : K5774-03
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AQ9

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 00:48:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 02 07:20:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.289	3.962	8564422	11141852	11.377	10.632
27) SA Decachlor...	7.962	8.996	11786979	13914338	14.460	12.253
Target Compounds						
10) B trans-Chl...	0.000	6.045	0	1360147	N.D.	0.954
15) B Endosulfa...	0.000	6.876	0	3346054	N.D.	2.584


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111319\
Data File : PD055951.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Nov 2019 19:30
Operator : SG\AJ
Sample : K5774-03
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
C0AQ9

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 00:48:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 02 07:20:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

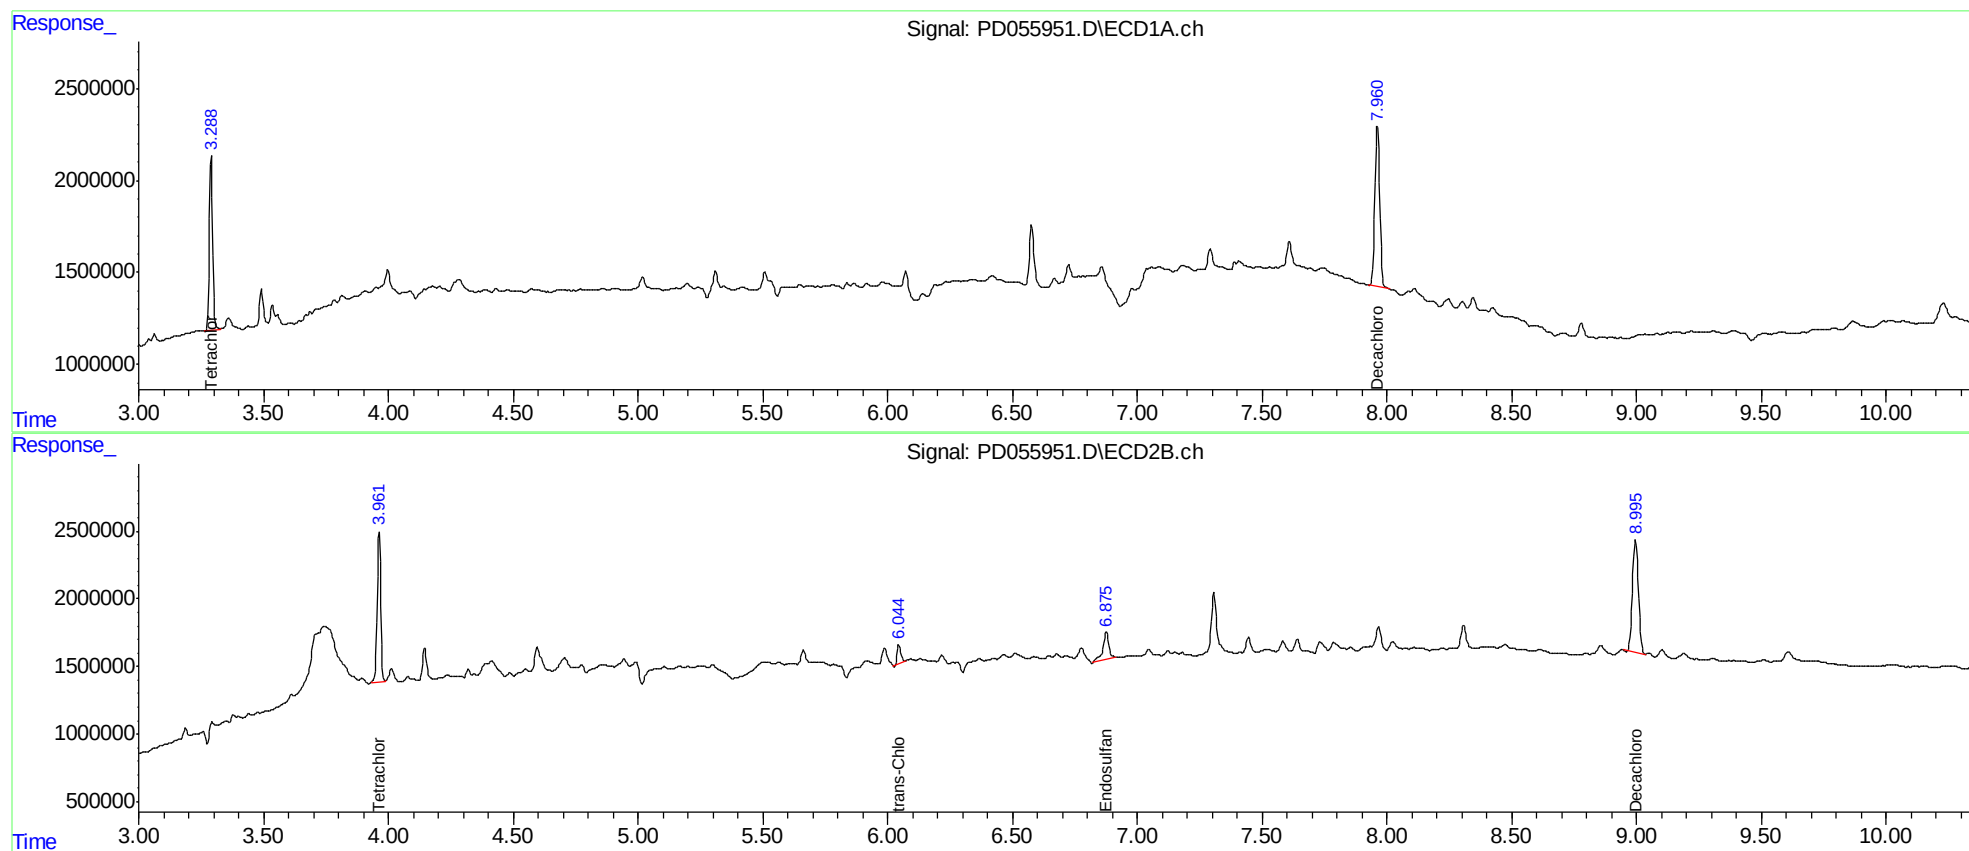


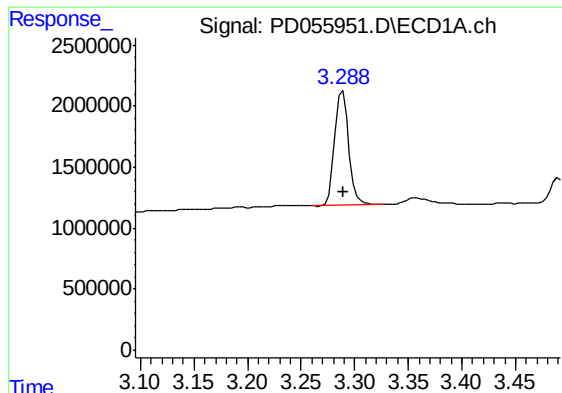

#1 Tetrachloro-m-xylene


R.T.: 3.289 min
Delta R.T.: 0.000 min
Response: 8564422
Conc: 11.38 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AQ9

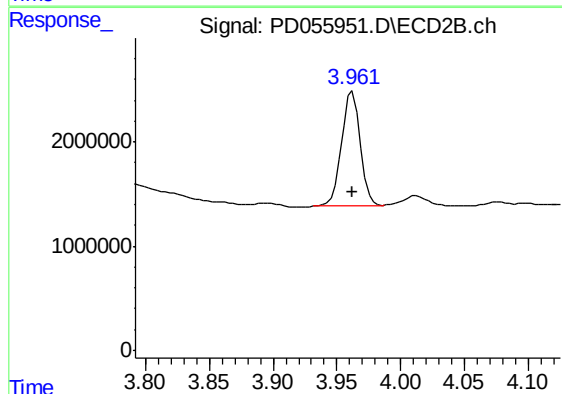


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: 0.000 min
Response: 11141852
Conc: 10.63 ng/ml

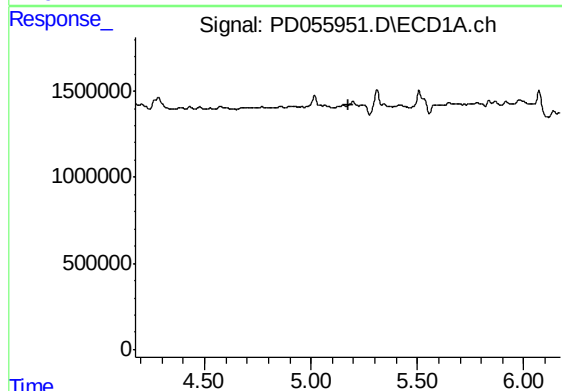


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.174 min
Response: 0
Conc: N.D.

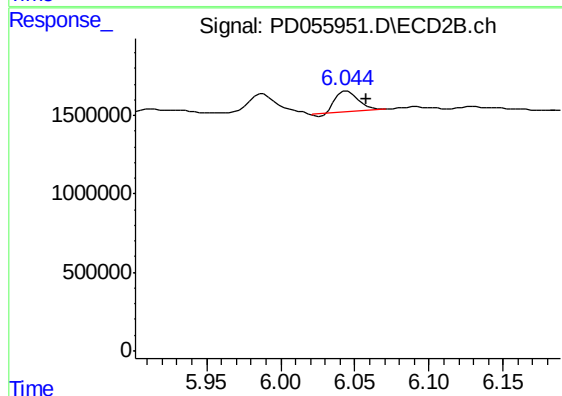

#10 trans-Chlordane


R.T.: 6.045 min
Delta R.T.: -0.013 min
Response: 1360147
Conc: 0.95 ng/ml

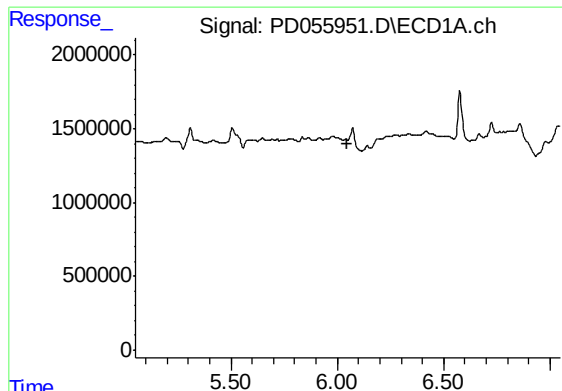

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.049 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C0AQ9

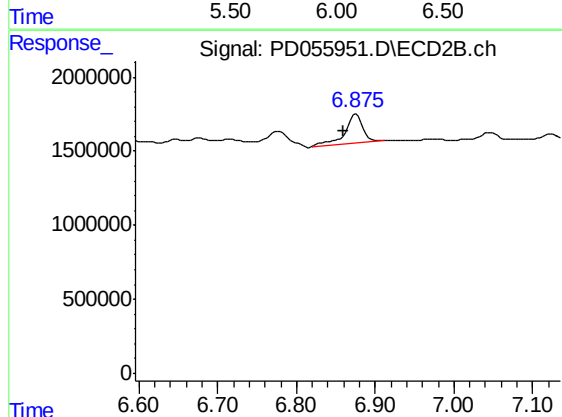


#15 Endosulfan II

R.T.: 6.876 min
Delta R.T.: 0.016 min
Response: 3346054
Conc: 2.58 ng/ml

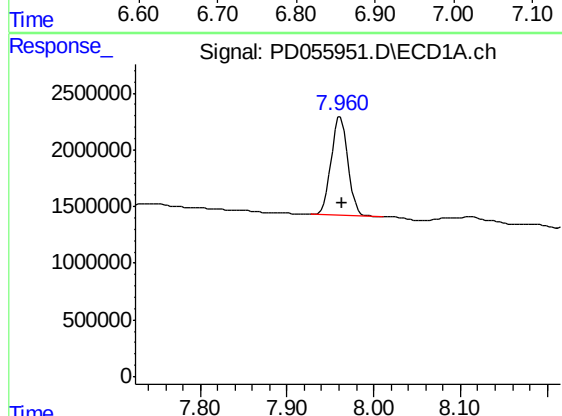

#27 Decachlorobiphenyl

R.T.: 7.962 min
Delta R.T.: -0.002 min
Response: 11786979
Conc: 14.46 ng/ml

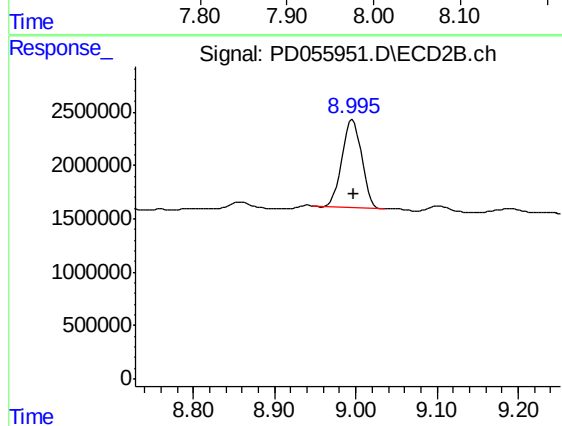

#27 Decachlorobiphenyl

R.T.: 8.996 min
Delta R.T.: 0.000 min
Response: 13914338
Conc: 12.25 ng/ml