

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111319\
Data File : PD055933.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Nov 2019 14:46
Operator : SG\AJ
Sample : INDA343
Misc :
ALS Vial : 24 Sample Multiplier: 1


Instrument :
ECD_D
LabSampleId :
INDA343

Manual Integrations
APPROVED

Ankita
11/15/2019 8:48:32 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 03:19:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 02 07:20:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

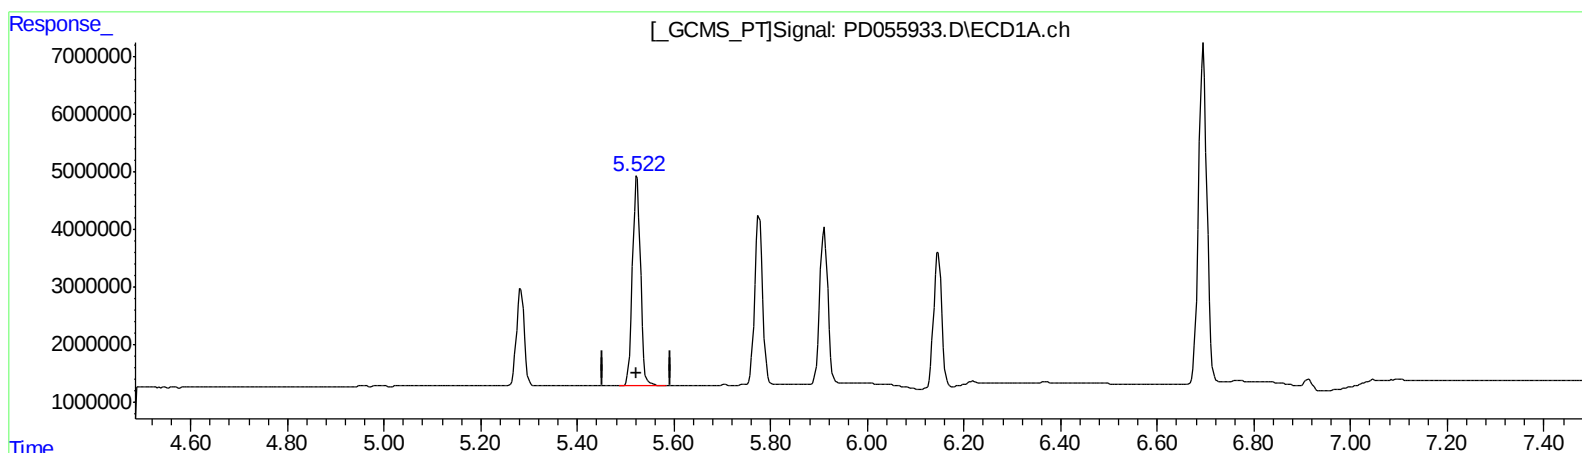

(13) Dieldrin (MA)
5.523min 44.775 ng/ml
response 42115204

(13) Dieldrin #2 (MA)
6.436min 43.176 ng/ml
response 61032420

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111319\
Data File : PD055933.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Nov 2019 14:46
Operator : SG\AJ
Sample : INDA343
Misc :
ALS Vial : 24 Sample Multiplier: 1


Instrument :
ECD_D
LabSampleId :
INDA343

Manual Integrations
APPROVED

Ankita
11/15/2019 8:48:32 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 03:19:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 02 07:20:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

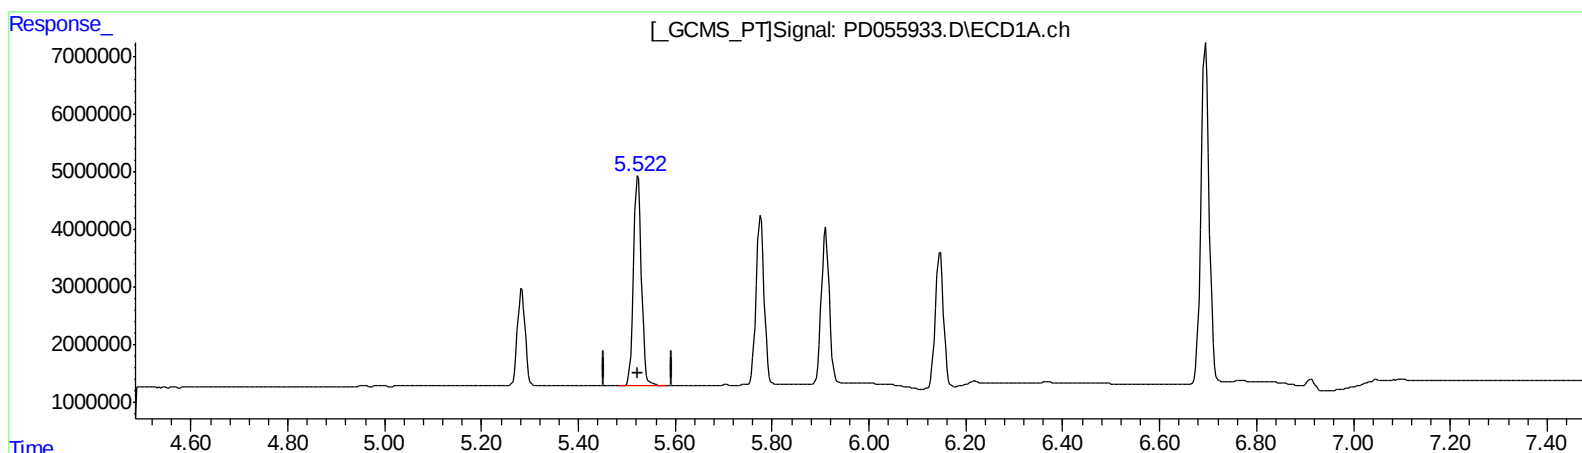

(13) Dieldrin (MA)
5.523min 44.775 ng/ml
response 42115204

(13) Dieldrin #2 (MA)
6.435min 43.821 ng/ml m
response 61944920

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111319\
 Data File : PD055933.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Nov 2019 14:46
 Operator : SG\AJ
 Sample : INDA343
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 LabSampleId :
 INDA343

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 03:19:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 02 07:20:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Manual Integrations
 APPROVED

Ankita
 11/15/2019 8:48:32 AM

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.289	3.962	16861304	22347161	22.399	21.325
27) SA Decachlor...	7.963	8.997	36138359	46675675	44.335	41.104
Target Compounds						
2) A alpha-BHC	3.715	4.349	23788175	30814889	22.593	21.625
3) MA gamma-BHC...	3.990	4.631	22356818	30048732	21.857	21.328
4) MA Heptachlor	4.276	5.137	19721086	31286023	20.829	21.512
9) A Endosulfan I	5.283	6.180	18966969	28207042	22.633	21.664
13) MA Dieldrin	5.523	6.435	42115204	61944920	44.775	43.821m
14) MA Endrin	5.776	6.653	33612468	48488729	41.899	42.117
16) A 4,4'-DDD	5.911	6.775	30878940	48950890	43.721	43.837
17) MA 4,4'-DDT	6.147	7.072	27575252	45871809	42.553	42.186
20) A Methoxychlor	6.695	7.529	70072928	128.5E6	187.333	206.155

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

3 AJ
 11/16/19