

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111323\
 Data File : PD079616.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Nov 2023 18:11
 Operator : AR\AJ
 Sample : 05311-16
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TP-6

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/10/2023
 Supervised By :Ankita Jodhani 11/10/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 20:12:28 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102023.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 20 04:44:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.569	2.804	26037743	42374672	16.127	18.302
2) SA Decachlor...	9.116	7.948	24003803	33664136	11.966	13.811
Target Compounds						
11) B alpha-Chl...	6.061	5.073	54668155	50488177	23.975	17.593m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111323\
Data File : PD079616.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Nov 2023 18:11
Operator : AR\AJ
Sample : 05311-16
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
TP-6


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 11/10/2023
Supervised By : Ankita Jodhani 11/10/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 20:12:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102023.M
Quant Title : GC Extractables
QLast Update : Fri Oct 20 04:44:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

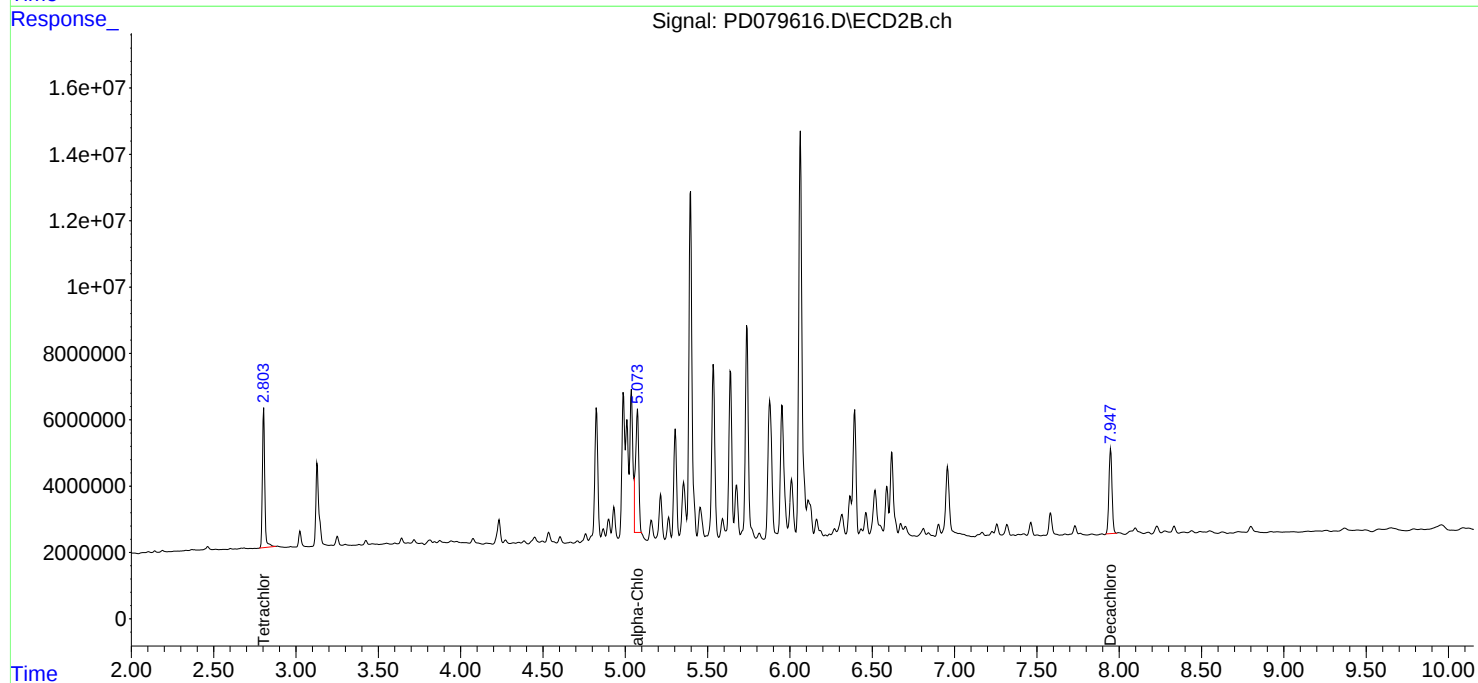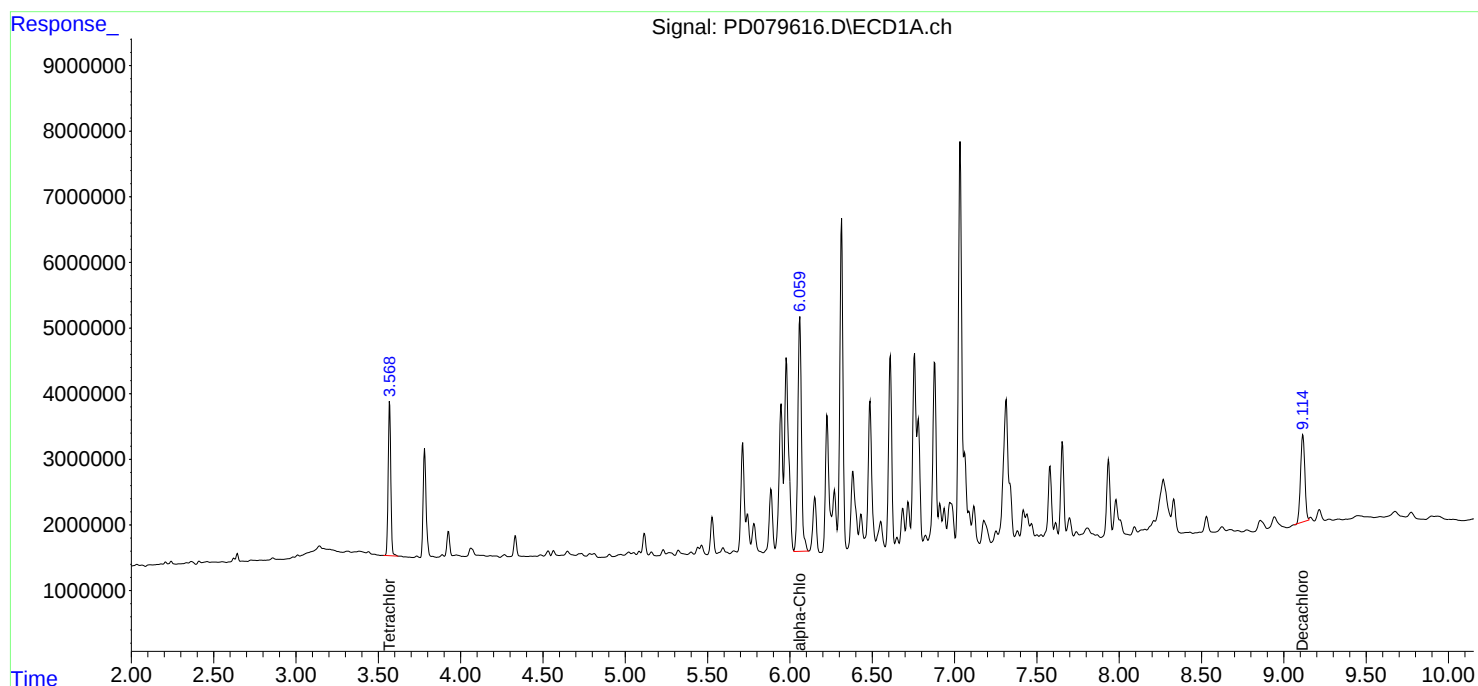

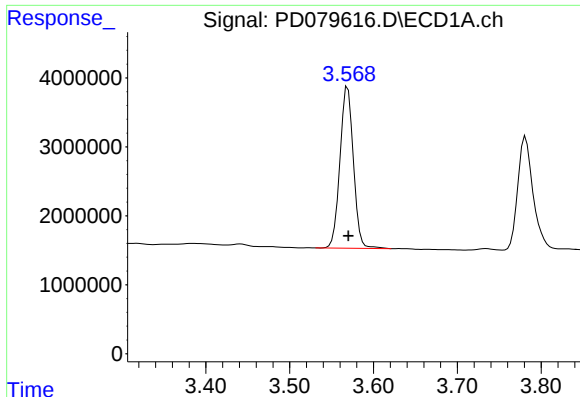


#1 Tetrachloro-m-xylene

R.T.: 3.569 min
Delta R.T.: 0.000 min
Response: 26037743
Conc: 16.13 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-6


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/10/2023
Supervised By :Ankita Jodhani 11/10/2023

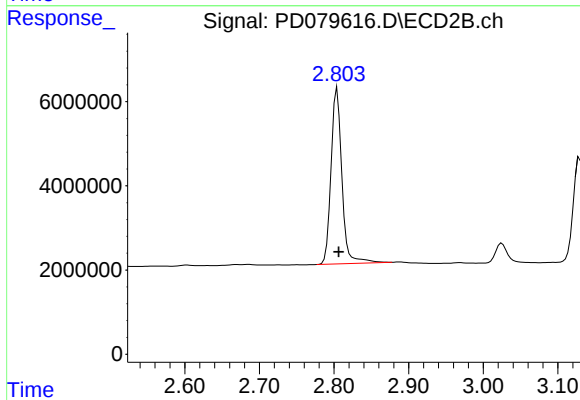


#1 Tetrachloro-m-xylene

R.T.: 2.804 min
Delta R.T.: -0.002 min
Response: 42374672
Conc: 18.30 ng/ml

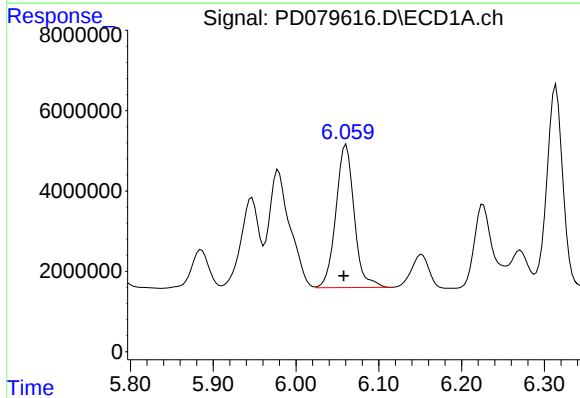


#11 alpha-Chlordane

R.T.: 6.061 min
Delta R.T.: 0.003 min
Response: 54668155
Conc: 23.98 ng/ml

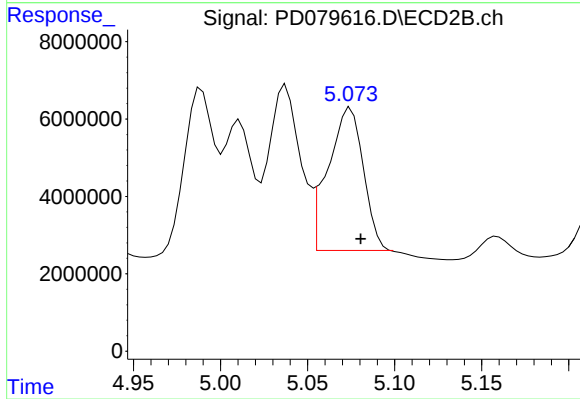

#11 alpha-Chlordane

R.T.: 5.073 min
Delta R.T.: -0.007 min
Response: 50488177
Conc: 17.59 ng/ml m

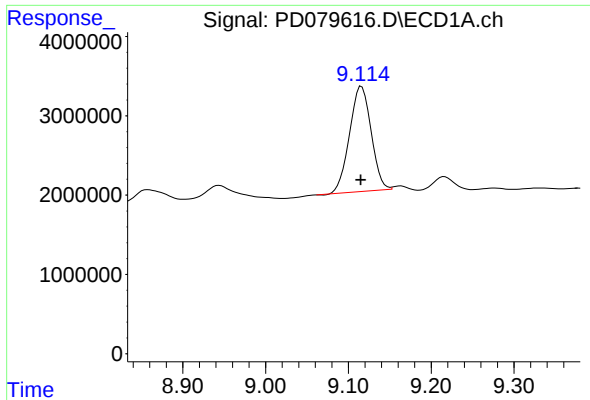


#28 Decachlorobiphenyl

R.T.: 9.116 min
Delta R.T.: 0.001 min
Response: 24003803
Conc: 11.97 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-6

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/10/2023
Supervised By :Ankita Jodhani 11/10/2023

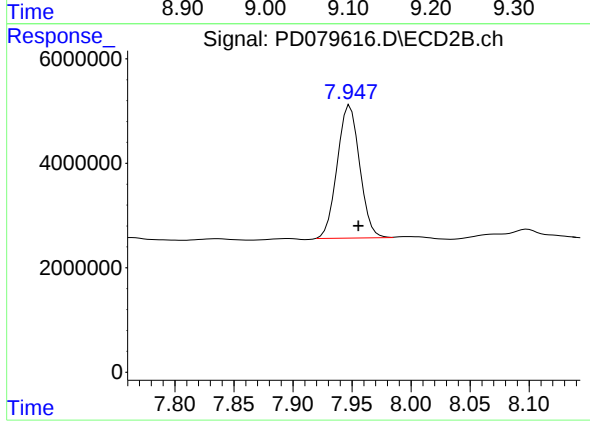

#28 Decachlorobiphenyl

R.T.: 7.948 min
Delta R.T.: -0.007 min
Response: 33664136
Conc: 13.81 ng/ml