

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD111323\  
 Data File : PD079623.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 09 Nov 2023 19:58  
 Operator : AR\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_D  
 ClientSampleId :  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Nov 10 03:18:07 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD102023.M  
 Quant Title : GC Extractables  
 QLast Update : Fri Oct 20 04:44:01 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound        | RT#1  | RT#2  | Resp#1   | Resp#2   | ng/ml  | ng/ml  |
|-----------------------------|-----------------|-------|-------|----------|----------|--------|--------|
| -----                       |                 |       |       |          |          |        |        |
| System Monitoring Compounds |                 |       |       |          |          |        |        |
| 1)                          | SA Tetrachlo... | 3.569 | 2.804 | 34807619 | 57081564 | 21.558 | 24.654 |
| 28)                         | SA Decachlor... | 9.116 | 7.949 | 40759687 | 48208846 | 20.319 | 19.778 |

Target Compounds

-----



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD111323\  
Data File : PD079623.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 09 Nov 2023 19:58  
Operator : AR\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
I.BLK

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Nov 10 03:18:07 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD102023.M  
Quant Title : GC Extractables  
QLast Update : Fri Oct 20 04:44:01 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

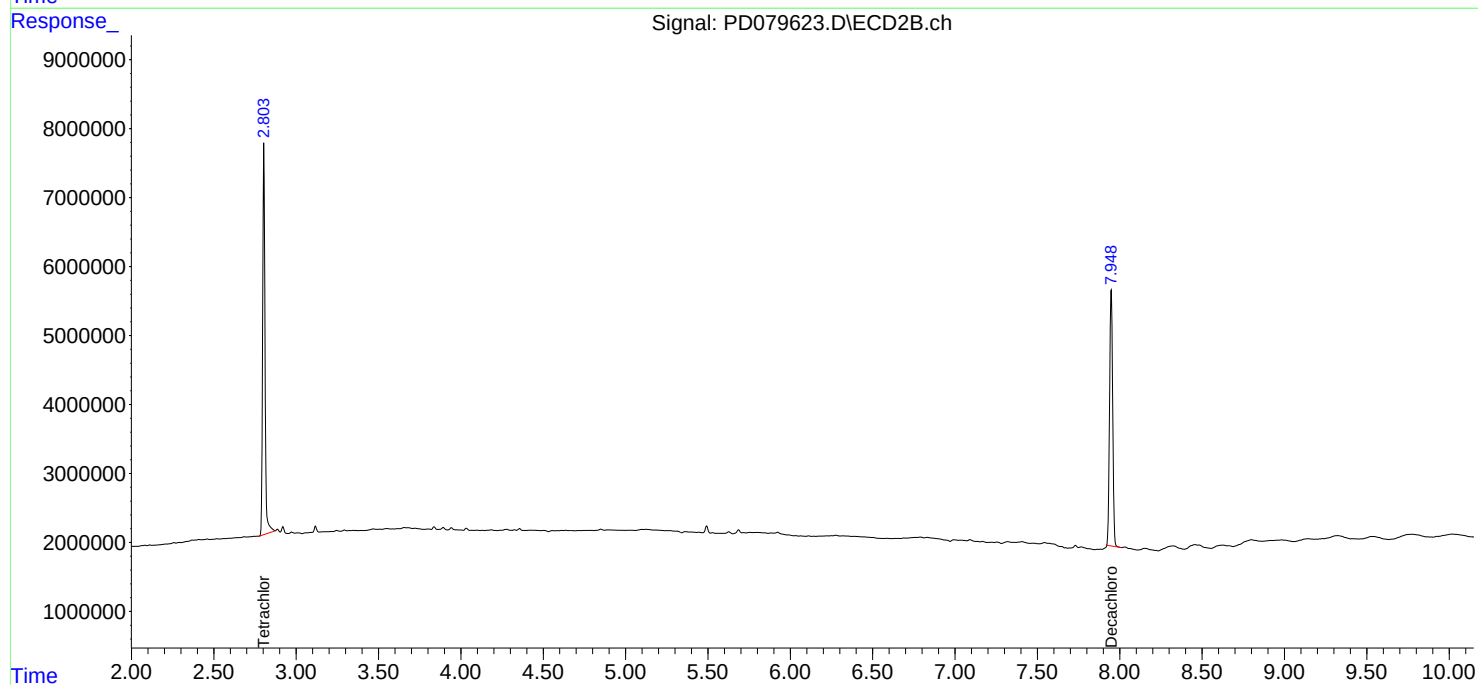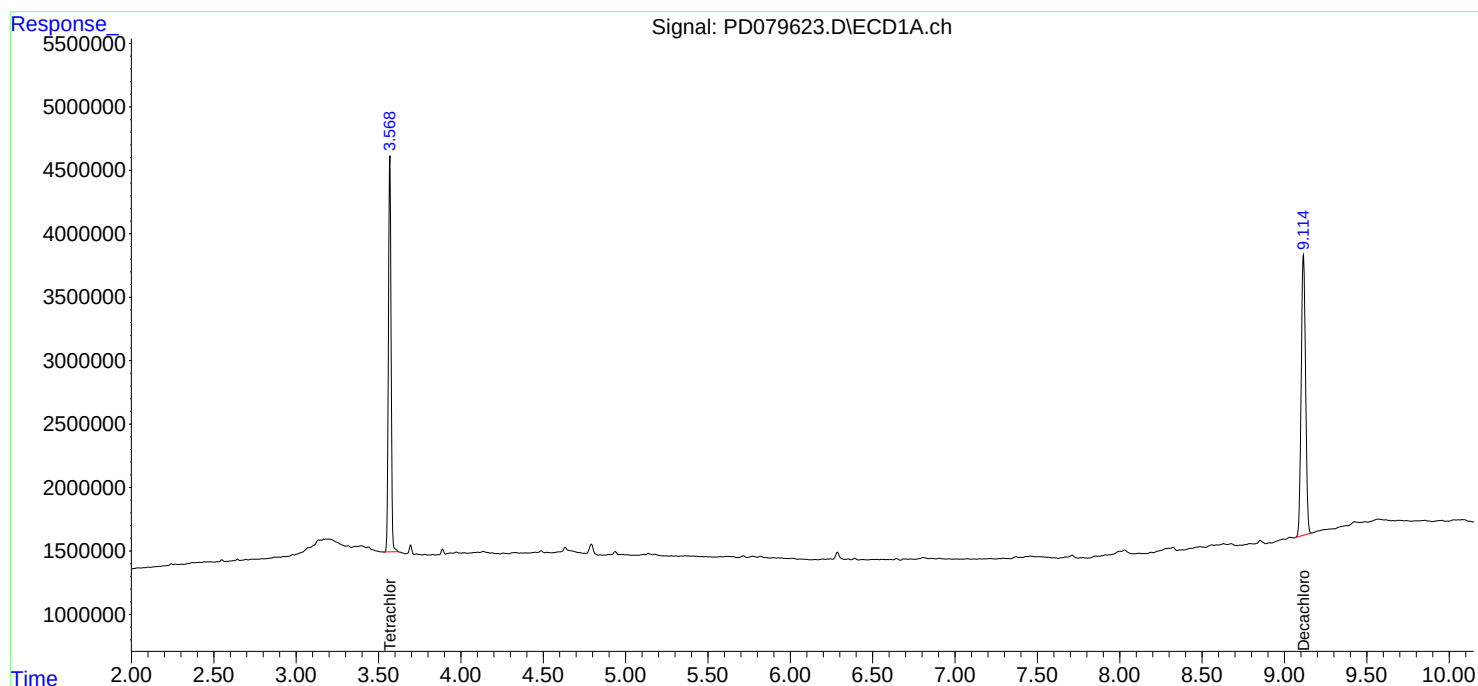


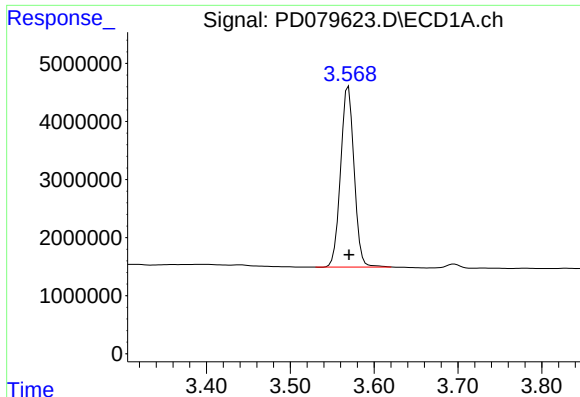

#1 Tetrachloro-m-xylene


R.T.: 3.569 min  
Delta R.T.: 0.000 min  
Response: 34807619  
Conc: 21.56 ng/ml

Instrument :  
ECD\_D  
ClientSampleId :  
I.BLK

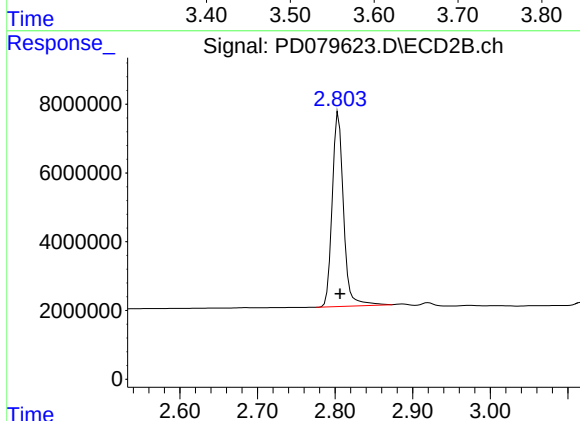


#1 Tetrachloro-m-xylene

R.T.: 2.804 min  
Delta R.T.: -0.002 min  
Response: 57081564  
Conc: 24.65 ng/ml

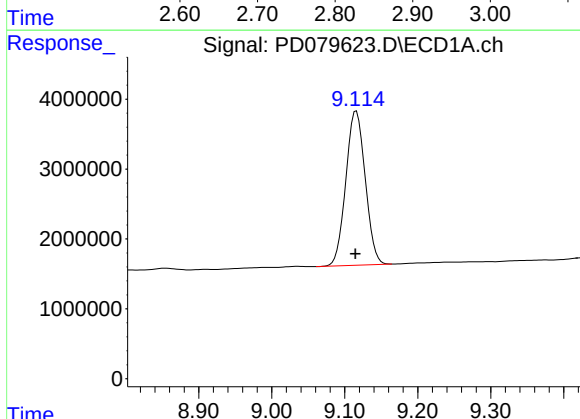

#28 Decachlorobiphenyl

R.T.: 9.116 min  
Delta R.T.: 0.001 min  
Response: 40759687  
Conc: 20.32 ng/ml

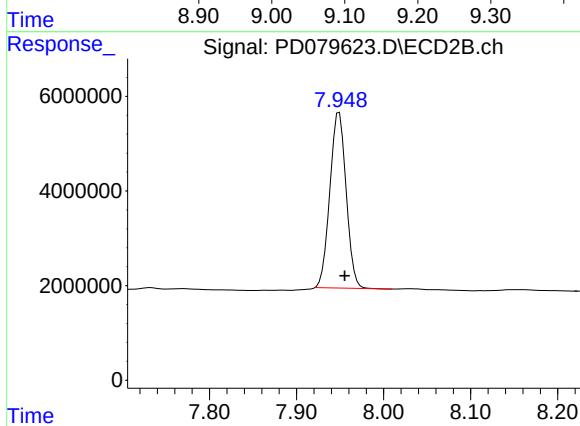

#28 Decachlorobiphenyl

R.T.: 7.949 min  
Delta R.T.: -0.006 min  
Response: 48208846  
Conc: 19.78 ng/ml